

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121523\
 Data File : VN080497.D
 Acq On : 15 Dec 2023 10:50
 Operator : JC\MD
 Sample : VN1215WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1215WBL01

Quant Time: Dec 16 02:49:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 13 01:57:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	222596	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	412513	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	423919	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	187510	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	162016	56.987	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 113.980%	
35) Dibromofluoromethane	8.165	113	133651	51.100	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.200%	
50) Toluene-d8	10.565	98	470648	48.250	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 96.500%	
62) 4-Bromofluorobenzene	12.847	95	187680	50.669	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 101.340%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121523\
Data File : VN080497.D
Acq On : 15 Dec 2023 10:50
Operator : JC\MD
Sample : VN1215WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1215WBL01

Quant Time: Dec 16 02:49:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 13 01:57:14 2023
Response via : Initial Calibration




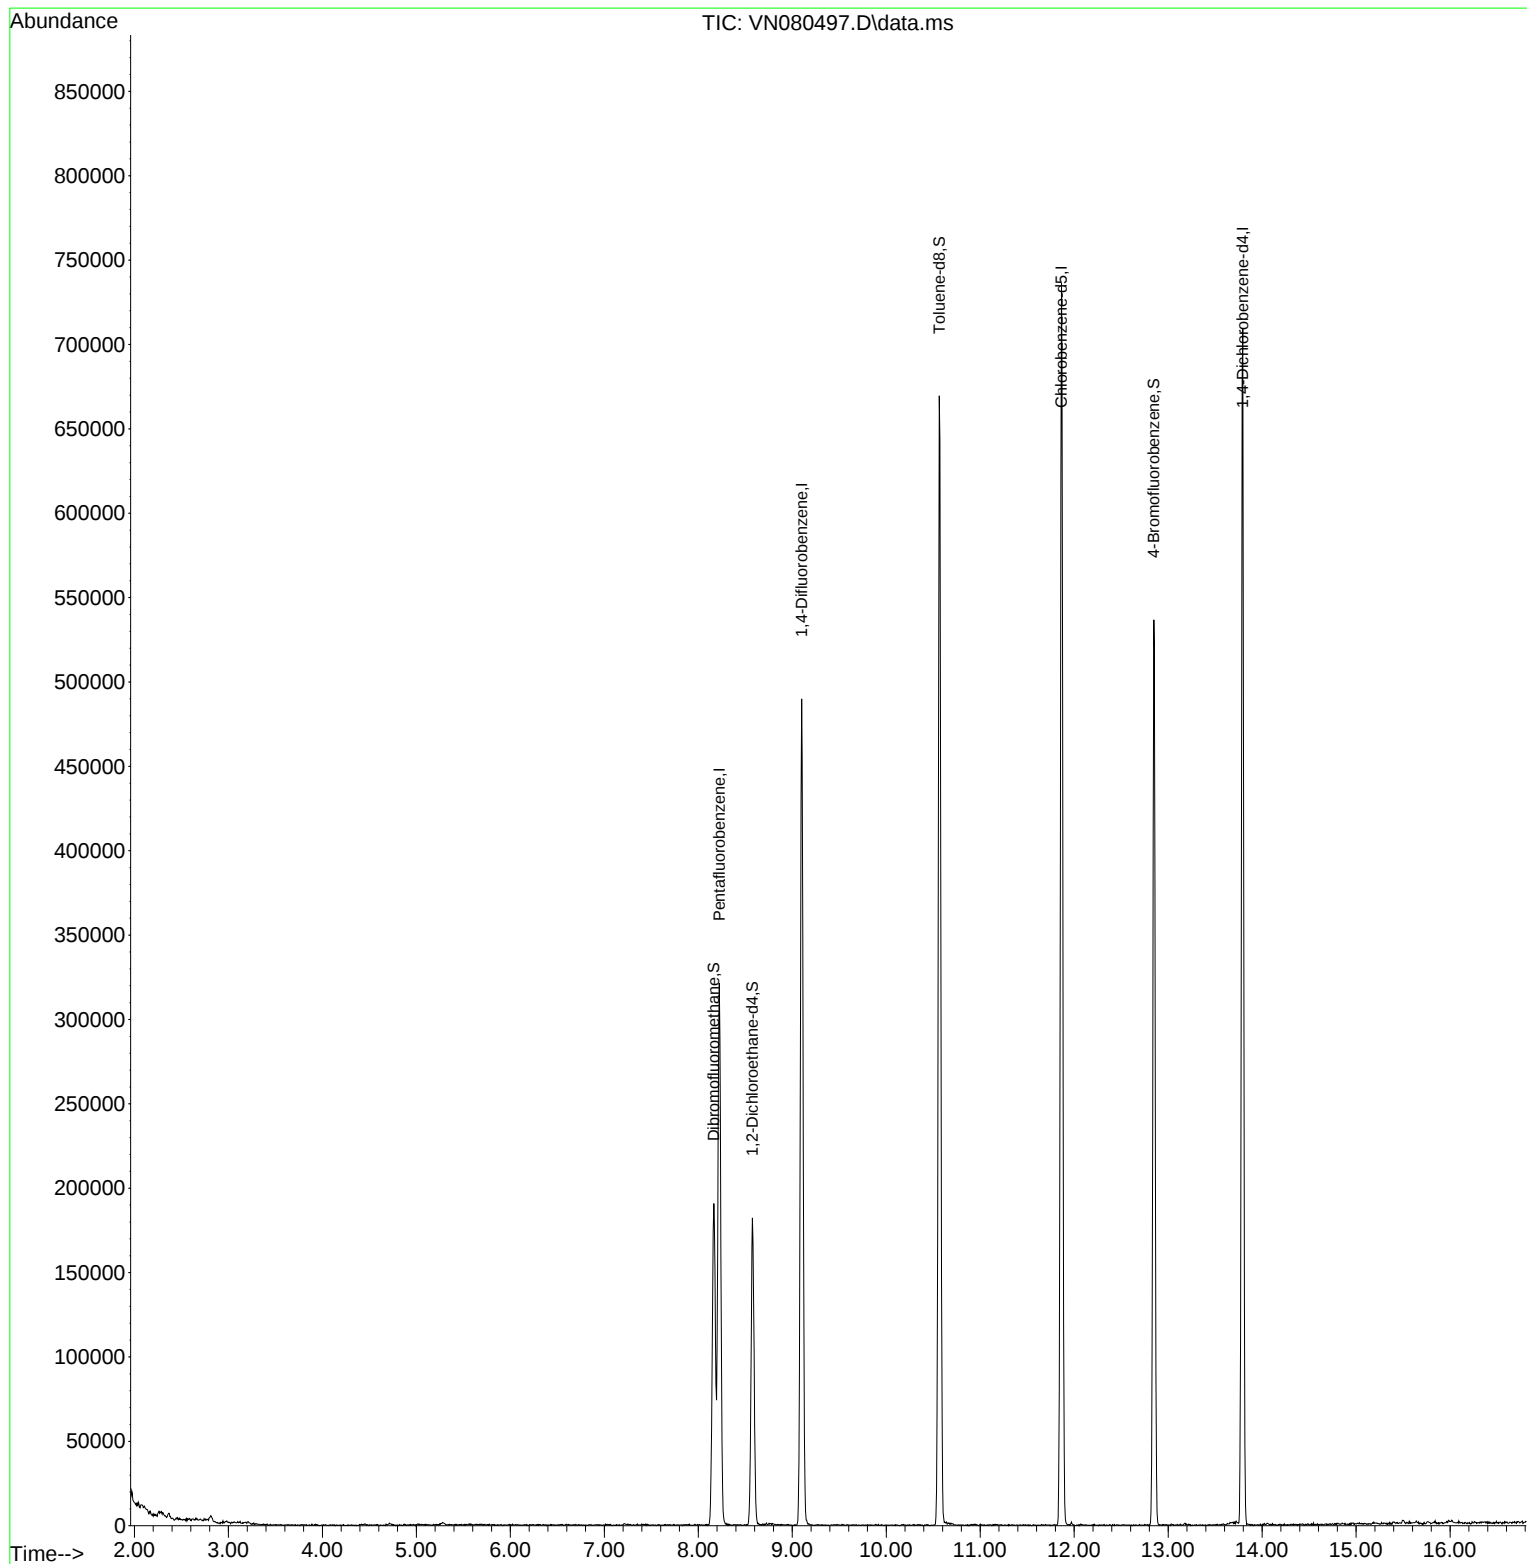


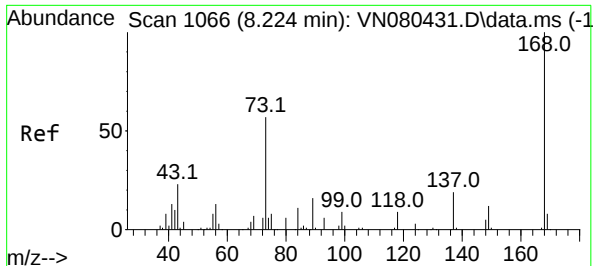

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50




Instrument :
MSVOA_N
ClientSampleId :
VN1215WBL01


Tgt Ion:168 Resp: 222596
Ion Ratio Lower Upper
168 100
99 70.6 53.0 79.6

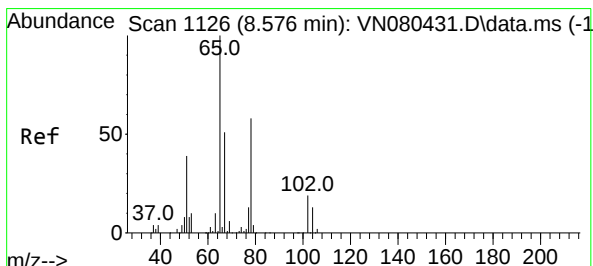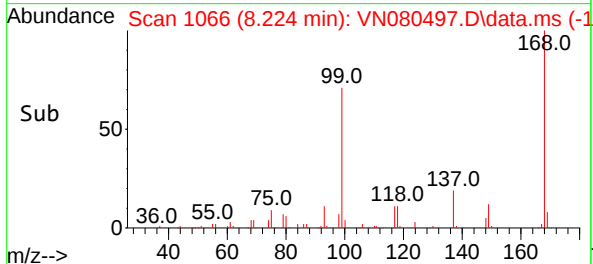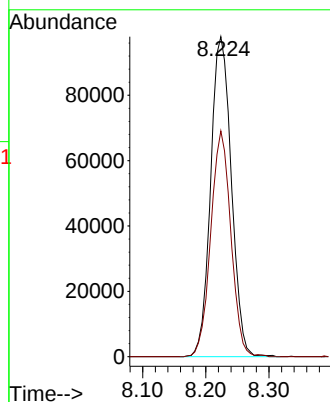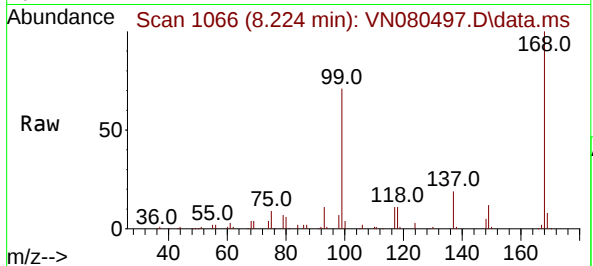

#33
1,2-Dichloroethane-d4
Concen: 56.987 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50

Tgt Ion: 65 Resp: 162016
Ion Ratio Lower Upper
65 100
67 47.9 0.0 106.6


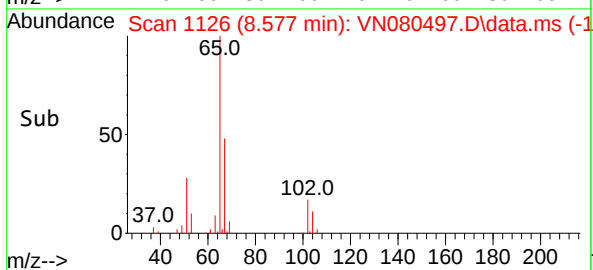
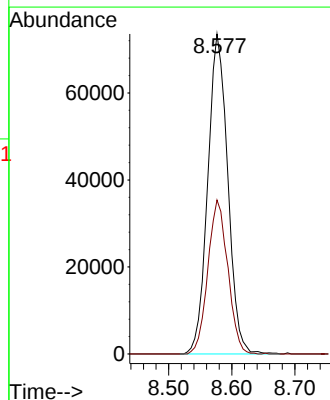
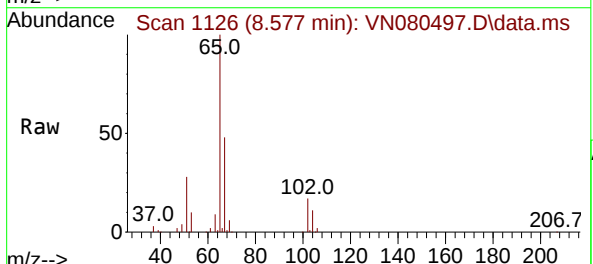


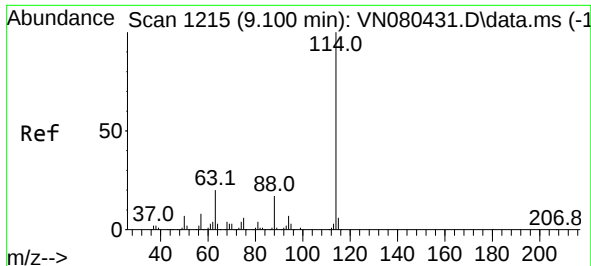

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50




Instrument :
MSVOA_N
ClientSampleId :
VN1215WBL01


Tgt Ion:114 Resp: 412513
Ion Ratio Lower Upper
114 100
63 20.6 0.0 36.4
88 18.2 0.0 30.6

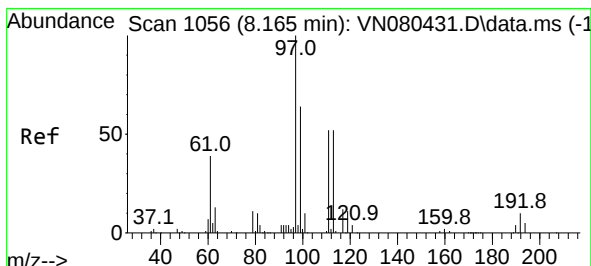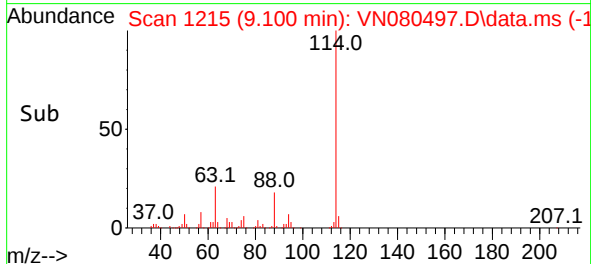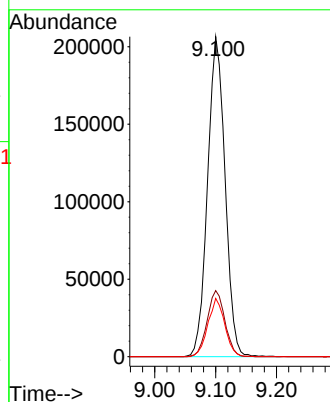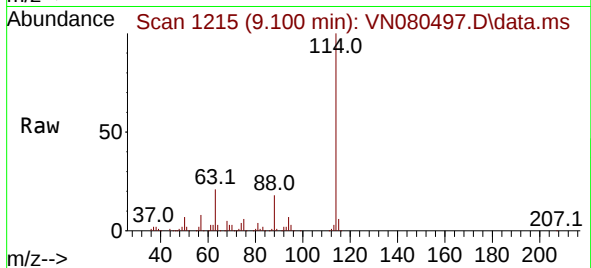

#35
Dibromofluoromethane
Concen: 51.100 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50

Tgt Ion:113 Resp: 133651
Ion Ratio Lower Upper
113 100
111 103.3 82.6 123.8
192 19.1 12.7 19.1


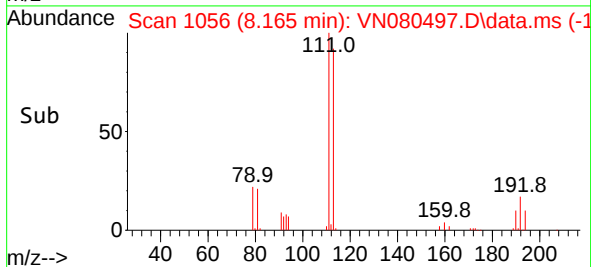
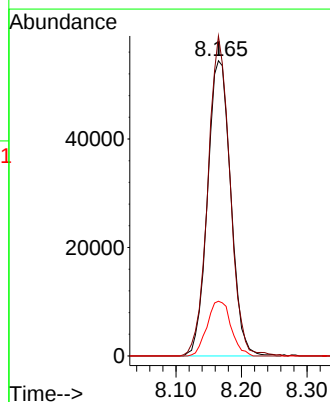
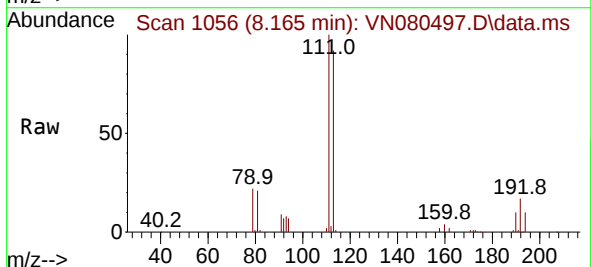


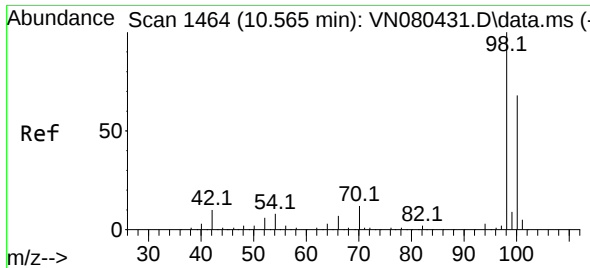

#50
Toluene-d8
Concen: 48.250 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50




Instrument :
MSVOA_N
ClientSampleId :
VN1215WBL01


Tgt Ion: 98 Resp: 470648
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

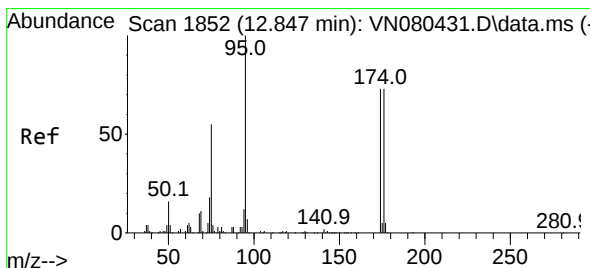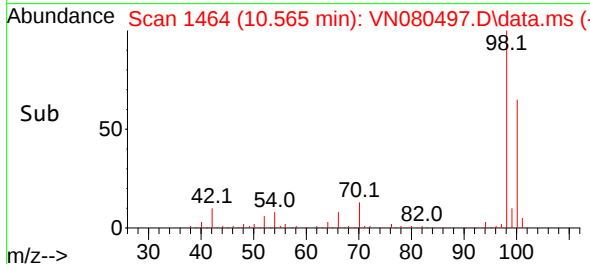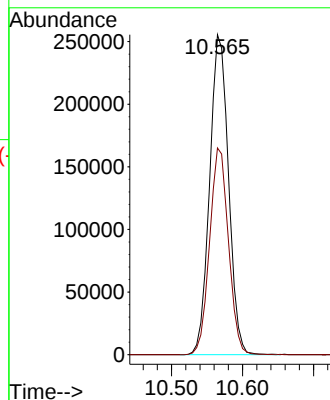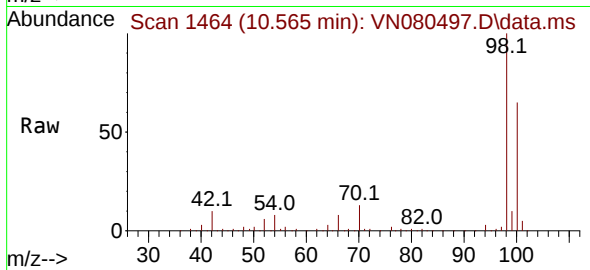

#62
4-Bromofluorobenzene
Concen: 50.669 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50

Tgt Ion: 95 Resp: 187680
Ion Ratio Lower Upper
95 100
174 75.4 0.0 143.8
176 73.5 0.0 135.8


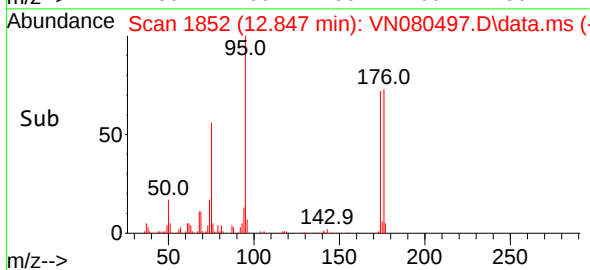
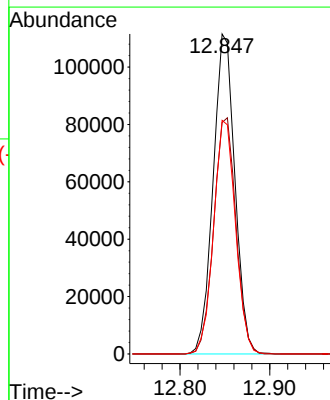
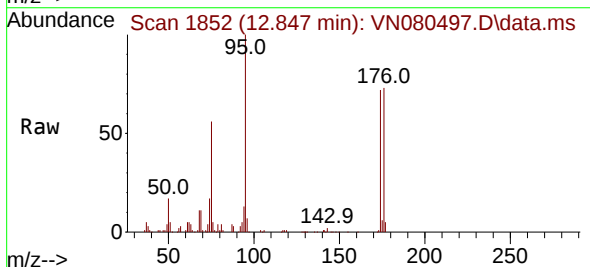


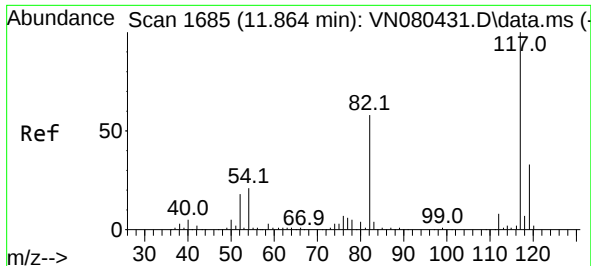

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50

Instrument :
MSVOA_N
ClientSampleId :
VN1215WBL01

Tgt Ion:117 Resp: 423919
Ion Ratio Lower Upper
117 100
82 59.9 44.0 66.0
119 31.6 25.6 38.4

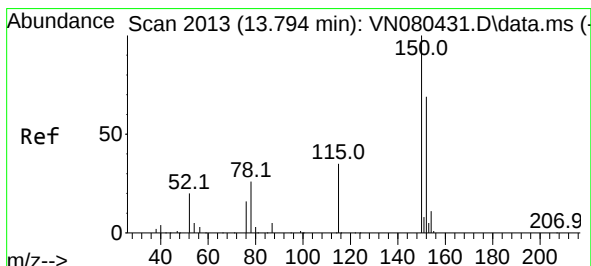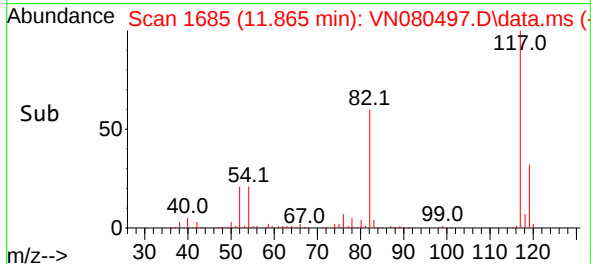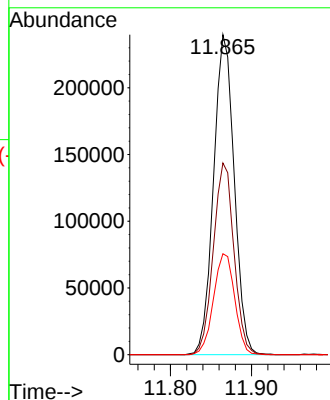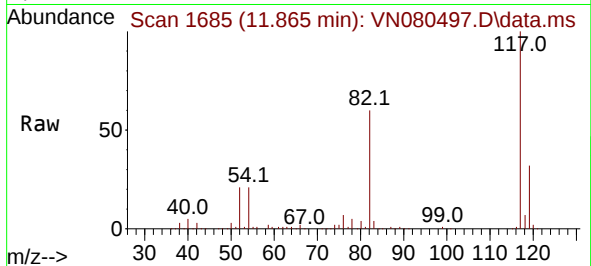

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080497.D
Acq: 15 Dec 2023 10:50

Tgt Ion:152 Resp: 187510
Ion Ratio Lower Upper
152 100
115 67.0 32.3 96.8
150 158.0 0.0 355.8

