
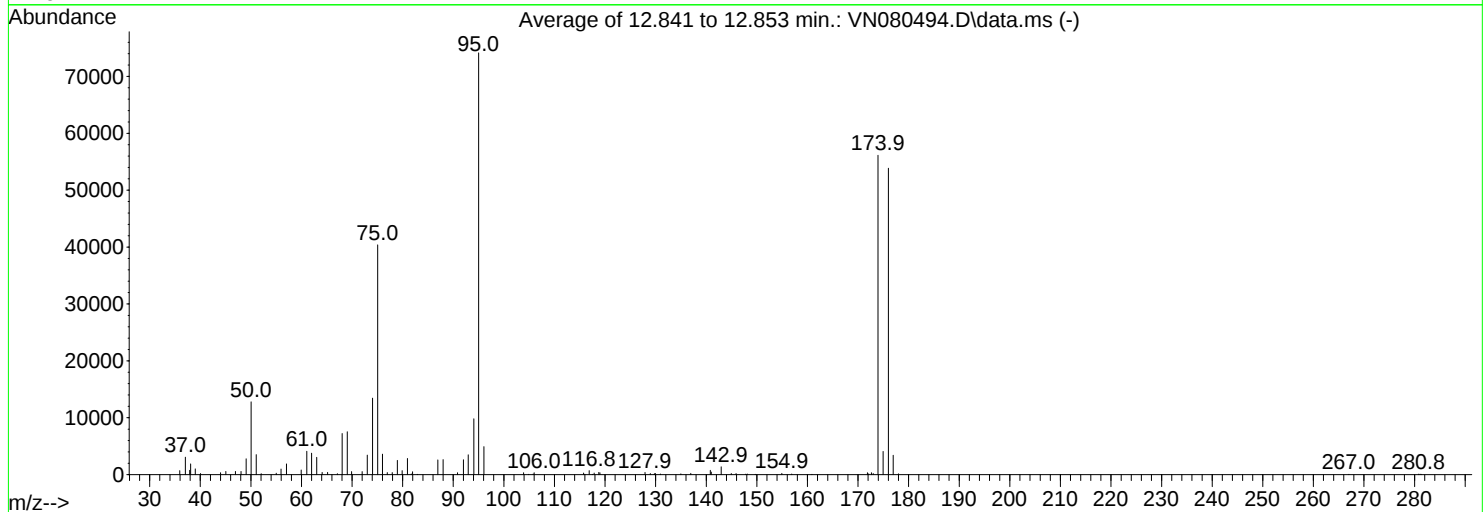


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121523\
Data File : VN080494.D
Acq On : 15 Dec 2023 09:01
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

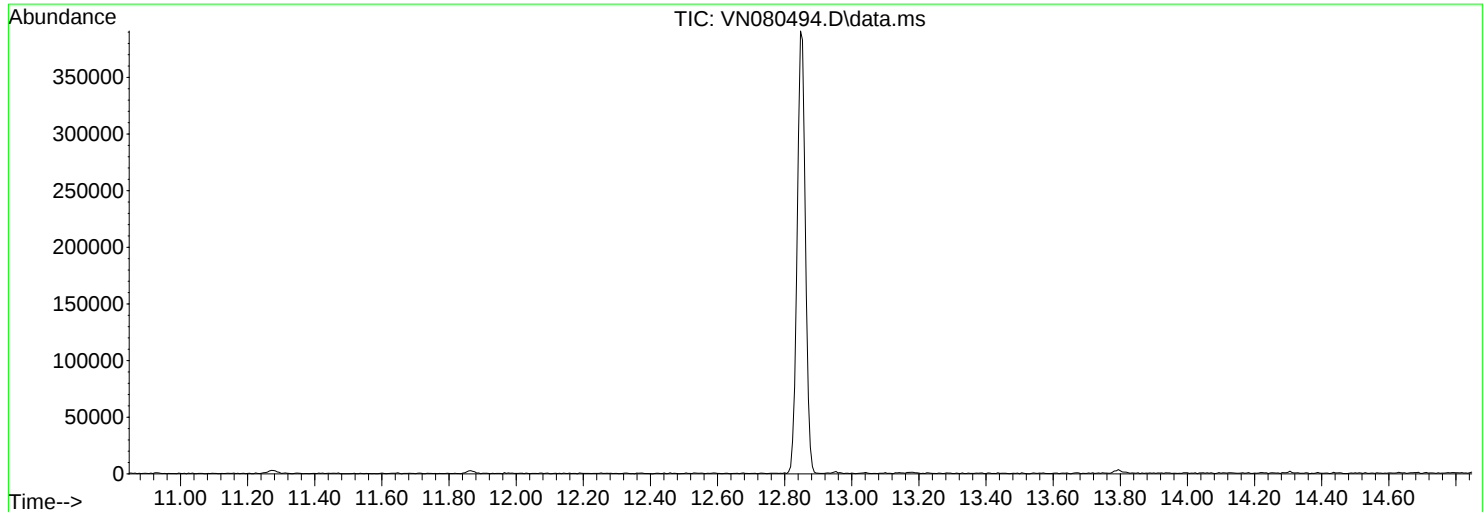

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	12808	PASS
75	95	30	60	54.5	40403	PASS
95	95	100	100	100.0	74147	PASS
96	95	5	9	6.6	4918	PASS
173	174	0.00	2	0.4	203	PASS
174	95	50	100	75.7	56141	PASS
175	174	5	9	7.3	4092	PASS
176	174	95	101	96.0	53875	PASS
177	176	5	9	6.3	3414	PASS

Average of 12.841 to 12.853 min.: VN080494.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	694	50.05	12808	65.15	406	77.95	36
37.05	3058	51.05	3529	67.10	159	78.95	251
37.90	772	52.05	162	68.05	7216	79.90	71
38.10	1889	55.00	245	69.05	7545	80.95	283
39.00	1020	55.95	993	69.90	530	81.70	126
40.05	198	57.05	1881	72.00	527	81.95	499
44.00	331	59.95	814	73.00	3444	82.90	53
45.05	565	61.05	4099	74.05	13450	86.95	2603
46.95	575	62.00	3777	75.05	40403	88.00	2639
48.05	555	63.00	3042	76.00	3613	90.85	354
49.05	2777	64.10	396	76.95	382	92.00	2624

Average of 12.841 to 12.853 min.: VN080494.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	3489	117.50	51	136.95	214	160.90	62
94.05	9814	117.85	272	140.80	765	171.85	351
95.00	74147	118.75	410	141.00	451	172.10	132
96.05	4918	119.00	352	142.95	1373	172.65	350
103.90	332	127.90	390	144.95	203	173.00	203
104.90	61	128.95	201	145.90	198	173.95	56141
105.80	111	129.70	79	147.80	93	174.95	4092
106.00	337	129.80	163	148.10	102	176.00	53875
115.75	279	129.95	193	149.70	54	176.95	3414
116.00	55	130.95	120	154.95	233	178.00	151
116.85	699	135.00	132	156.90	122	267.00	68

Average of 12.841 to 12.853 min.: VN080494.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
280.80	84						
281.10	73						
281.30	64						

Instrument :

MSVOA_N

ClientSampleId :

BFB