


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121620\
Data File : VN065155.D
Acq On : 15 Dec 2020 20:33
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121620W.M
Title : Sw846 8260
Last Update : Wed Dec 16 08:46:21 2020

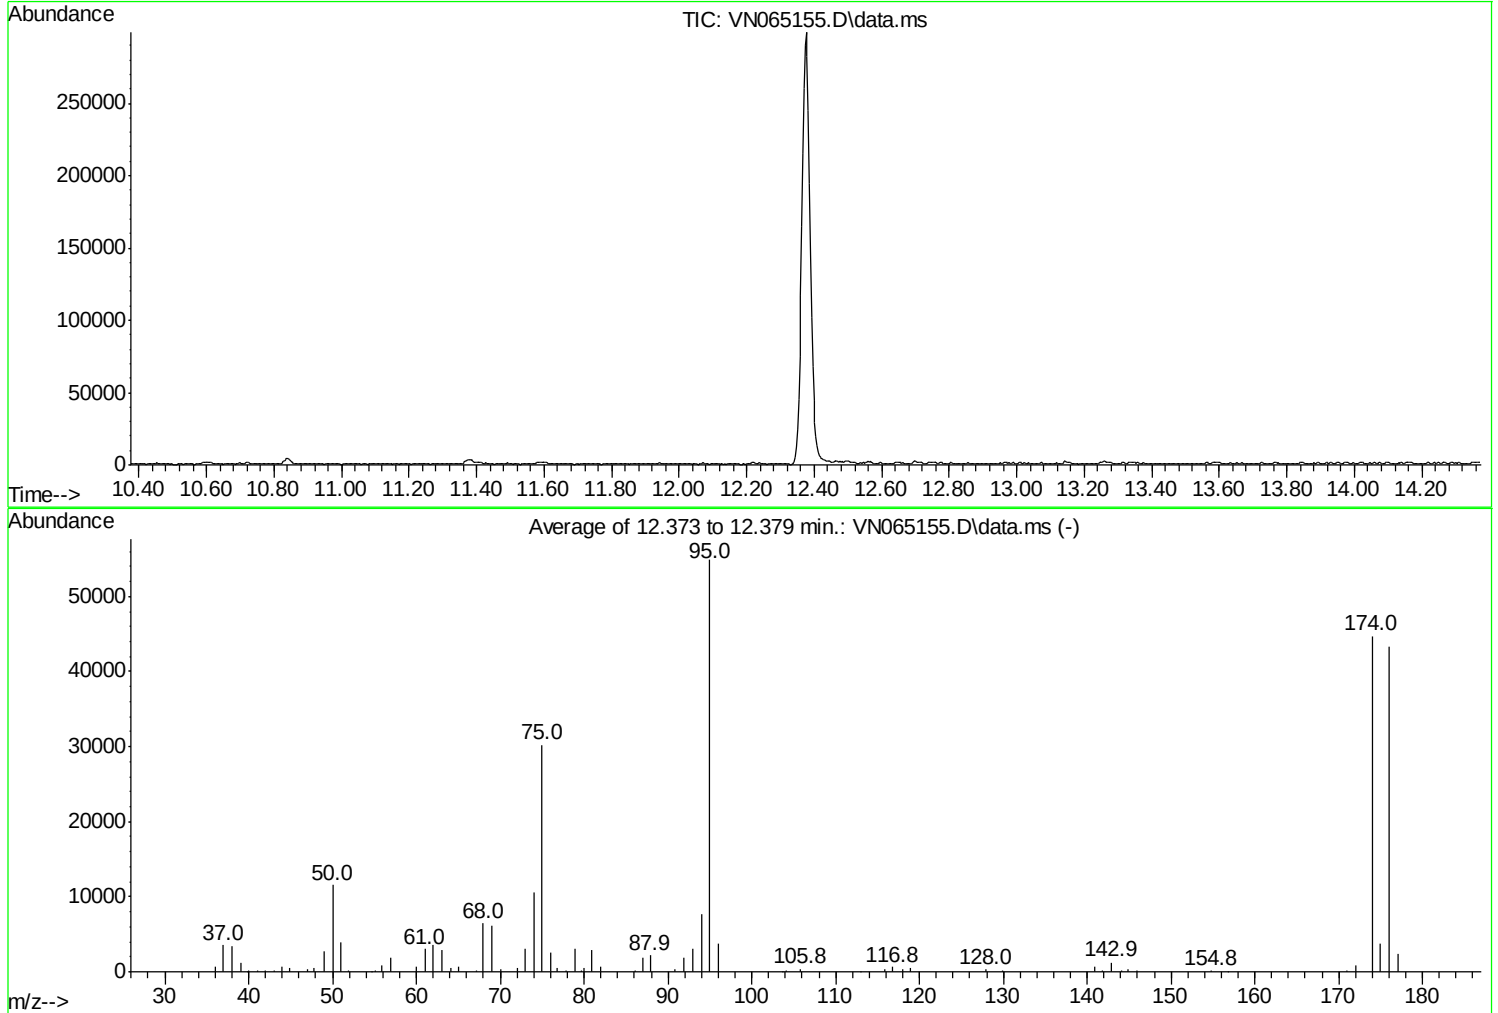

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.1	11562	PASS
75	95	30	60	55.0	30187	PASS
95	95	100	100	100.0	54885	PASS
96	95	5	9	6.9	3790	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.5	44736	PASS
175	174	5	9	8.4	3743	PASS
176	174	95	101	97.0	43379	PASS
177	176	5	9	5.6	2436	PASS