


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121620\
 Data File : VN065164.D
 Acq On : 16 Dec 2020 9:25
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N121520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Dec 15 15:18:54 2020

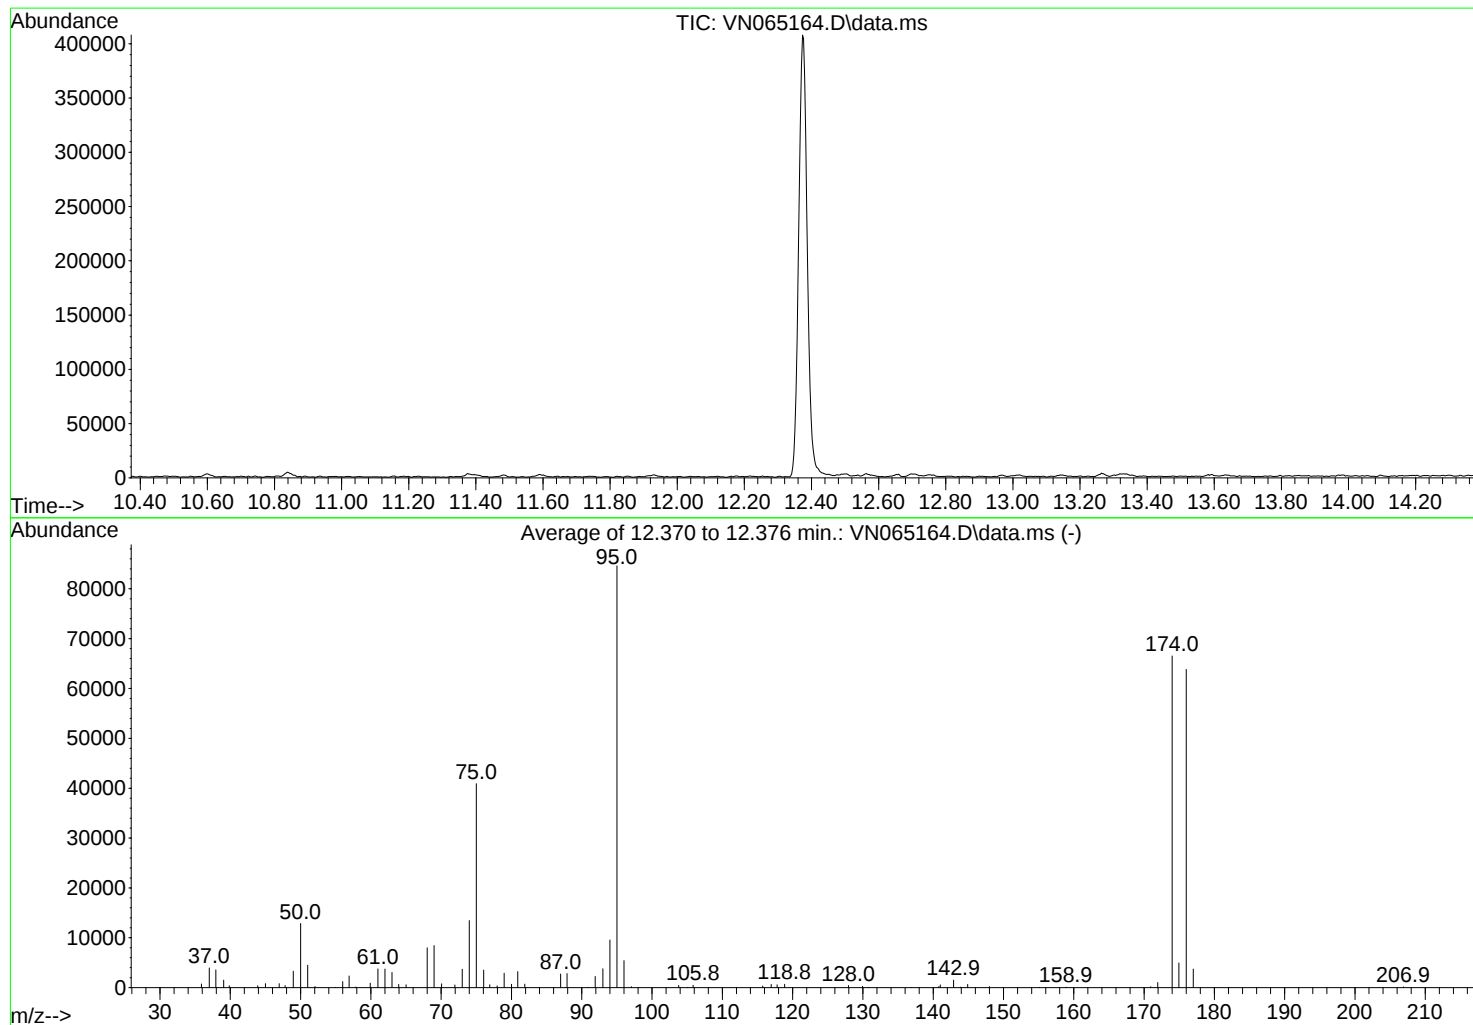

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12859	PASS
75	95	30	60	48.4	40907	PASS
95	95	100	100	100.0	84603	PASS
96	95	5	9	6.4	5414	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.7	66541	PASS
175	174	5	9	7.4	4938	PASS
176	174	95	101	96.0	63851	PASS
177	176	5	9	5.8	3730	PASS