

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121621\
 Data File : VN070133.D
 Acq On : 16 Dec 2021 13:14
 Operator : JC/MD
 Sample : M5011-20
 Misc : 3.83g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 16 15:47:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.080	168	1189414	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	2297670	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	2460579	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	1282226	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	962000	52.383	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 104.760%			
35) Dibromofluoromethane	8.018	113	637612	44.303	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 88.600%			
50) Toluene-d8	10.440	98	2995789	51.840	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 103.680%			
62) 4-Bromofluorobenzene	12.733	95	1286037	61.428	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 122.860%			
Target Compounds						Qvalue
3) Chloromethane	2.295	50	3623	0.208	ug/l	100
13) Acrolein	4.025	56	658	0.223	ug/l #	1
16) Acetone	4.315	43	16013	1.450	ug/l #	85
18) Methyl Acetate	4.856	43	7761	0.233	ug/l #	60
20) Methylene Chloride	5.068	84	5375	0.366	ug/l #	85
25) 2-Butanone	7.353	43	162424	10.821	ug/l #	89
29) Tetrahydrofuran	7.702	42	10086	1.107	ug/l #	68
31) Cyclohexane	8.080	56	30241	1.183	ug/l #	13
36) 1,1-Dichloropropene	8.077	75	101062	4.620	ug/l #	49
37) Ethyl Acetate	7.353	43	162424	4.989	ug/l #	68
38) Carbon Tetrachloride	8.077	117	124645	5.811	ug/l #	16
49) 1,4-Dioxane	9.590	88	398	0.987	ug/l #	69
51) 4-Methyl-2-Pentanone	10.336	43	6291	0.201	ug/l #	37
53) t-1,3-Dichloropropene	10.708	75	225	2.802	ug/l #	53
54) cis-1,3-Dichloropropene	10.185	75	172	2.005	ug/l #	33
56) Ethyl methacrylate	10.762	69	309	2.289	ug/l #	1
58) 2-Chloroethyl Vinyl ether	9.818	63	79	18.398	ug/l	99
59) 2-Hexanone	11.097	43	8762	0.371	ug/l	90
60) Dibromochloromethane	11.290	129	547	2.406	ug/l	90
71) Bromoform	12.465	173	1133	2.802	ug/l #	29
74) N-amyl acetate	12.312	43	16724	0.331	ug/l #	59
76) 1,2,3-Trichloropropane	12.733	75	704028	19.146	ug/l #	1
77) Bromobenzene	12.961	156	99131	3.699	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	704028	61.634	ug/l #	5
83) tert-Butylbenzene	13.321	119	19973	0.246	ug/l #	35
89) n-Butylbenzene	13.940	91	18970	0.271	ug/l #	74
90) Hexachloroethane	14.214	117	6058	0.400	ug/l #	8
93) 1,2,4-Trichlorobenzene	15.265	180	6403	3.165	ug/l	90
95) Naphthalene	15.507	128	63478	4.917	ug/l	99
96) 1,2,3-Trichlorobenzene	15.700	180	6971	2.759	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121621\
Data File : VN070133.D
Acq On : 16 Dec 2021 13:14
Operator : JC/MD
Sample : M5011-20
Misc : 3.83g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Dec 16 15:47:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 03 08:46:47 2021
Response via : Initial Calibration

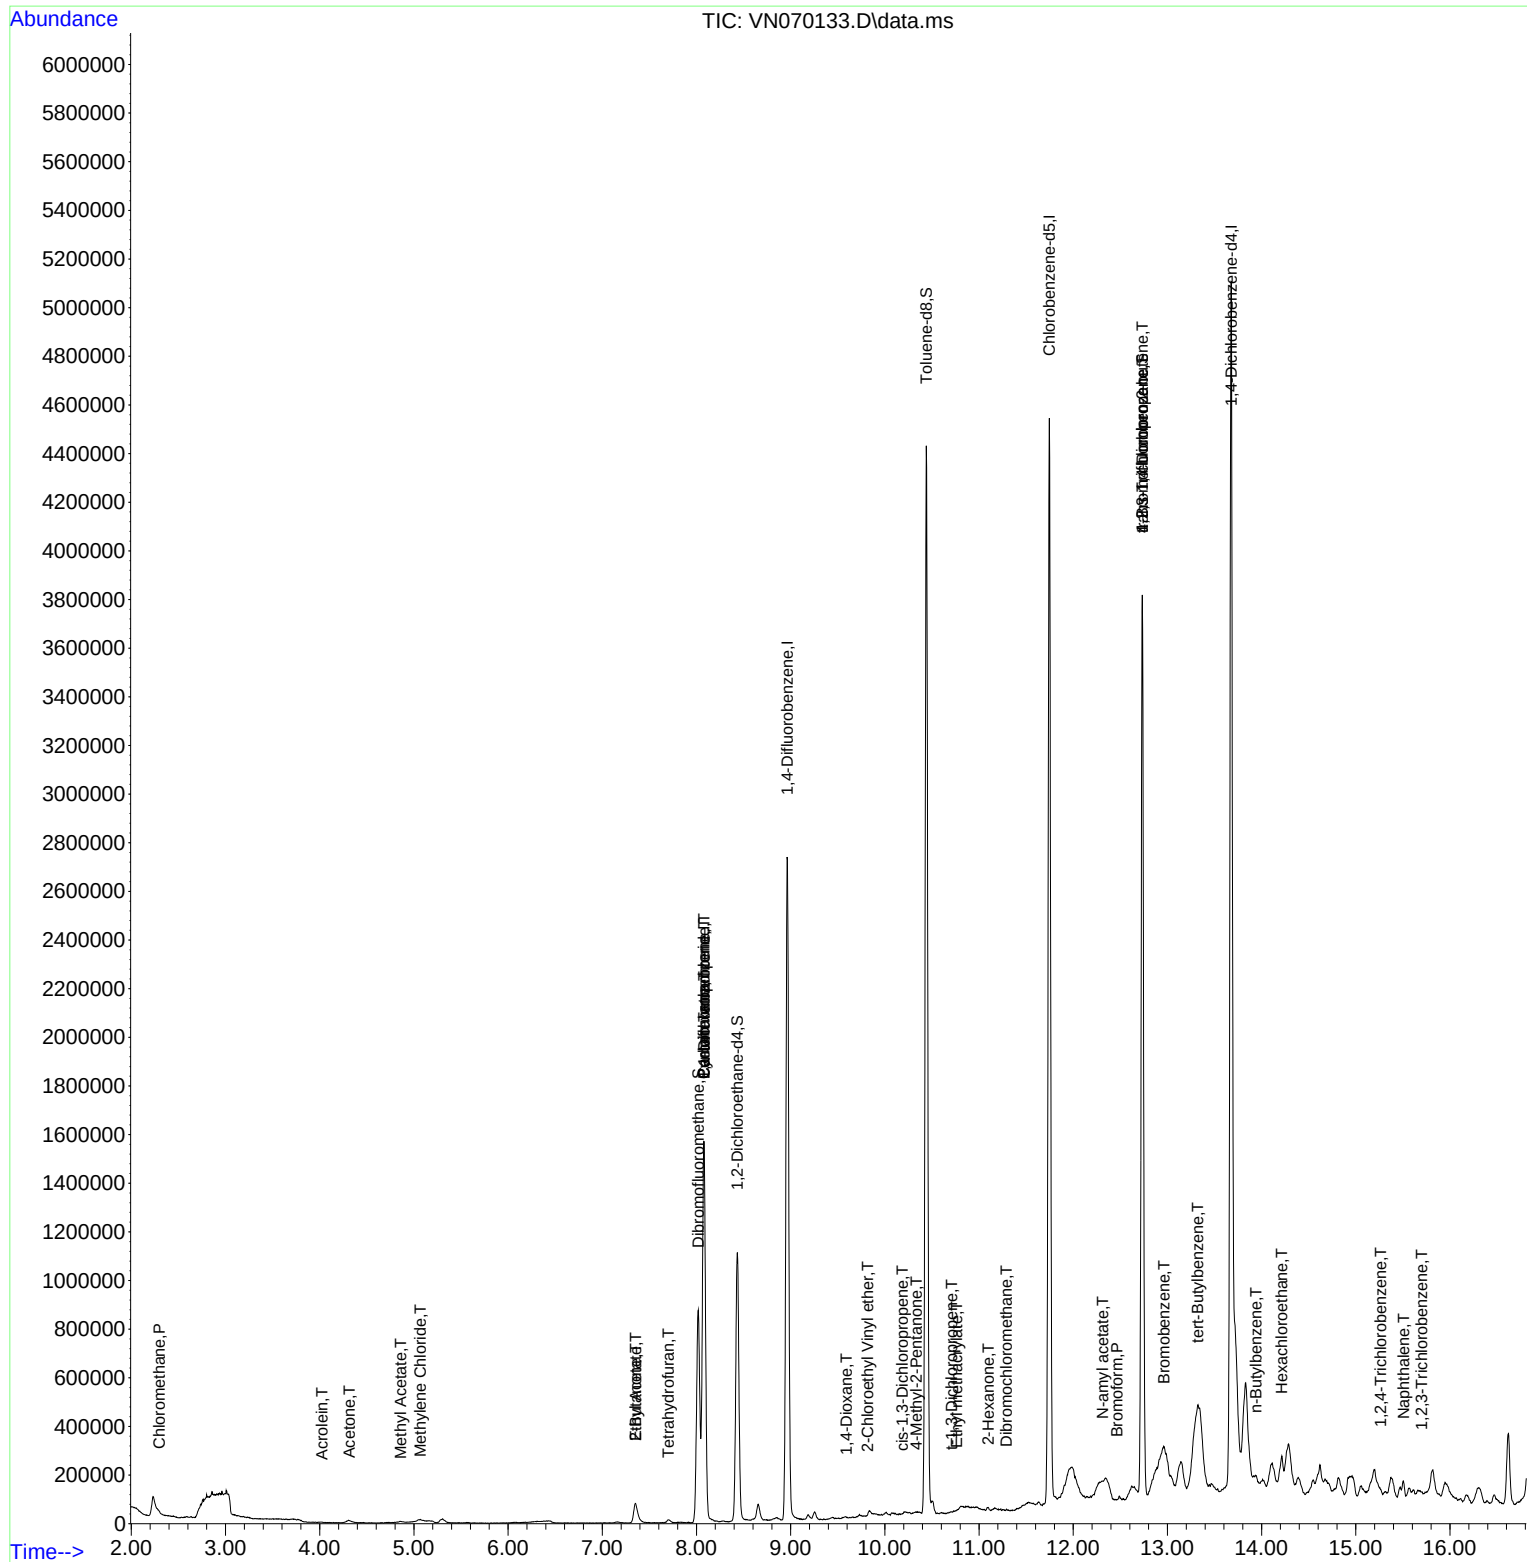



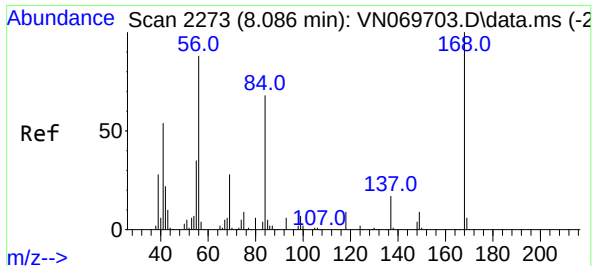


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :



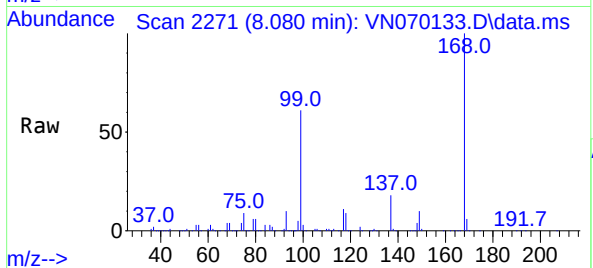



Tgt Ion:168 Resp: 1189414
Ion Ratio Lower Upper
168 100
99 61.1 41.3 61.9

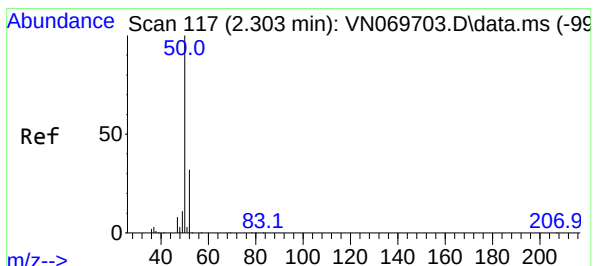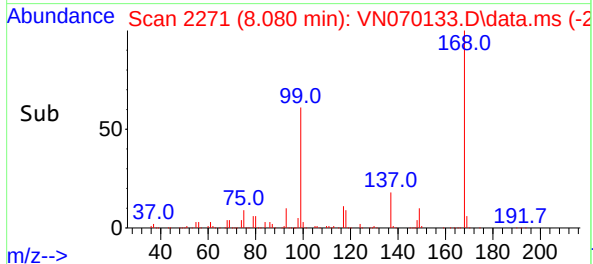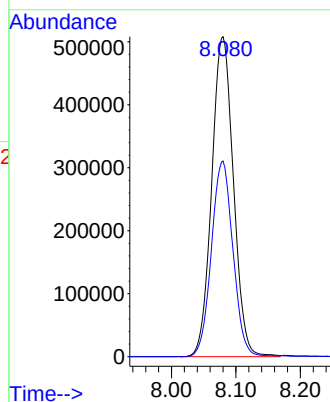

#3
Chloromethane
Concen: 0.208 ug/l
RT: 2.295 min Scan# 114
Delta R.T. -0.008 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 50 Resp: 3623
Ion Ratio Lower Upper
50 100
52 31.4 25.4 38.0


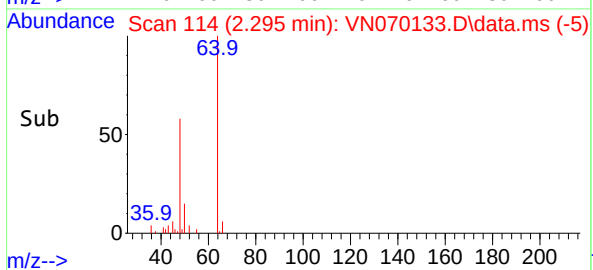
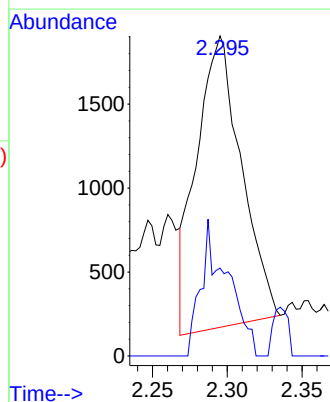
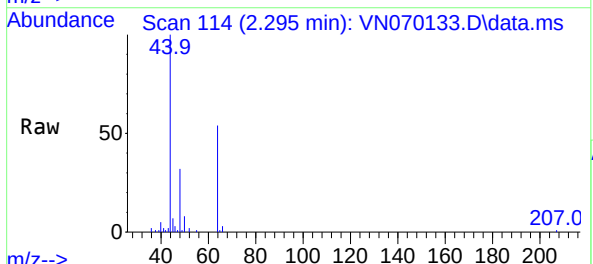




#13
Acrolein
Concen: 0.223 ug/l
RT: 4.025 min Scan# 71
Delta R.T. -0.013 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 658
Ion Ratio Lower Upper
56 100
55 189.5 56.6 85.0#



#16
Acetone
Concen: 1.450 ug/l
RT: 4.315 min Scan# 867
Delta R.T. 0.024 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 43 Resp: 16013
Ion Ratio Lower Upper
43 100
58 37.0 23.1 34.7#


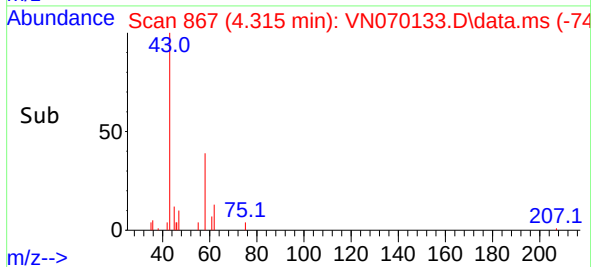

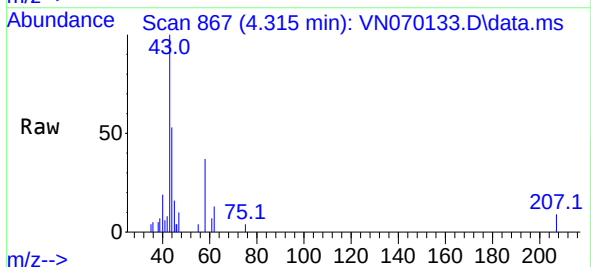


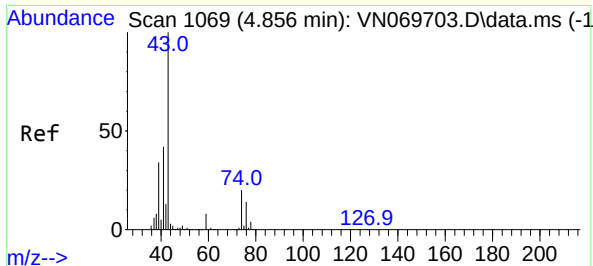

#18
Methyl Acetate
Concen: 0.233 ug/l
RT: 4.856 min Scan# 1148
Delta R.T. -0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 7761
Ion Ratio Lower Upper
43 100
74 4.4 19.4 29.2#

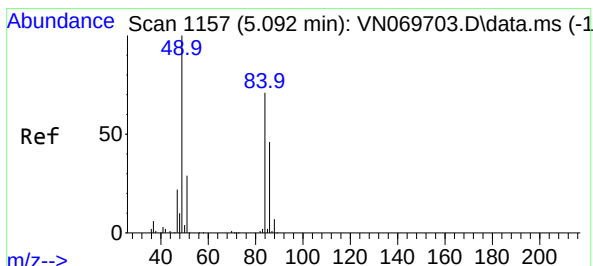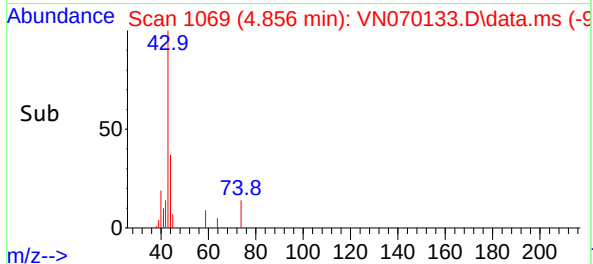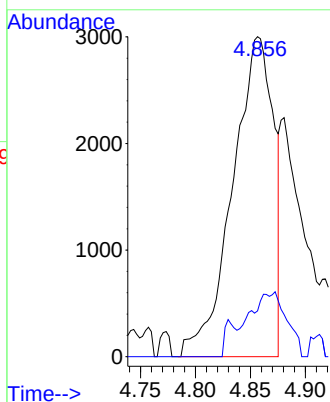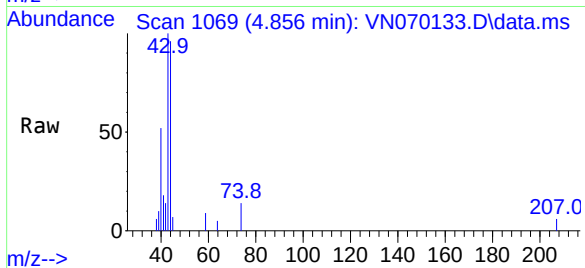

#20
Methylene Chloride
Concen: 0.366 ug/l
RT: 5.068 min Scan# 1148
Delta R.T. -0.024 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 84 Resp: 5375
Ion Ratio Lower Upper
84 100
49 100.2 93.5 140.3
51 37.0 29.4 44.2
86 48.0 53.0 79.4#


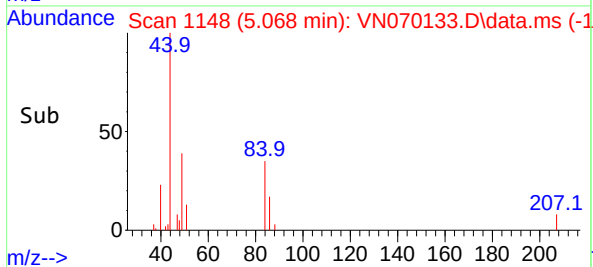
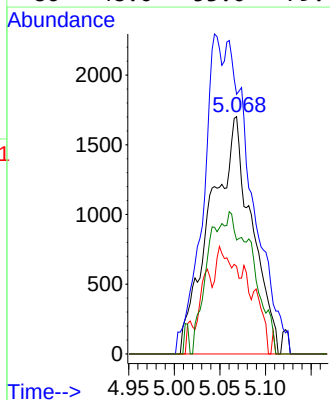
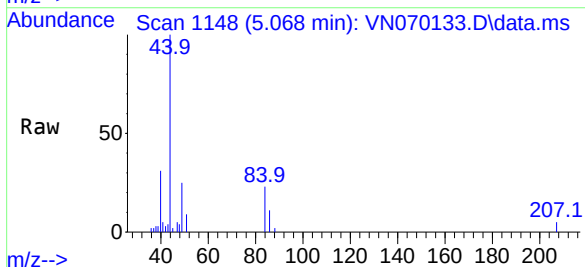


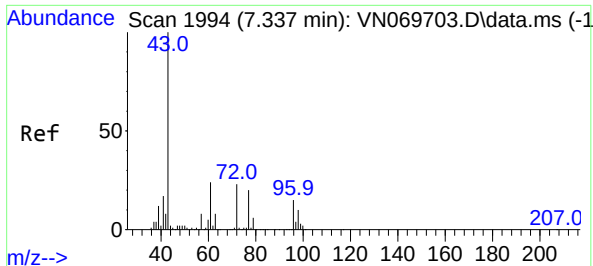

#25
2-Butanone
Concen: 10.821 ug/l
RT: 7.353 min Scan# 20
Delta R.T. 0.016 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 162424
Ion Ratio Lower Upper
43 100
72 21.6 21.7 32.5#

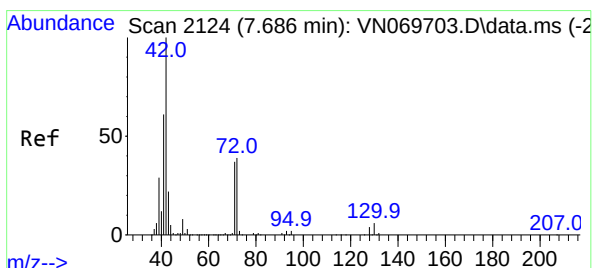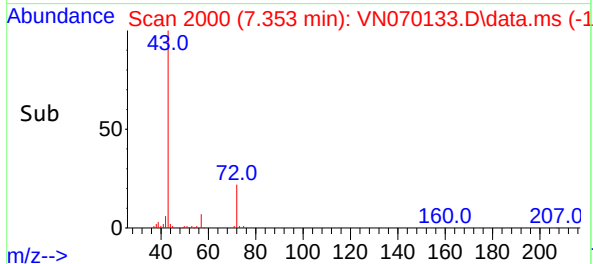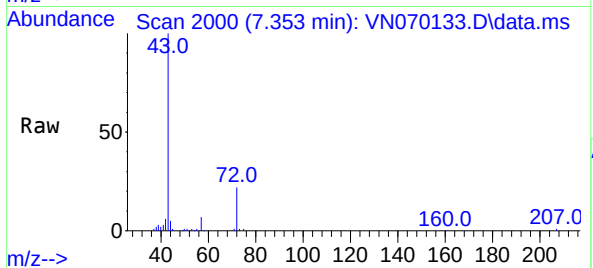

#29
Tetrahydrofuran
Concen: 1.107 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.016 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Tgt Ion: 42 Resp: 10086
Ion Ratio Lower Upper
42 100
72 37.8 36.3 54.5
71 8.8 34.7 52.1#

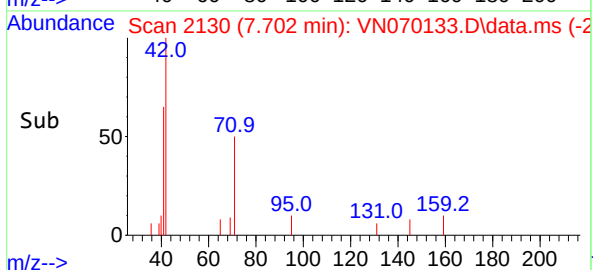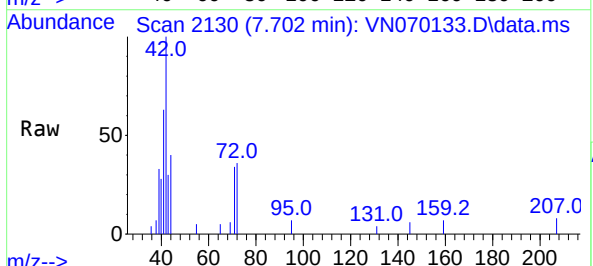






#31
Cyclohexane
Concen: 1.183 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.013 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 30241
Ion Ratio Lower Upper
56 100
69 156.9 27.1 40.7#
84 128.9 73.4 110.0#

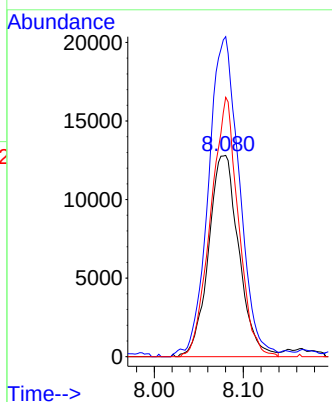

#33
1,2-Dichloroethane-d4
Concen: 52.383 ug/l
RT: 8.434 min Scan# 2403
Delta R.T. -0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Tgt Ion: 65 Resp: 962000
Ion Ratio Lower Upper
65 100
67 50.9 0.0 103.0

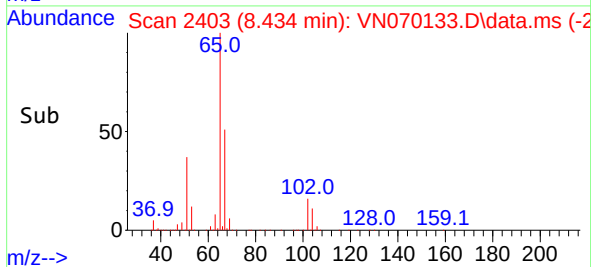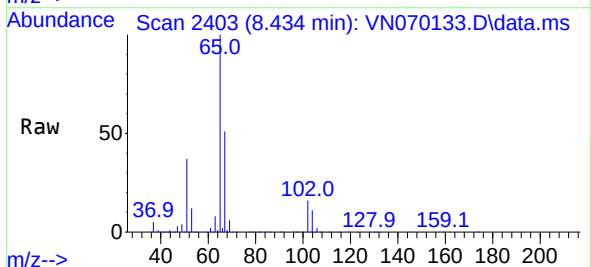



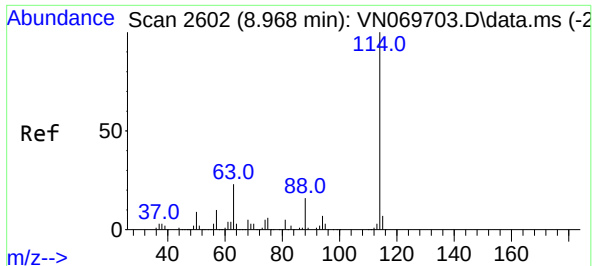


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :



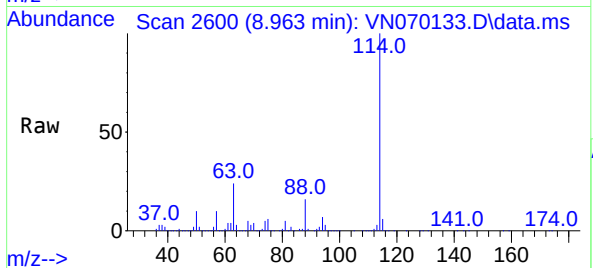



Tgt Ion:114 Resp: 2297670
Ion Ratio Lower Upper
114 100
63 23.9 0.0 37.8
88 16.5 0.0 27.4

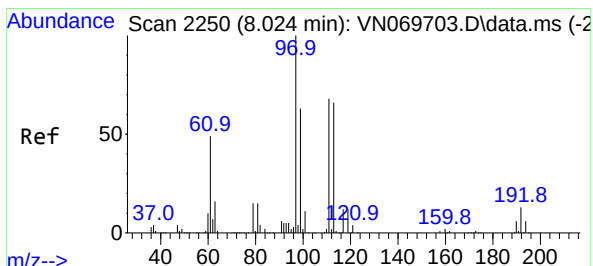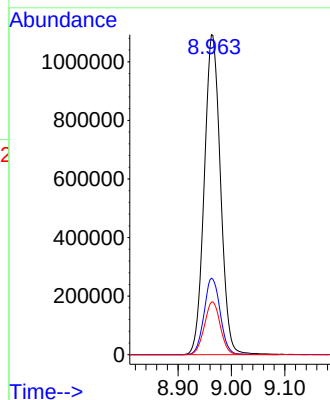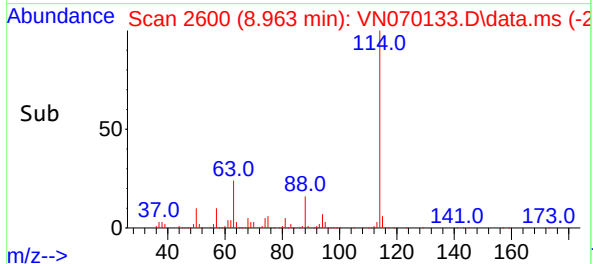

#35
Dibromofluoromethane
Concen: 44.303 ug/l
RT: 8.018 min Scan# 2248
Delta R.T. -0.005 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion:113 Resp: 637612
Ion Ratio Lower Upper
113 100
111 103.8 82.2 123.2
192 19.3 16.9 25.3

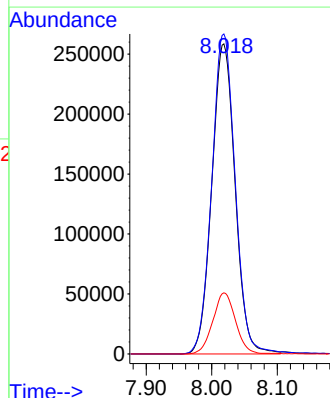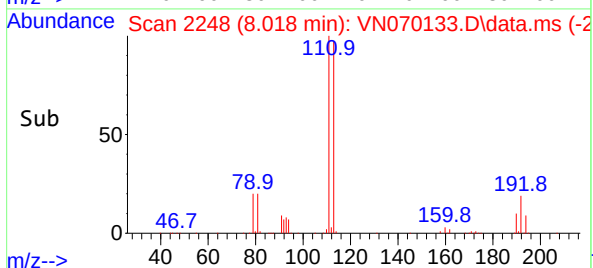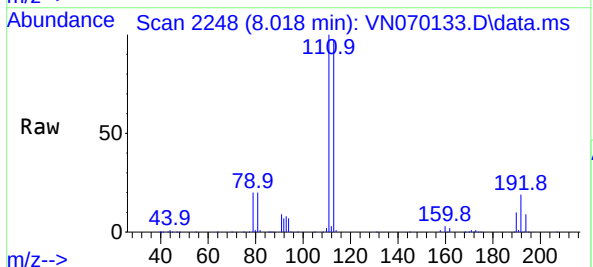

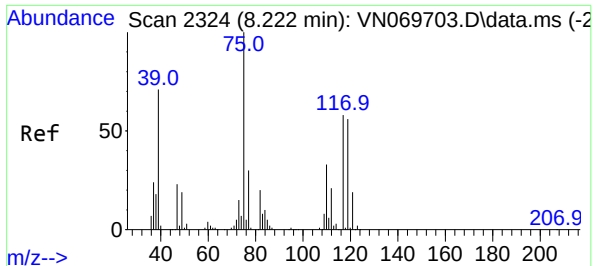

#36

1,1-Dichloropropene

Concen: 4.620 ug/l

RT: 8.077 min Scan# 21

Delta R.T. -0.145 min

Lab File: VN070133.D

Acq: 16 Dec 2021 13:14

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 75 Resp: 101062

Ion Ratio Lower Upper

75 100

110 8.4 18.4 55.2#

77 0.2 24.4 36.6#

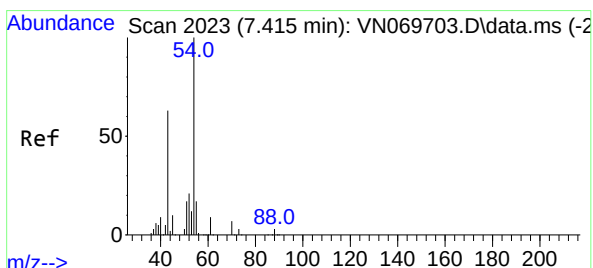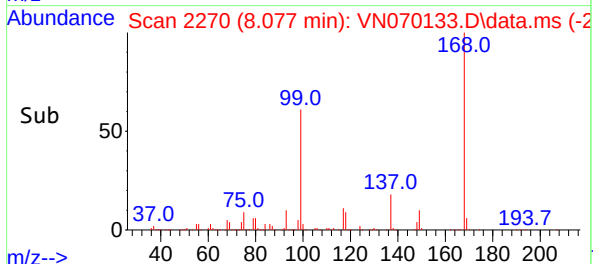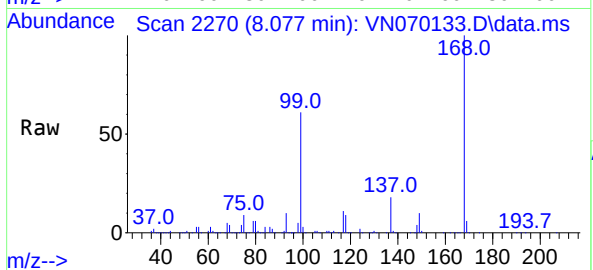

#37

Ethyl Acetate

Concen: 4.989 ug/l

RT: 7.353 min Scan# 2000

Delta R.T. -0.062 min

Lab File: VN070133.D

Acq: 16 Dec 2021 13:14




Tgt Ion: 43 Resp: 162424


Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#


70 0.0 7.9 11.9#

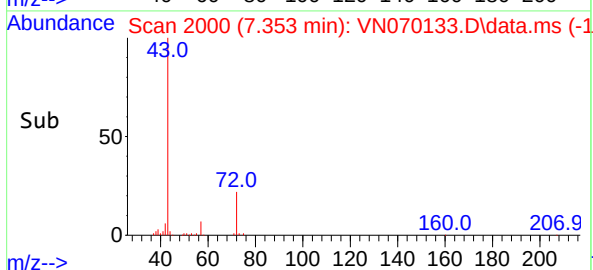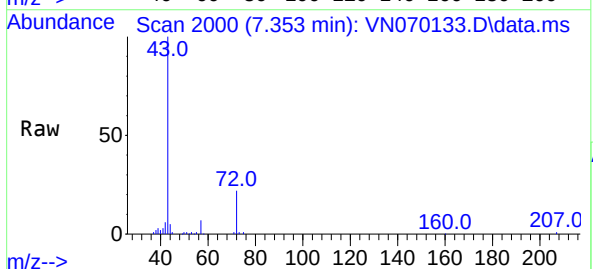






#38
Carbon Tetrachloride
Concen: 5.811 ug/l
RT: 8.077 min Scan# 21
Delta R.T. -0.129 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 124645
Ion Ratio Lower Upper
117 100
119 4.4 76.1 114.1#
121 0.0 24.2 36.2#

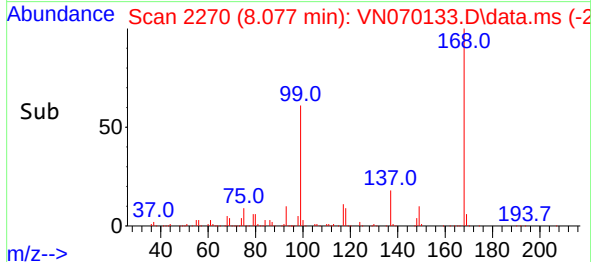

#49
1,4-Dioxane
Concen: 0.987 ug/l
RT: 9.590 min Scan# 2834
Delta R.T. 0.019 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 88 Resp: 398
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 47.2 50.6 75.8#


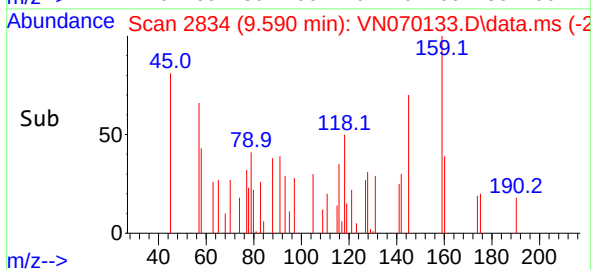






#50
Toluene-d8
Concen: 51.840 ug/l
RT: 10.440 min Scan# 3152
Delta R.T. -0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 2995789
Ion Ratio Lower Upper
98 100
100 64.1 50.4 75.6



#51
4-Methyl-2-Pentanone
Concen: 0.201 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Tgt Ion: 43 Resp: 6291
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#

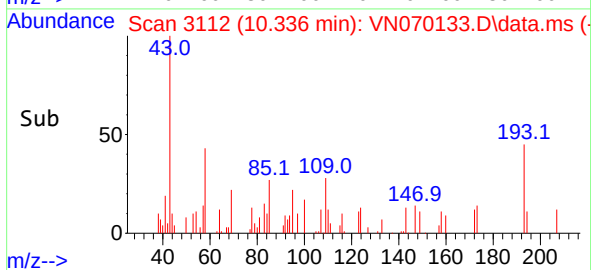






#53
t-1,3-Dichloropropene
Concen: 2.802 ug/l
RT: 10.708 min Scan# 31
Delta R.T. -0.011 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 75 Resp: 225
Ion Ratio Lower Upper
75 100
77 58.1 25.6 38.4#

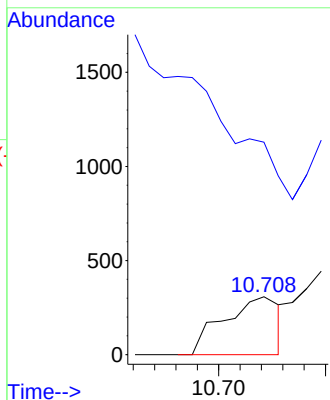


#54
cis-1,3-Dichloropropene
Concen: 2.005 ug/l
RT: 10.185 min Scan# 3056
Delta R.T. -0.006 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14



Tgt Ion: 75 Resp: 172
Ion Ratio Lower Upper
75 100
77 96.4 26.4 39.6#
39 25.4 42.5 63.7#



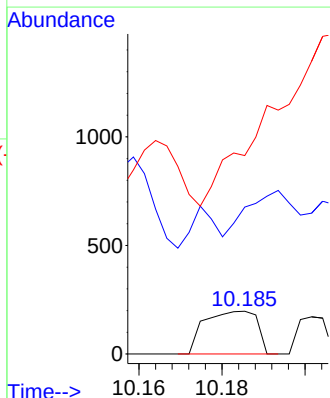





#56
Ethyl methacrylate
Concen: 2.289 ug/l
RT: 10.762 min Scan# 3199
Delta R.T. 0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 309
Ion Ratio Lower Upper
69 100
41 313.3 51.4 77.0#
39 0.0 34.6 52.0#



#58
2-Chloroethyl Vinyl ether
Concen: 18.398 ug/l
RT: 9.818 min Scan# 2919
Delta R.T. -0.225 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 63 Resp: 79
Ion Ratio Lower Upper
63 100
106 30.4 23.9 35.9









#59
2-Hexanone
Concen: 0.371 ug/l
RT: 11.097 min Scan# 31
Delta R.T. 0.010 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 8762
Ion Ratio Lower Upper
43 100
58 61.0 26.9 80.7



#60
Dibromochloromethane
Concen: 2.406 ug/l
RT: 11.290 min Scan# 3468
Delta R.T. 0.050 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 129 Resp: 547
Ion Ratio Lower Upper
129 100
127 85.6 38.6 116.0









#62
4-Bromofluorobenzene
Concen: 61.428 ug/l
RT: 12.733 min Scan# 4005
Delta R.T. 0.002 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 1286037
Ion Ratio Lower Upper
95 100
174 74.9 0.0 187.2
176 72.8 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 117 Resp: 2460579
Ion Ratio Lower Upper
117 100
82 60.0 42.4 63.6
119 32.3 25.4 38.2


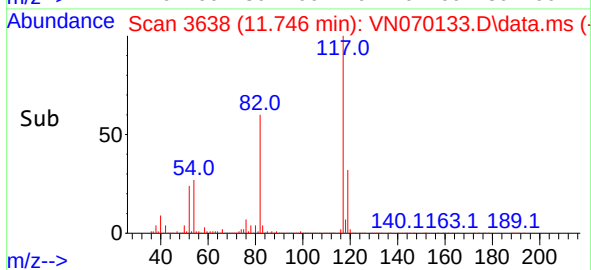






#71
Bromoform
Concen: 2.802 ug/l
RT: 12.465 min Scan# 3904
Delta R.T. 0.005 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 1133
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

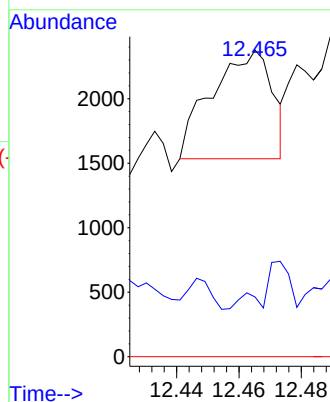

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion:152 Resp: 1282226
Ion Ratio Lower Upper
152 100
115 68.1 27.5 82.5
150 147.9 0.0 344.4


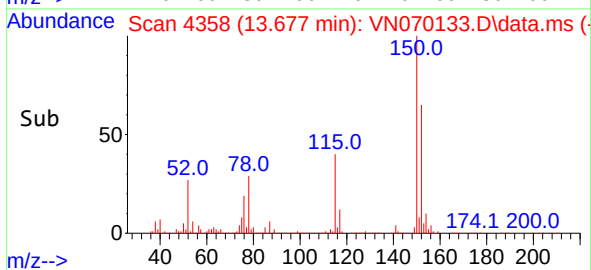
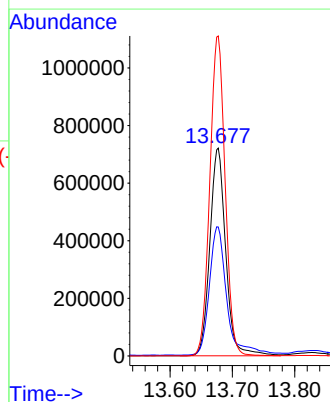





#74
N-amy1 acetate
Concen: 0.331 ug/l
RT: 12.312 min Scan# 3849
Delta R.T. -0.075 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 16724
Ion Ratio Lower Upper
43 100
70 15.1 33.4 50.0#
55 7.3 19.3 28.9#
61 0.0 18.5 27.7#

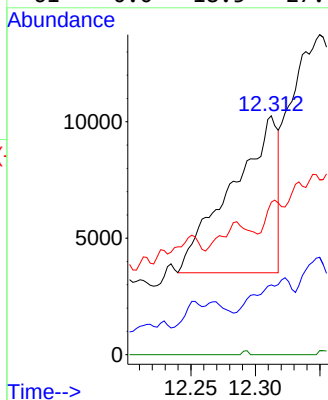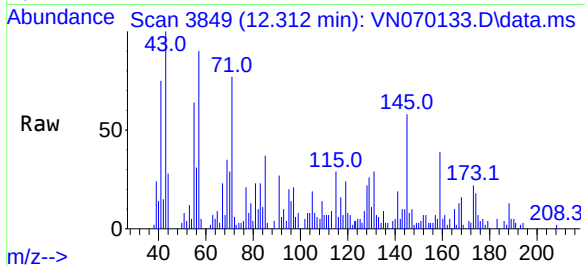

#76
1,2,3-Trichloropropane
Concen: 19.146 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.148 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Tgt Ion: 75 Resp: 704028
Ion Ratio Lower Upper
75 100
77 0.9 82.6 247.8#

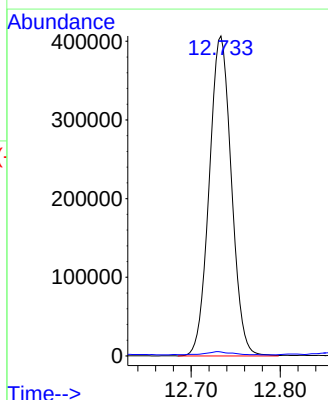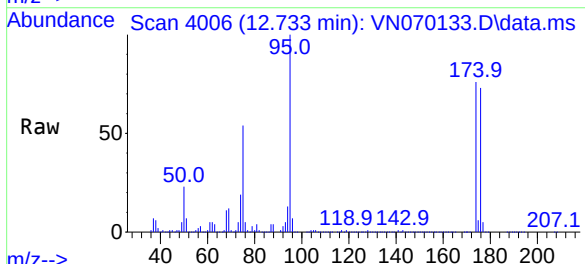






#77
Bromobenzene
Concen: 3.699 ug/l
RT: 12.961 min Scan# 4091
Delta R.T. 0.099 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:156 Resp: 99131
Ion Ratio Lower Upper
156 100
77 0.0 90.6 271.8#
158 0.0 48.9 146.7#

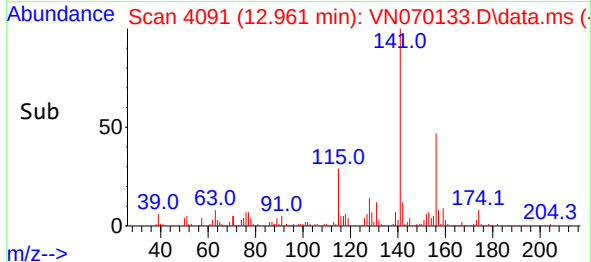


#81
trans-1,4-Dichloro-2-butene
Concen: 61.634 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Tgt Ion: 75 Resp: 704028
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

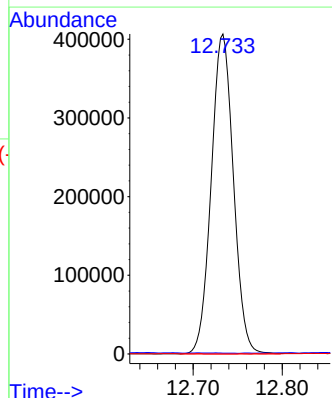






#83
tert-Butylbenzene
Concen: 0.246 ug/l
RT: 13.321 min Scan# 41
Delta R.T. -0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:119 Resp: 19973
Ion Ratio Lower Upper
119 100
91 7.2 31.5 94.5#
134 1.2 12.4 37.4#

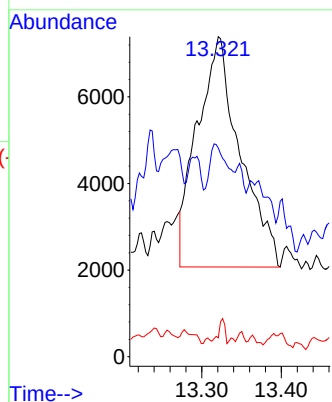

#89
n-Butylbenzene
Concen: 0.271 ug/l
RT: 13.940 min Scan# 4456
Delta R.T. -0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion: 91 Resp: 18970
Ion Ratio Lower Upper
91 100
92 42.3 25.4 76.0
134 0.0 13.6 40.8#


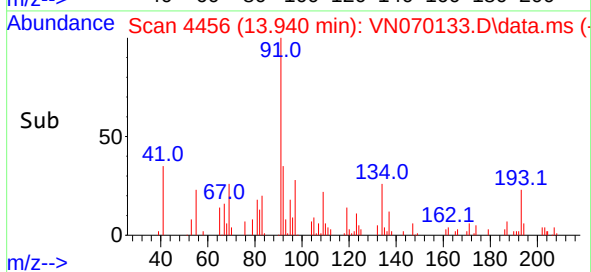
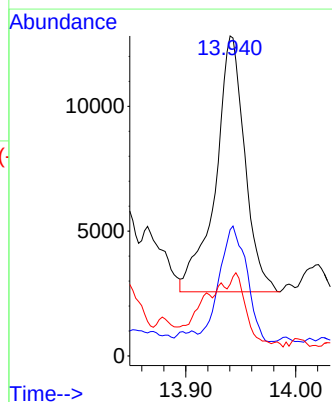





#90
Hexachloroethane
Concen: 0.400 ug/l
RT: 14.214 min Scan# 4557
Delta R.T. 0.003 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 6058
Ion Ratio Lower Upper
117 100
201 2.2 43.9 131.6#

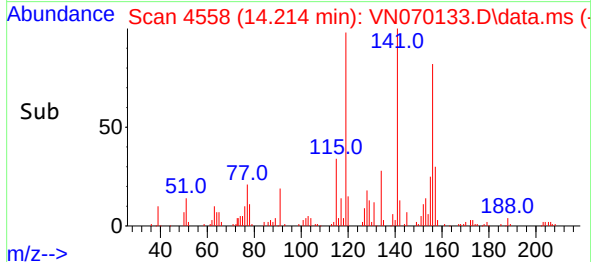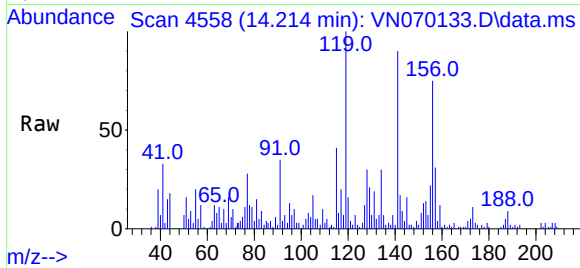

#93
1,2,4-Trichlorobenzene
Concen: 3.165 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion:180 Resp: 6403
Ion Ratio Lower Upper
180 100
182 90.9 48.3 144.9
145 15.8 14.5 43.5


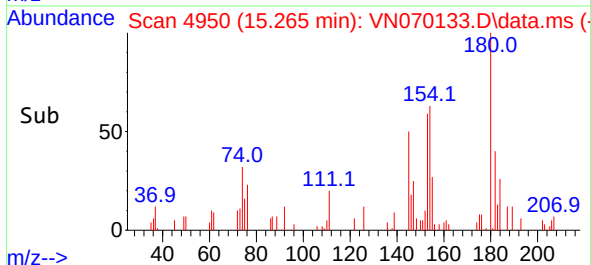
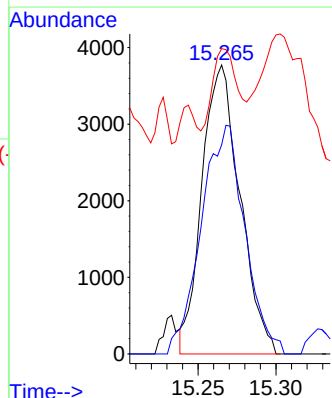
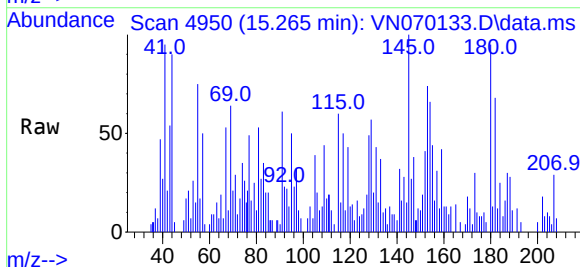




#95
Naphthalene
Concen: 4.917 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 63478
Ion Ratio Lower Upper
128 100
127 13.5 10.5 15.7
129 10.7 8.7 13.1

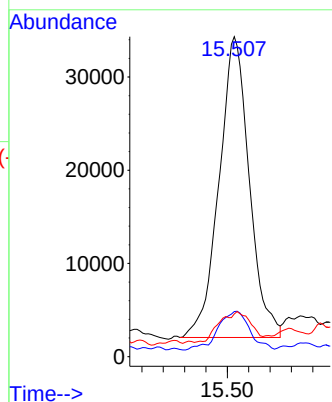

#96
1,2,3-Trichlorobenzene
Concen: 2.759 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.002 min
Lab File: VN070133.D
Acq: 16 Dec 2021 13:14

Tgt Ion:180 Resp: 6971
Ion Ratio Lower Upper
180 100
182 92.2 47.4 142.2
145 58.5 15.0 45.1#

