

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
 Data File : VN075844.D
 Acq On : 16 Dec 2022 13:50
 Operator : JC\MD
 Sample : N6088-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-2022-12-12

Quant Time: Dec 17 08:39:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	387149	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	604601	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	509529	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	205116	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	198869	47.217	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	94.440%
35) Dibromofluoromethane	8.177	113	178929	47.788	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.580%
50) Toluene-d8	10.571	98	688995	49.217	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.440%
62) 4-Bromofluorobenzene	12.853	95	208630	44.996	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
Data File : VN075844.D
Acq On : 16 Dec 2022 13:50
Operator : JC\MD
Sample : N6088-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-2022-12-12

Quant Time: Dec 17 08:39:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration



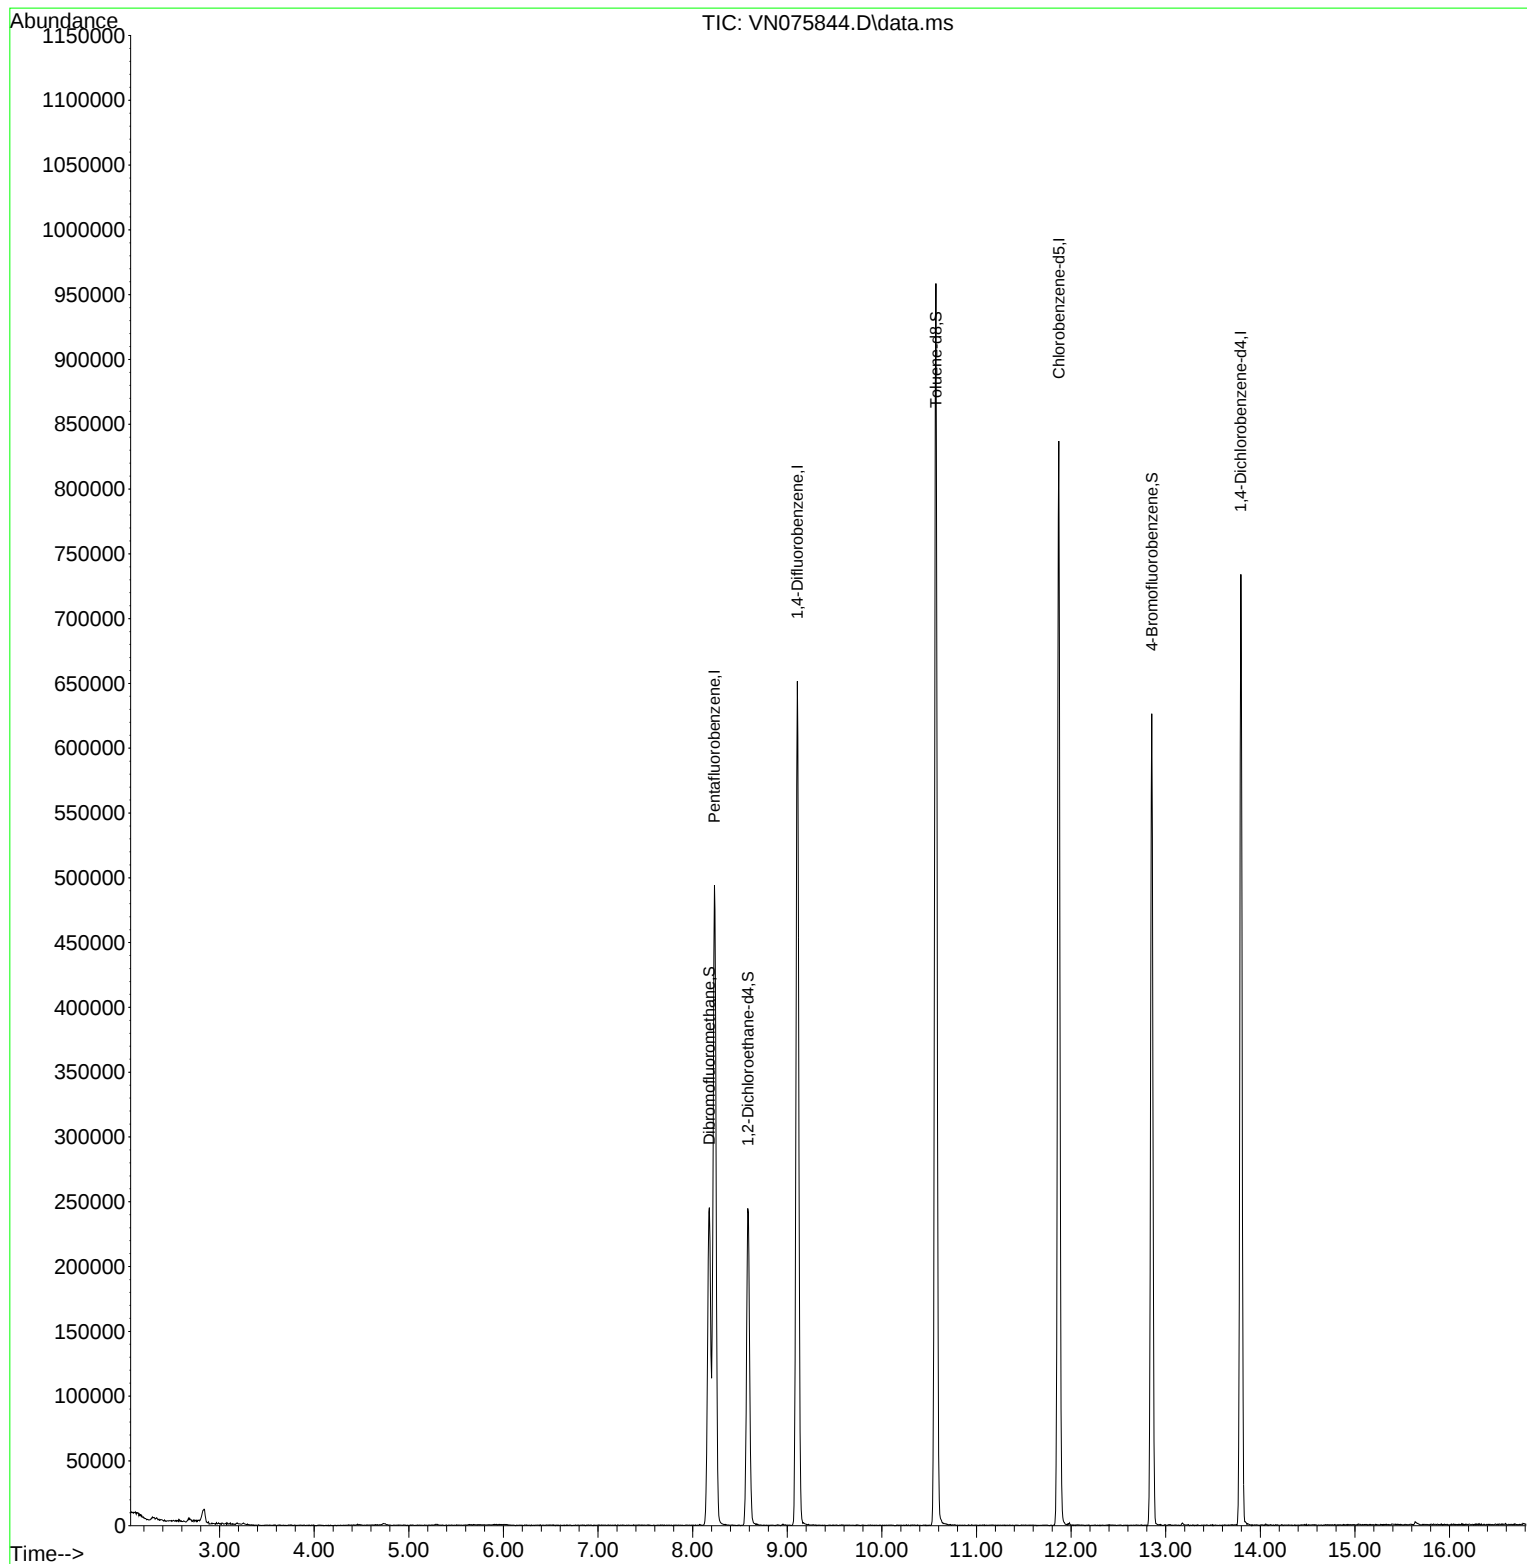


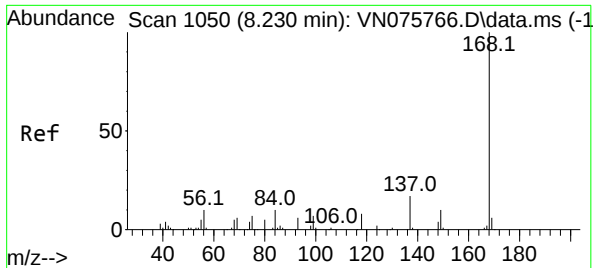

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50




Instrument :
MSVOA_N
ClientSampleId :
TB-2022-12-12

Tgt Ion:168 Resp: 387149
Ion Ratio Lower Upper
168 100
99 53.5 44.2 66.4

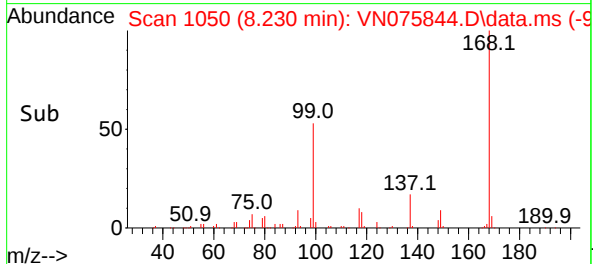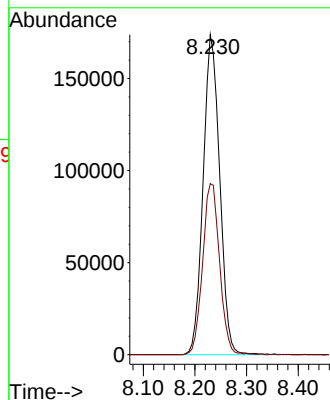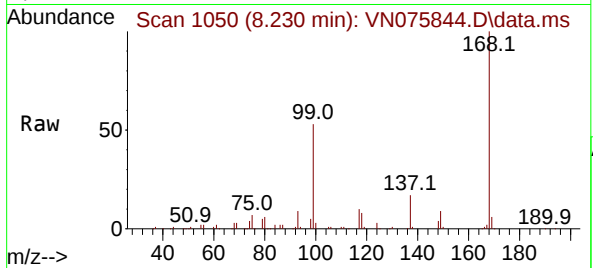

#33
1,2-Dichloroethane-d4
Concen: 47.217 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50

Tgt Ion: 65 Resp: 198869
Ion Ratio Lower Upper
65 100
67 51.7 0.0 103.4

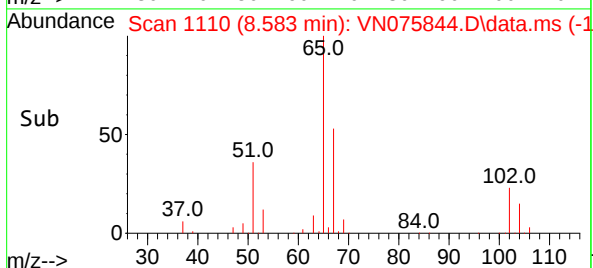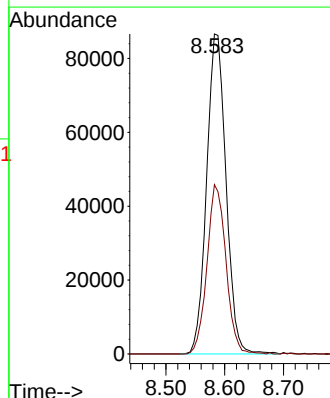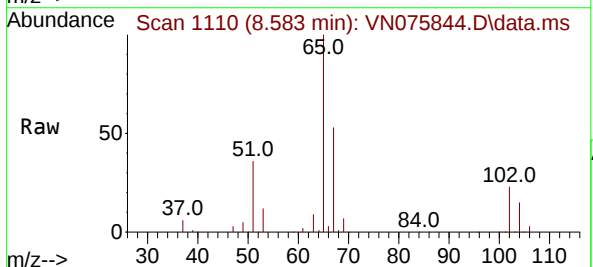



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075844.D

Acq: 16 Dec 2022 13:50

Instrument :

MSVOA_N

ClientSampleId :

TB-2022-12-12




Tgt Ion:114 Resp: 604601

Ion Ratio Lower Upper

114 100

63 17.8 0.0 34.4

88 14.2 0.0 28.8

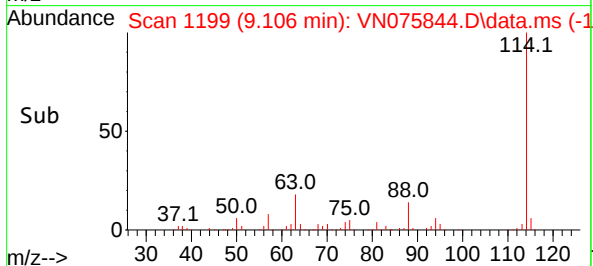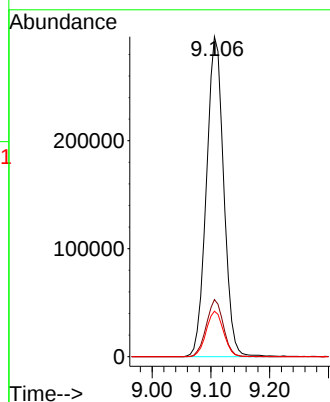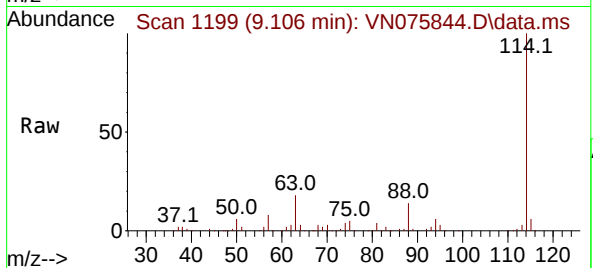

#35

Dibromofluoromethane

Concen: 47.788 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN075844.D

Acq: 16 Dec 2022 13:50




Tgt Ion:113 Resp: 178929


Ion Ratio Lower Upper

113 100

111 102.8 83.4 125.2

192 19.9 16.1 24.1


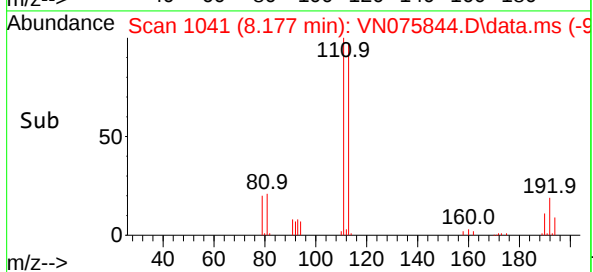
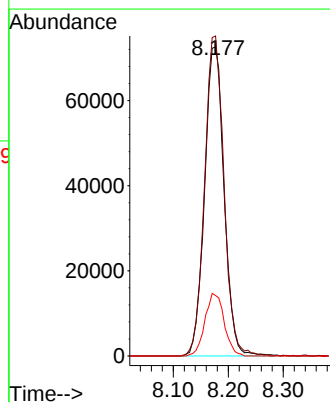
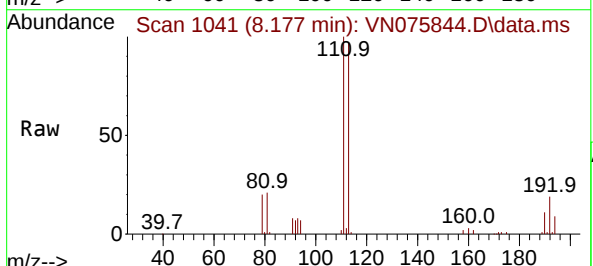


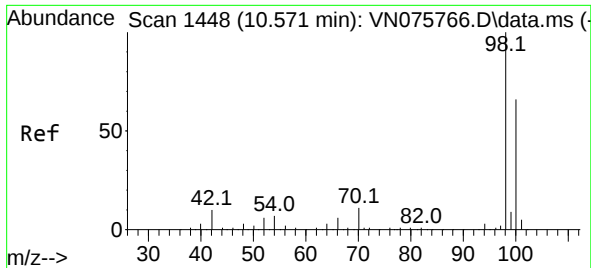

#50
Toluene-d8
Concen: 49.217 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50




Instrument :
MSVOA_N
ClientSampleId :
TB-2022-12-12


Tgt Ion: 98 Resp: 688995
Ion Ratio Lower Upper
98 100
100 65.5 52.1 78.1

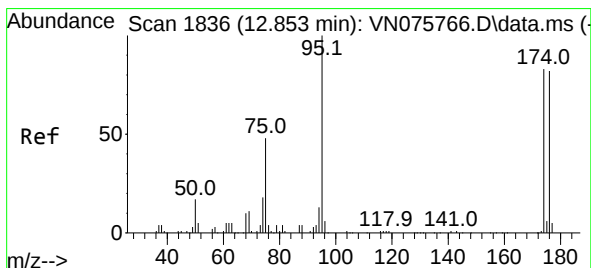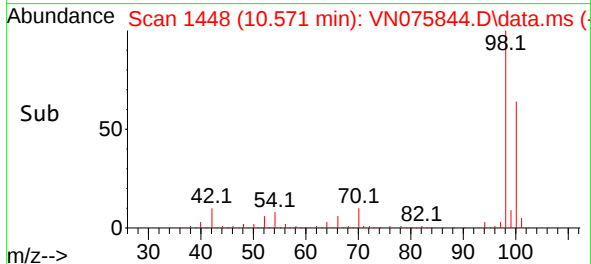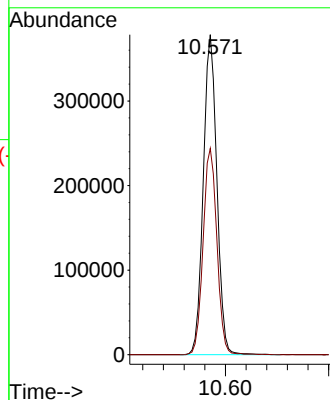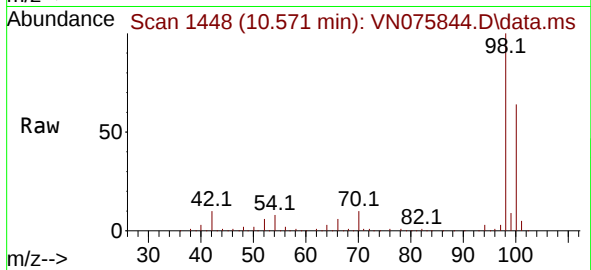

#62
4-Bromofluorobenzene
Concen: 44.996 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.000 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50

Tgt Ion: 95 Resp: 208630
Ion Ratio Lower Upper
95 100
174 87.4 0.0 171.6
176 84.1 0.0 169.2


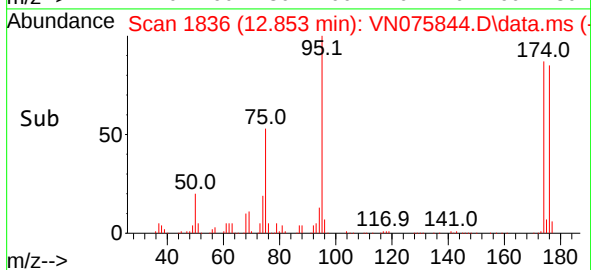
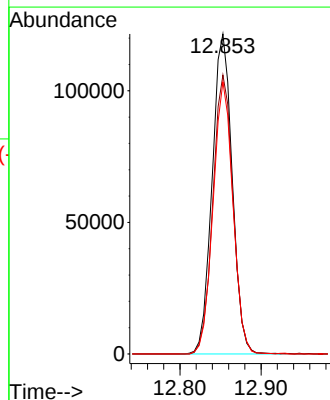
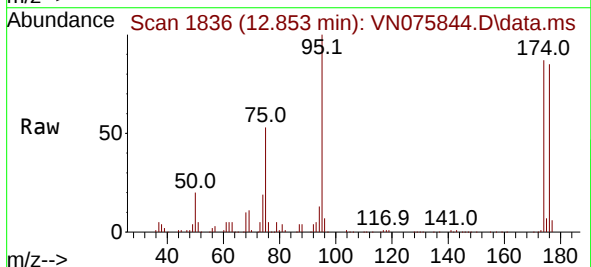


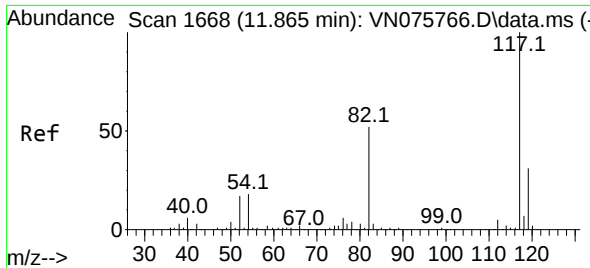

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50

Instrument :
MSVOA_N
ClientSampleId :
TB-2022-12-12

Tgt Ion:117 Resp: 509529
Ion Ratio Lower Upper
117 100
82 52.3 41.3 61.9
119 31.6 24.6 37.0

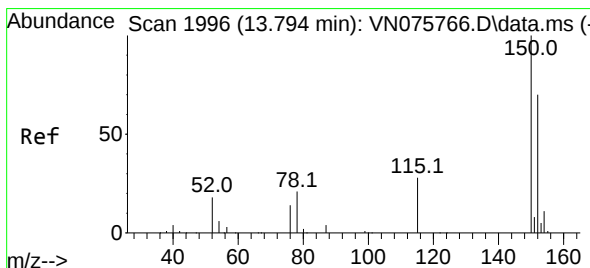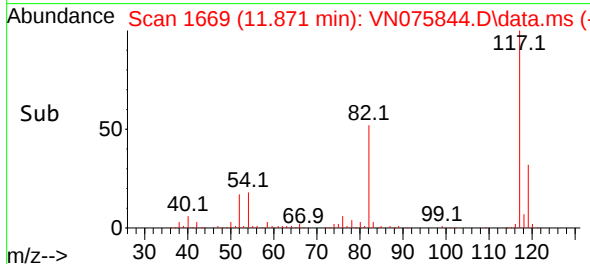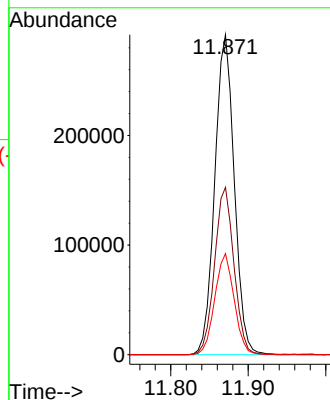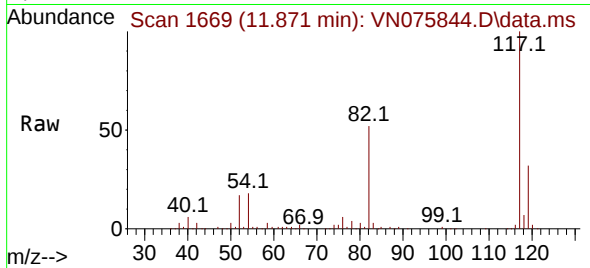

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075844.D
Acq: 16 Dec 2022 13:50

Tgt Ion:152 Resp: 205116
Ion Ratio Lower Upper
152 100
115 59.0 29.1 87.4
150 158.6 0.0 347.0

