

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121622\  
Data File : VN075853.D  
Acq On : 16 Dec 2022 17:26  
Operator : JC\MD  
Sample : N6107-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
COMP-SAMPLE-TANK-18-19-20-21-23

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M

Title : SW846 8260

Signal : TIC: VN075853.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.824       | 125           | 131         | 138          | rVB2     | 8006           | 18354         | 1.12%           | 0.216%        |
| 2         | 8.177       | 1030          | 1041        | 1045         | rBV      | 227852         | 543594        | 33.28%          | 6.403%        |
| 3         | 8.230       | 1045          | 1050        | 1066         | rVB      | 448102         | 998901        | 61.15%          | 11.766%       |
| 4         | 8.588       | 1100          | 1111        | 1121         | rBV      | 230972         | 516442        | 31.62%          | 6.083%        |
| 5         | 9.106       | 1190          | 1199        | 1213         | rBV      | 597431         | 1214113       | 74.33%          | 14.301%       |
| 6         | 10.571      | 1439          | 1448        | 1463         | rBV      | 893528         | 1633485       | 100.00%         | 19.240%       |
| 7         | 11.871      | 1660          | 1669        | 1683         | rBV      | 786732         | 1381579       | 84.58%          | 16.273%       |
| 8         | 12.853      | 1827          | 1836        | 1845         | rBV      | 584795         | 999892        | 61.21%          | 11.777%       |
| 9         | 13.794      | 1988          | 1996        | 2005         | rBV      | 707518         | 1183493       | 72.45%          | 13.940%       |




Sum of corrected areas: 8489853

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121622\  
Data File : VN075853.D  
Acq On : 16 Dec 2022 17:26  
Operator : JC\MD  
Sample : N6107-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
COMP-SAMPLE-TANK-18-19-20-21-23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

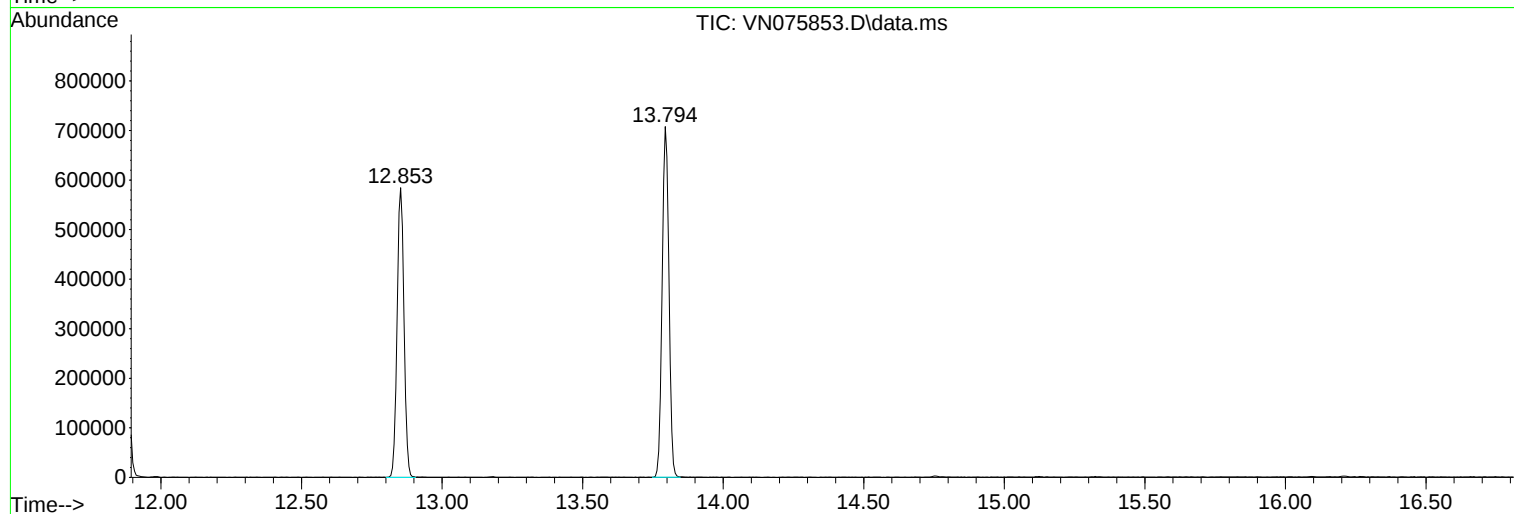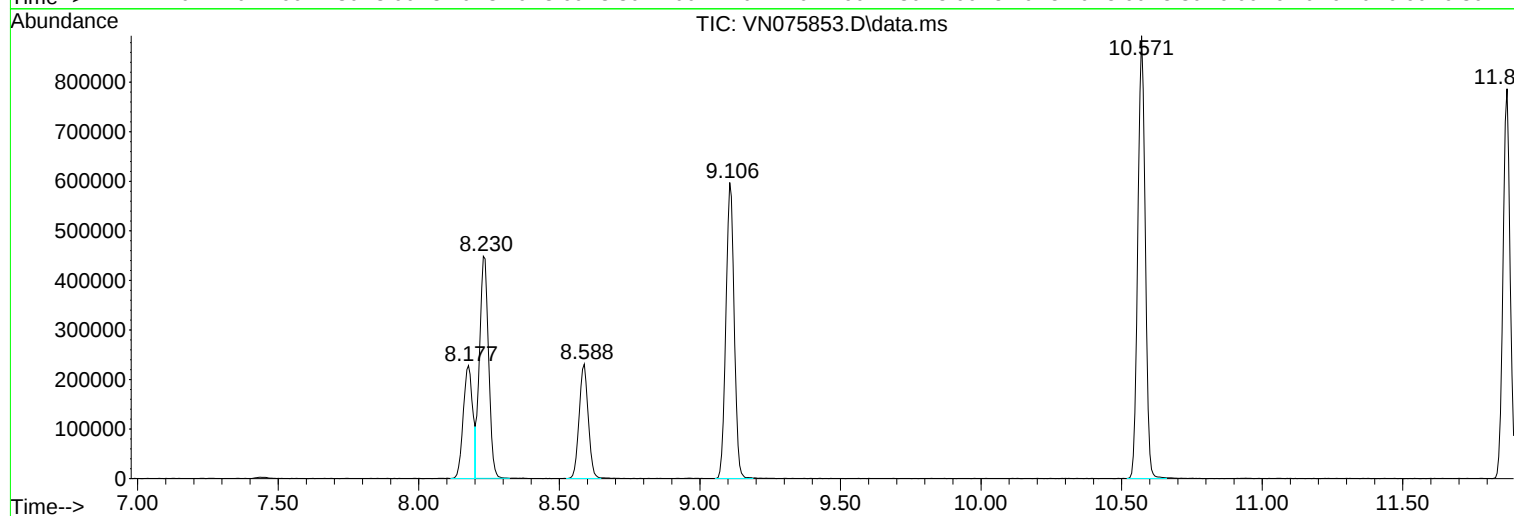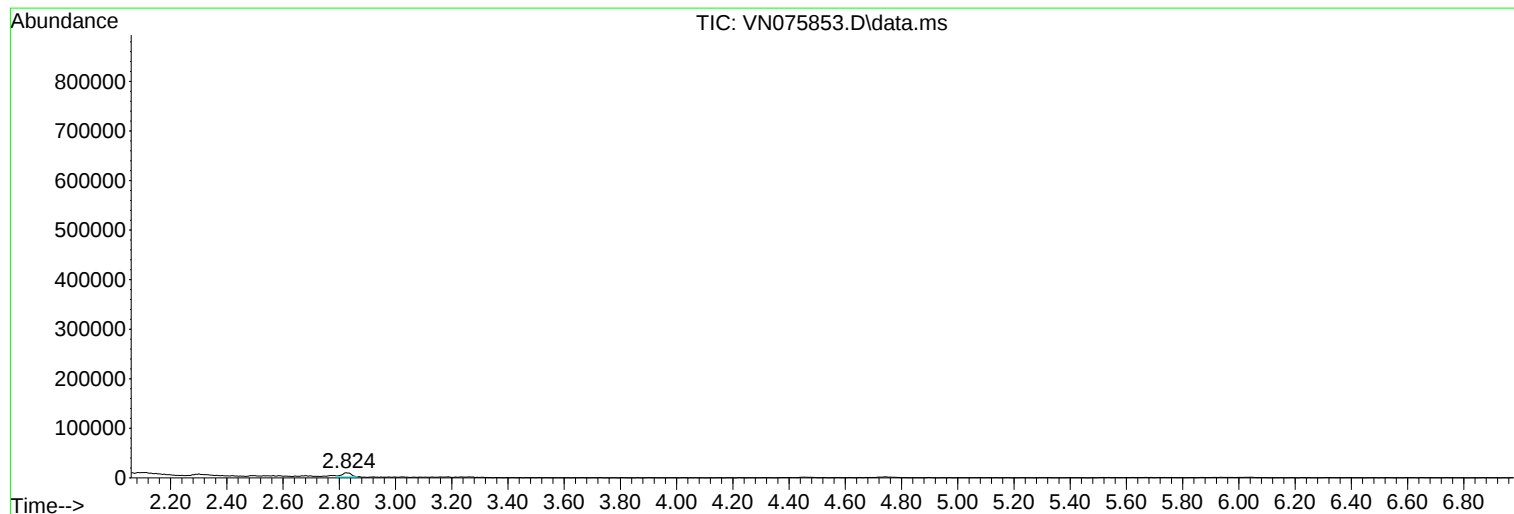

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121622\  
Data File : VN075853.D  
Acq On : 16 Dec 2022 17:26  
Operator : JC\MD  
Sample : N6107-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
COMP-SAMPLE-TANK-18-19-20-21-23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121622\  
Data File : VN075853.D  
Acq On : 16 Dec 2022 17:26  
Operator : JC\MD  
Sample : N6107-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
COMP-SAMPLE-TANK-18-19-20-21-23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |