

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
 Data File : VN075858.D
 Acq On : 16 Dec 2022 19:26
 Operator : JC\MD
 Sample : N6099-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PURGE-WATER-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260

Signal : TIC: VN075858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.830	127	132	139	rVB4	10717	26725	1.51%	0.249%
2	4.447	399	407	415	rBV2	6448	19103	1.08%	0.178%
3	7.971	998	1006	1017	rBV	132338	325055	18.41%	3.024%
4	8.177	1030	1041	1045	rBV	240187	575258	32.59%	5.351%
5	8.230	1045	1050	1060	rVB	481004	1073026	60.78%	9.982%
6	8.582	1099	1110	1123	rBV	241675	573120	32.47%	5.332%
7	9.106	1191	1199	1213	rBV	641312	1296246	73.43%	12.059%
8	9.359	1233	1242	1254	rBV	247521	502601	28.47%	4.676%
9	9.888	1326	1332	1342	rBV	28607	56849	3.22%	0.529%
10	10.571	1440	1448	1455	rBV	955860	1765345	100.00%	16.422%
11	10.635	1457	1459	1466	rVB	18938	28342	1.61%	0.264%
12	11.106	1532	1539	1546	rBV2	22244	41375	2.34%	0.385%
13	11.870	1661	1669	1678	rVB	825771	1502497	85.11%	13.977%
14	12.523	1765	1780	1781	rBV2	39757	105018	5.95%	0.977%
15	12.853	1828	1836	1846	rVB	674364	1151533	65.23%	10.712%
16	13.635	1959	1969	1973	rBV7	14696	51281	2.90%	0.477%
17	13.794	1989	1996	2006	rVB	798443	1343797	76.12%	12.501%
18	14.035	2025	2037	2049	rBV9	33069	145267	8.23%	1.351%
19	14.147	2052	2056	2072	rVB10	19560	69421	3.93%	0.646%
20	14.576	2117	2129	2138	rBV10	14905	55192	3.13%	0.513%
21	15.211	2231	2237	2248	rBV6	8756	21944	1.24%	0.204%
22	16.505	2453	2457	2466	rVB5	9515	20594	1.17%	0.192%




Sum of corrected areas: 10749589

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
Data File : VN075858.D
Acq On : 16 Dec 2022 19:26
Operator : JC\MD
Sample : N6099-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

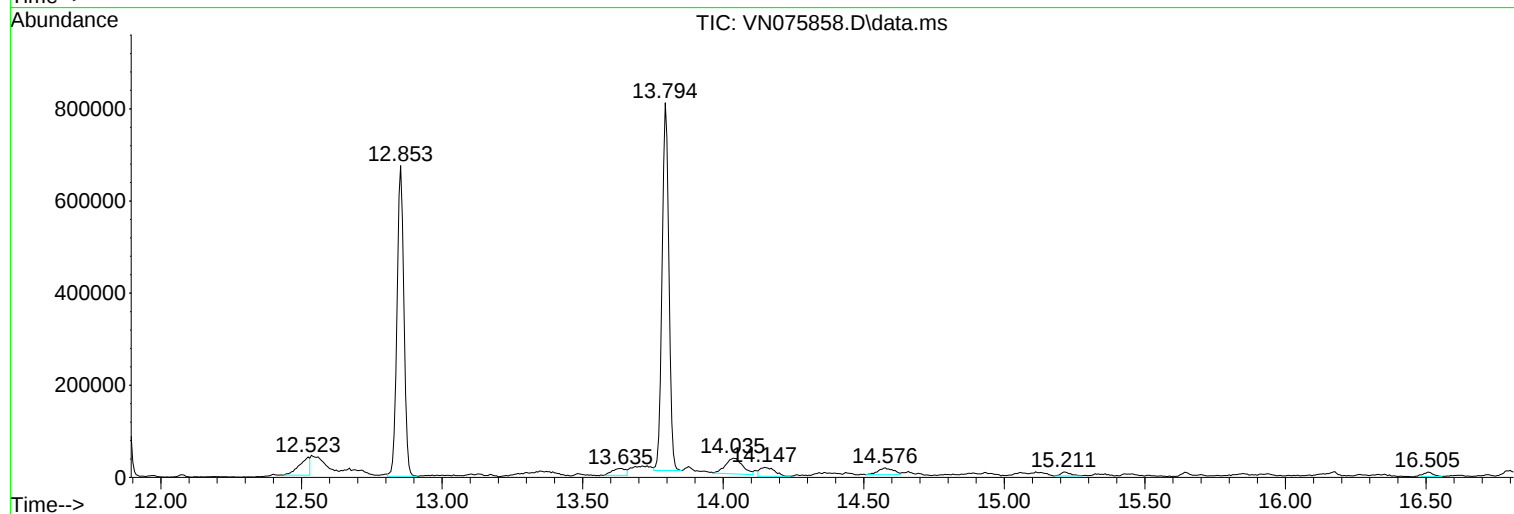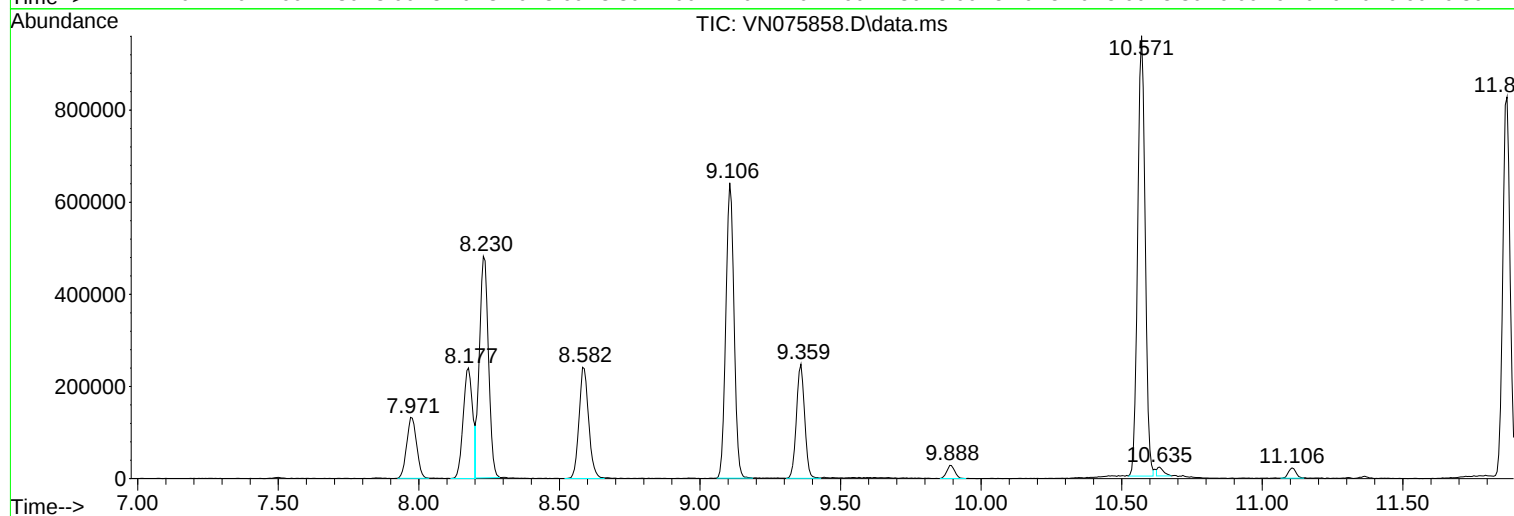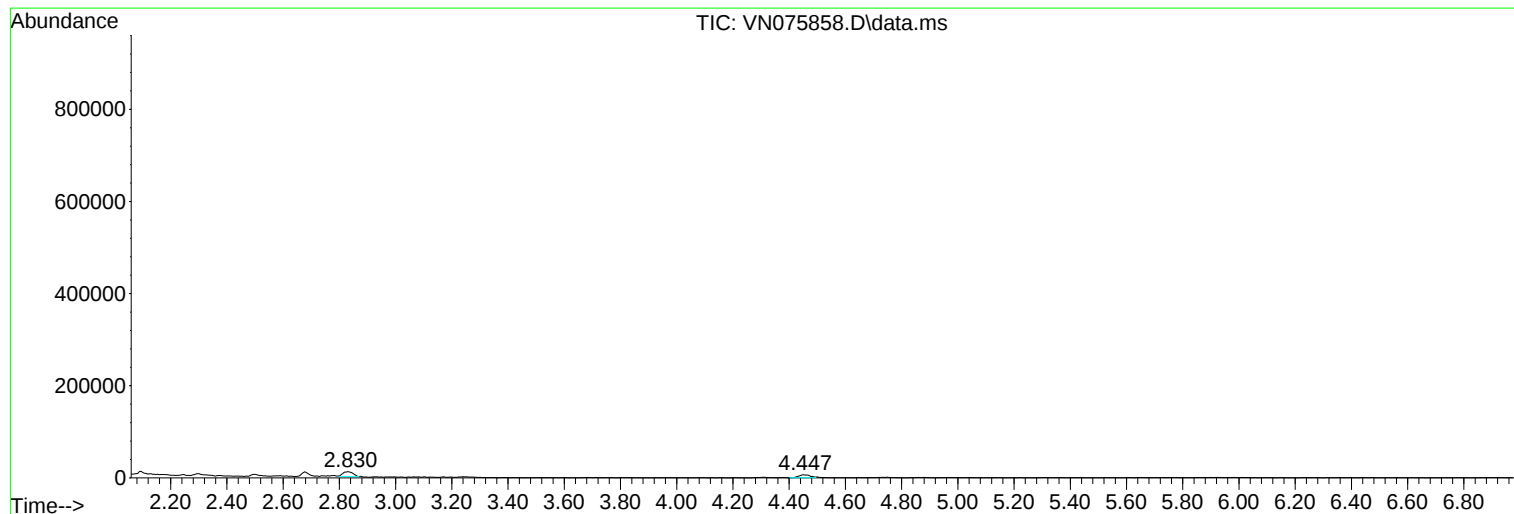

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
Data File : VN075858.D
Acq On : 16 Dec 2022 19:26
Operator : JC\MD
Sample : N6099-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER-2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 1,7-dimethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.035	5.41 ug/l	145267	1,4-Dichlorobenzene-d4	13.794

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 1,7-dimethyl-	156	C12H12	000575-37-1	96
2			Naphthalene, 1,6-dimethyl-	156	C12H12	000575-43-9	96
3			Naphthalene, 1,5-dimethyl-	156	C12H12	000571-61-9	95
4			Naphthalene, 2,6-dimethyl-	156	C12H12	000581-42-0	95
5			Naphthalene, 1,8-dimethyl-	156	C12H12	000569-41-5	94

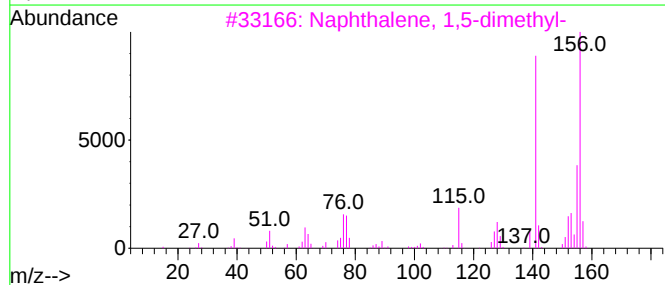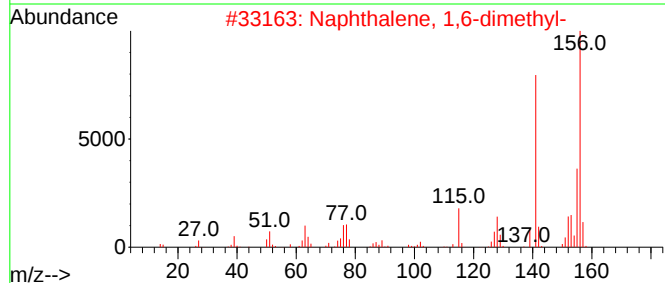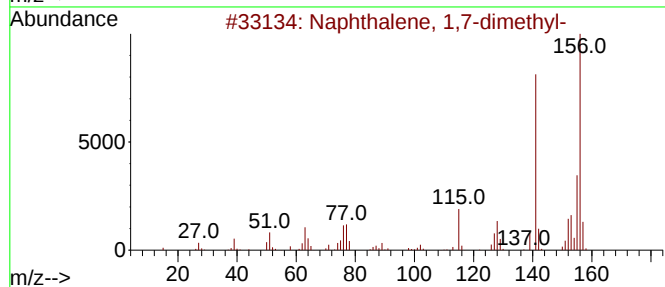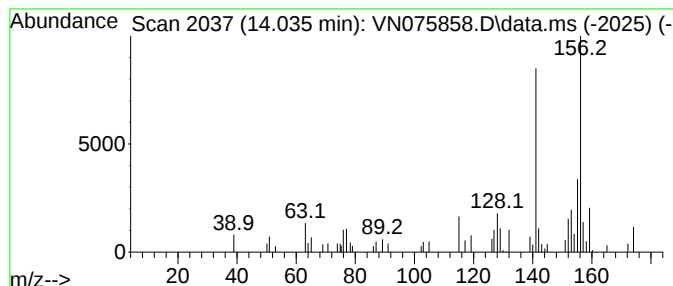

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
Data File : VN075858.D
Acq On : 16 Dec 2022 19:26
Operator : JC\MD
Sample : N6099-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PURGE-WATER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 1,...	14.035	5.4	ug/l	145267	4	13.794	1343800	50.0