
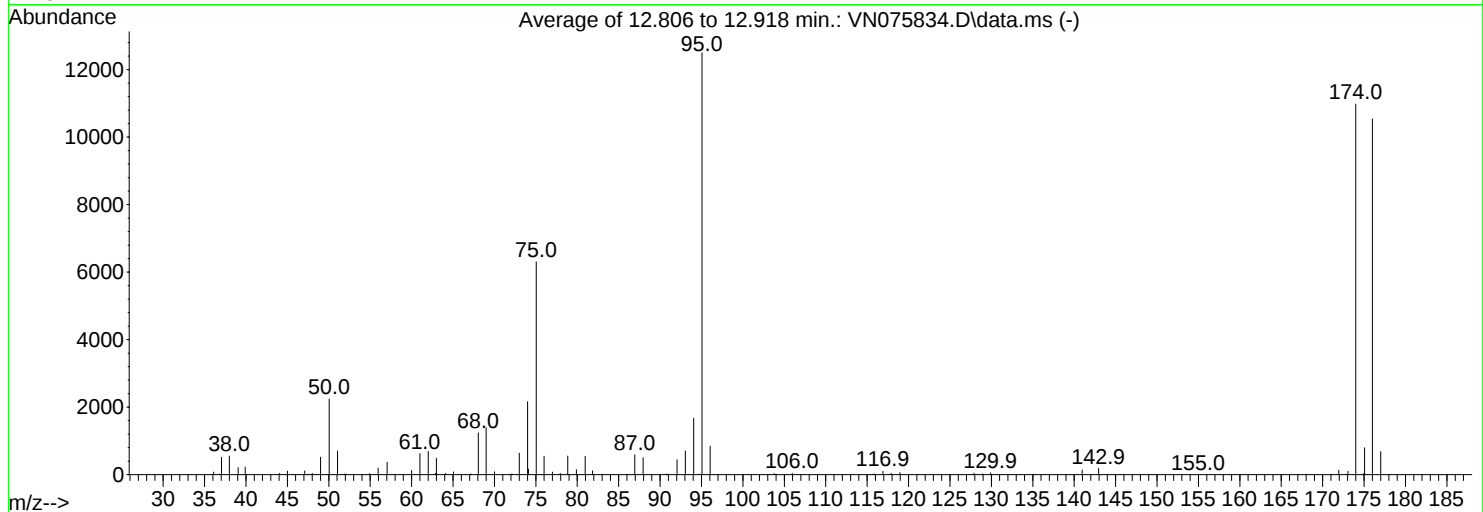


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121622\
 Data File : VN075834.D
 Acq On : 16 Dec 2022 09:19
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

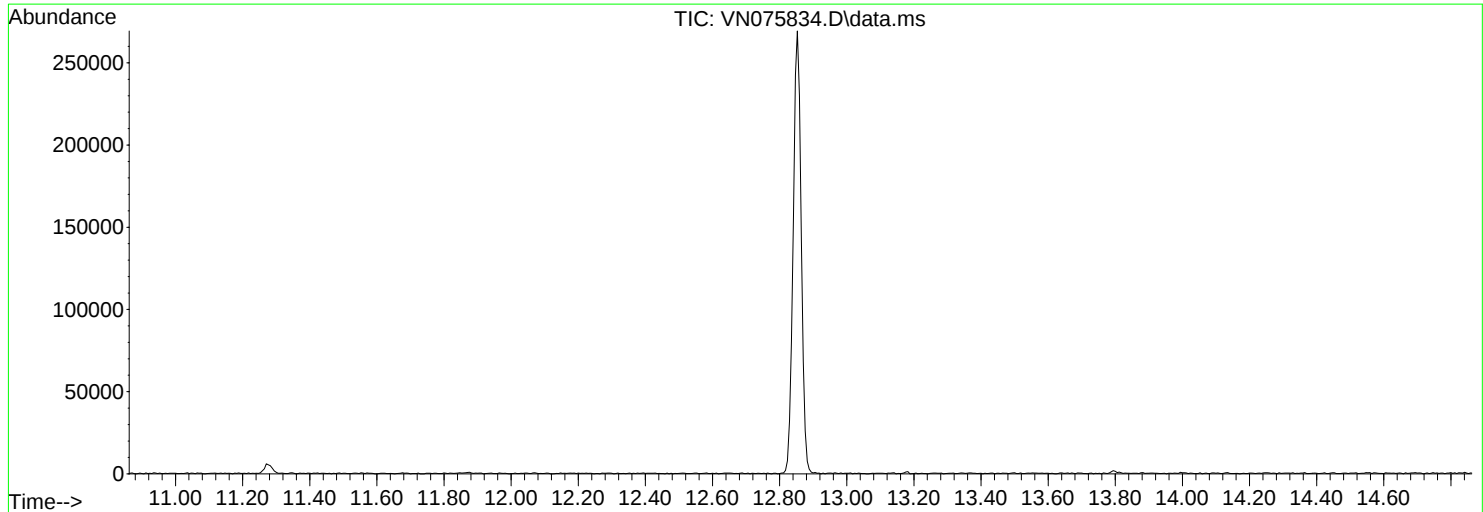

AutoFind: Averaged scan 1828 to 1847; Bkg corrected with scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	2243	PASS
75	95	30	60	50.5	6305	PASS
95	95	100	100	100.0	12496	PASS
96	95	5	9	6.7	842	PASS
173	174	0.00	2	0.9	99	PASS
174	95	50	100	87.9	10980	PASS
175	174	5	9	7.2	795	PASS
176	174	95	101	96.0	10544	PASS
177	176	5	9	6.5	684	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	8	47.10	108	57.05	365	70.00	8
36.10	78	47.50	12	60.00	122	71.80	1
36.80	19	47.90	13	61.00	624	72.10	2
37.05	519	48.05	34	62.00	689	73.00	63
38.00	552	49.00	517	62.90	39	74.00	2161
39.05	211	50.05	2243	63.00	486	74.10	167
39.90	225	51.05	699	64.10	36	75.05	6305
40.10	9	51.90	19	65.05	83	76.00	545
44.05	38	52.10	12	67.15	26	77.00	76
45.00	103	54.90	27	68.05	1238	77.60	11
45.80	8	55.95	196	69.00	1390	77.95	36

Average of 12.806 to 12.918 min.: VN075834.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.85	552	94.05	1673	118.95	63	171.95	134
79.90	146	94.80	15	127.90	43	172.80	16
80.95	542	95.05	12496	128.95	25	172.90	9
81.85	112	96.05	842	129.90	51	173.05	99
86.00	11	103.75	34	135.10	11	174.00	10980
86.95	586	104.00	16	140.95	139	174.90	29
87.95	501	105.95	38	142.95	183	175.05	795
90.75	21	115.70	8	144.90	11	176.00	10544
91.00	21	115.85	26	147.90	8	177.00	684
92.05	442	116.90	102	155.00	8	178.00	8
93.05	704	117.90	44	171.10	8		

Instrument :

MSVOA_N

ClientSampleId :

BFB