

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN121718\
 Data File : VN052936.D
 Acq On : 17 Dec 2018 19:11
 Operator : MD\SY
 Sample : PB115729ZHE#06
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115729ZHE#06

Quant Time: Dec 18 06:15:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121218W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 13 01:08:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1347583	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	2098945	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1903493	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	768570	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	691367	48.25	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.50%	
35) Dibromofluoromethane	7.59	113	453103	38.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	77.34%	
50) Toluene-d8	10.09	98	2583109	50.85	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.70%	
62) 4-Bromofluorobenzene	12.40	95	865770	50.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.60%	
Target Compounds						
16) Acetone	3.82	43	22098	6.867	ug/l	92
20) Methylene Chloride	4.55	84	25400	1.754	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN121718\
Data File : VN052936.D
Acq On : 17 Dec 2018 19:11
Operator : MD\SY
Sample : PB115729ZHE#06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB115729ZHE#06

Quant Time: Dec 18 06:15:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121218W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 13 01:08:35 2018
Response via : Initial Calibration

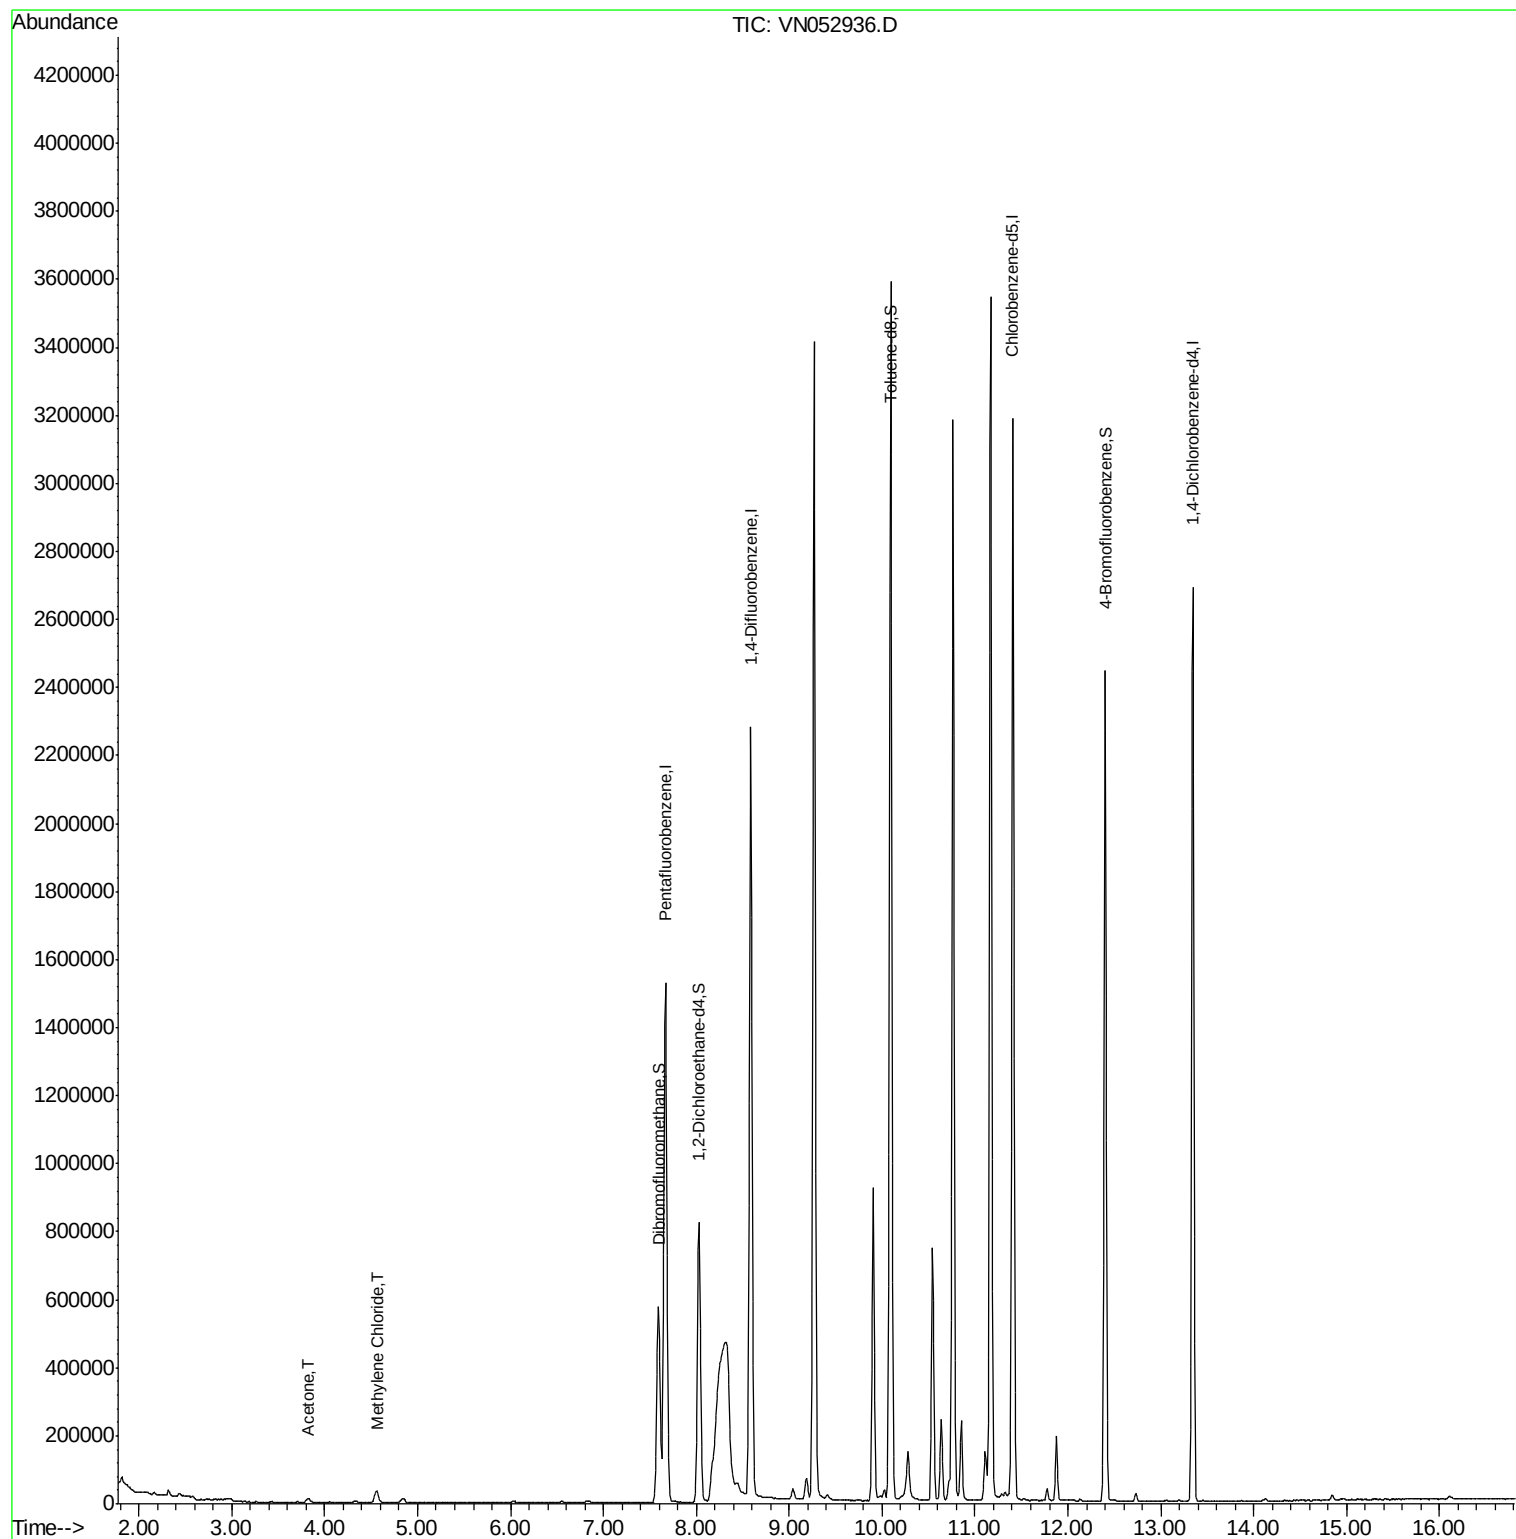

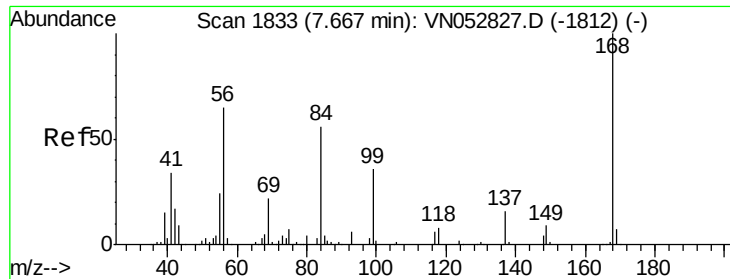

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN052936.D

Acq: 17 Dec 2018 19:11

Instrument :

MSVOA_N

ClientSampleId :


PB115729ZHE#06

Tgt Ion:168 Resp: 1347583

Ion Ratio Lower Upper

168 100

99 50.2 40.2 60.2

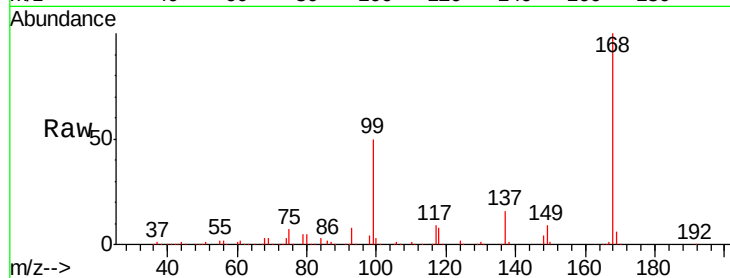

Abundance Ion 167.90 (167.60 to 168.60): VN052827.D (-1812) (-)

Ion 98.90 (98.60 to 99.60): VN052827.D (-1812) (-)

7.67

600000

500000

400000



300000

200000

100000

0

Time-->

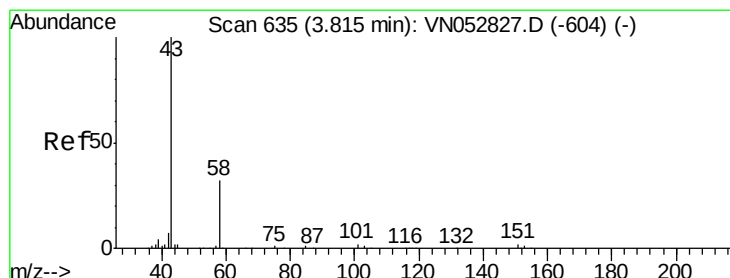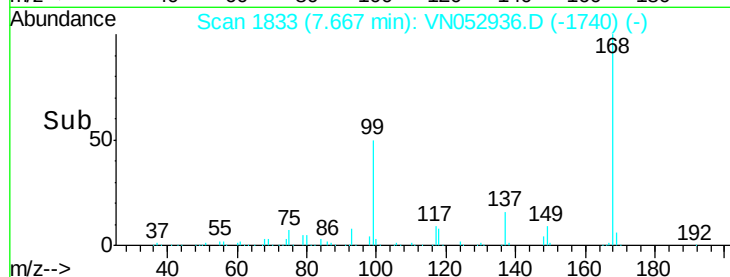

#16

Acetone

Concen: 6.867 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.00 min

Lab File: VN052936.D


Acq: 17 Dec 2018 19:11

Tgt Ion: 43 Resp: 22098

Ion Ratio Lower Upper

43 100

58 36.0 25.4 38.0

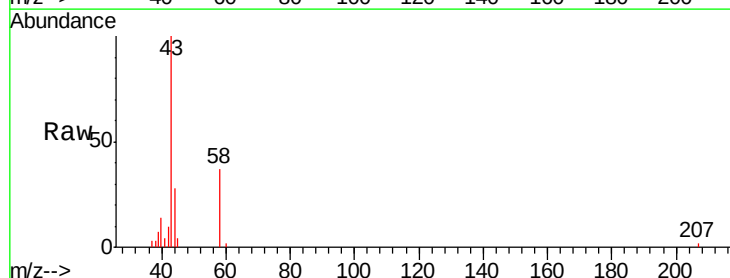

Abundance Ion 43.00 (42.70 to 43.70): VN052827.D (-604) (-)

Ion 58.00 (57.70 to 58.70): VN052827.D (-604) (-)

3.82

8000


6000


4000

2000

0

Time-->




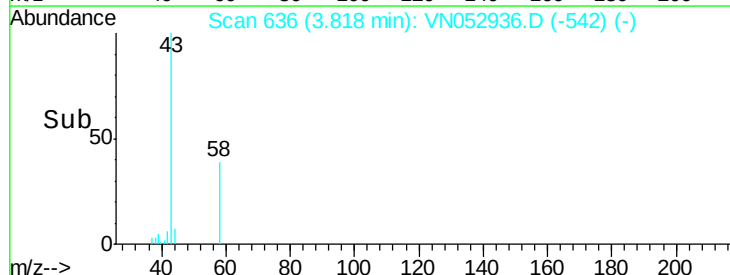


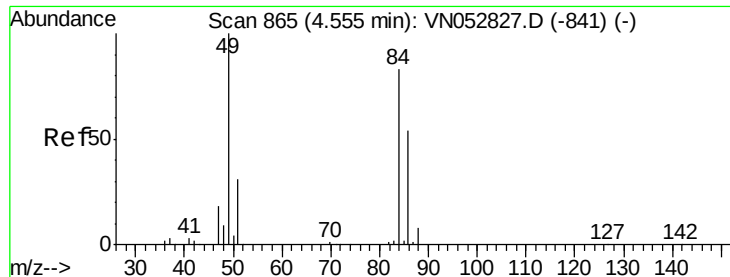

#20
Methylene Chloride
Concen: 1.754 ug/l
RT: 4.55 min Scan# 865
Delta R.T. 0.00 min
Lab File: VN052936.D
Acq: 17 Dec 2018 19:11




Instrument :
MSVOA_N
ClientSampleId :
PB115729ZHE#06


Tgt Ion: 84 Resp: 25400
Ion Ratio Lower Upper
84 100
49 118.7 96.8 145.2
51 34.8 29.9 44.9
86 61.7 51.8 77.6

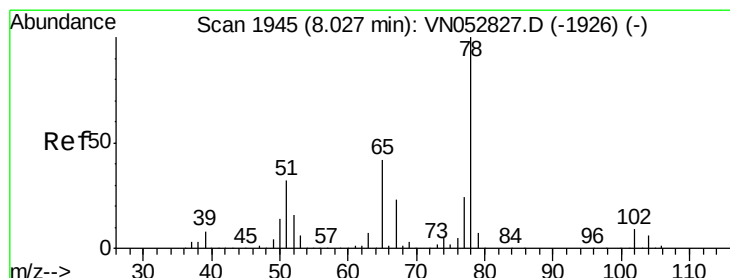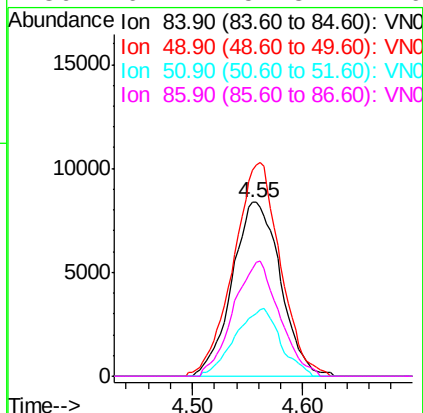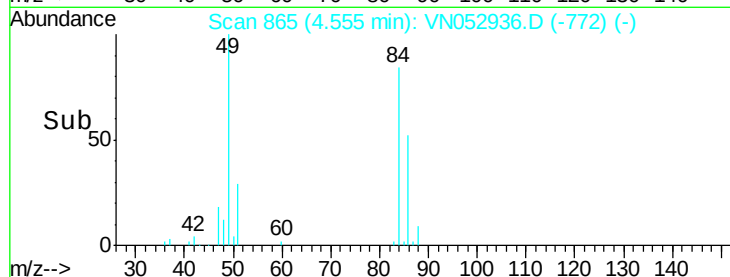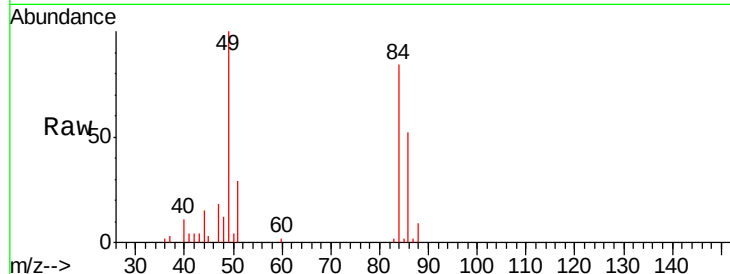

#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN052936.D
Acq: 17 Dec 2018 19:11

Tgt Ion: 65 Resp: 691367
Ion Ratio Lower Upper
65 100
67 54.7 0.0 110.4

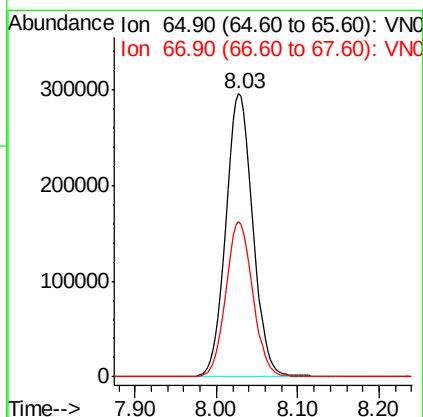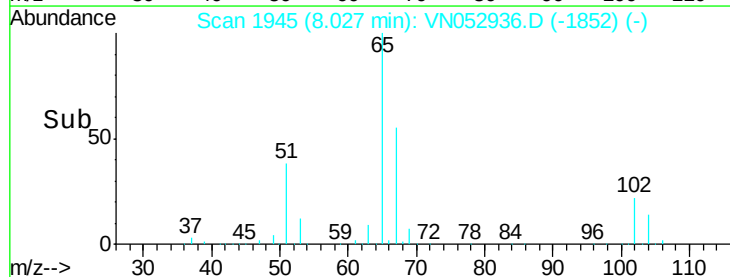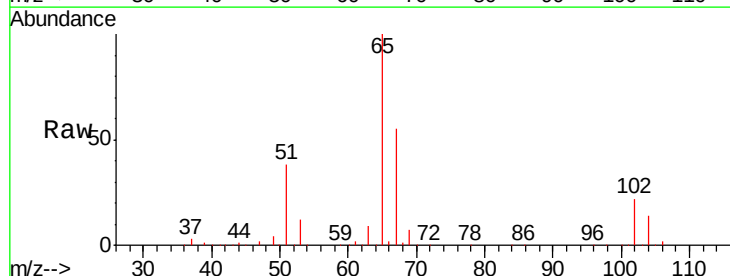


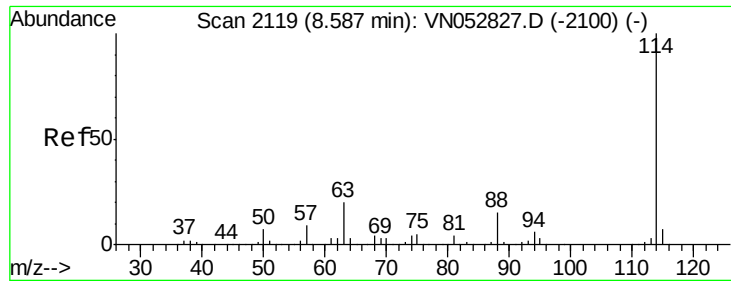




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN052936.D
 Acq: 17 Dec 2018 19:11

Instrument :
 MSVOA_N
 ClientSampleId :
 PB115729ZHE#06

Tgt Ion:114 Resp: 2098945
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 39.8
 88 15.3 0.0 31.0

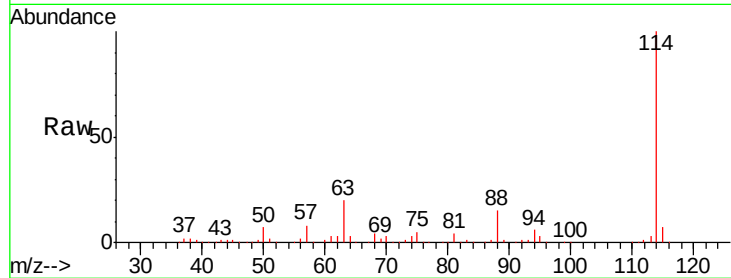


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

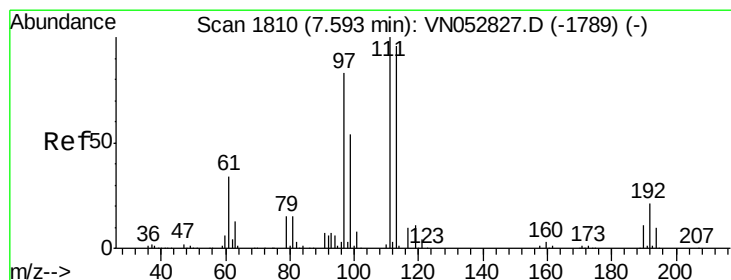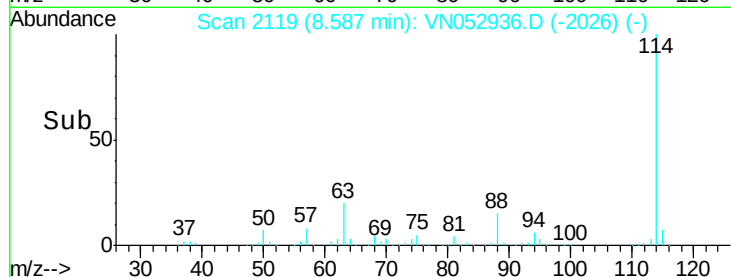
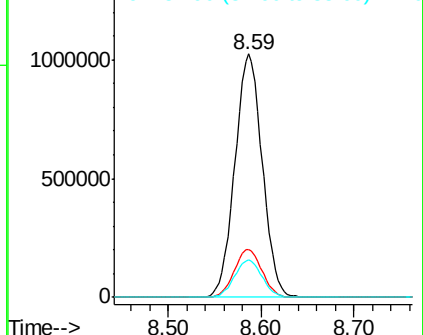



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN052936.D
 Acq: 17 Dec 2018 19:11

Tgt Ion:113 Resp: 453103
 Ion Ratio Lower Upper
 113 100
 111 101.2 83.0 124.4
 192 22.5 17.5 26.3

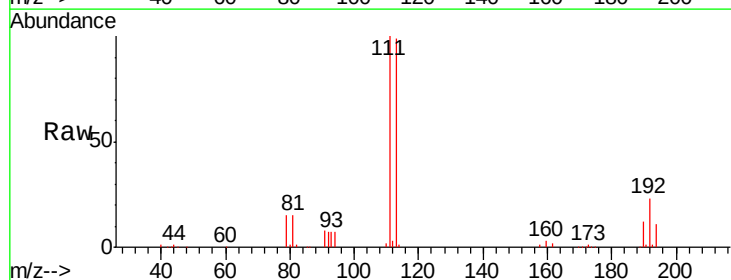

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

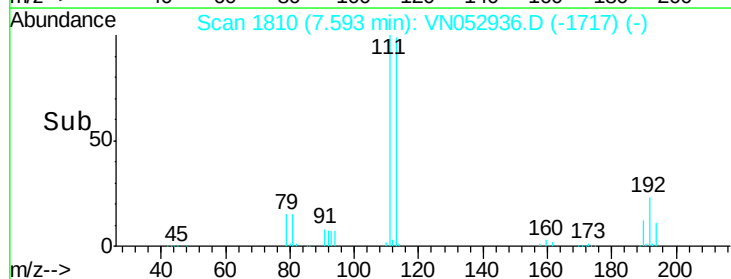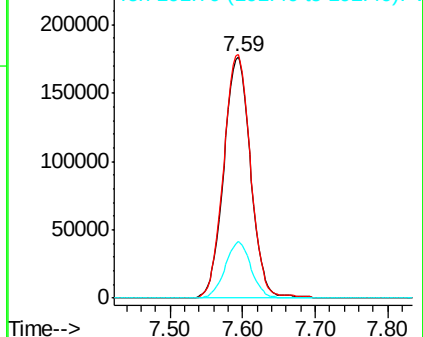

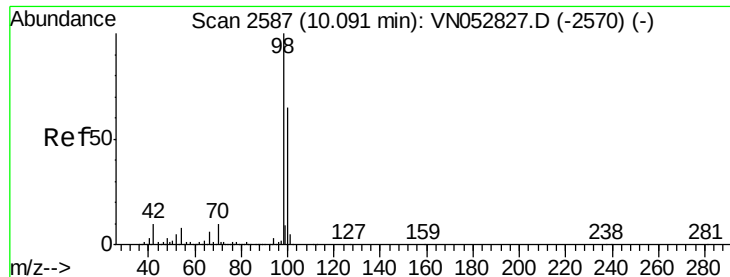

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN052936.D

Acq: 17 Dec 2018 19:11

Instrument :

MSVOA_N

ClientSampleId :


PB115729ZHE#06

Tgt Ion: 98 Resp: 2583109

Ion Ratio Lower Upper




98 100

100 64.0 51.6 77.4

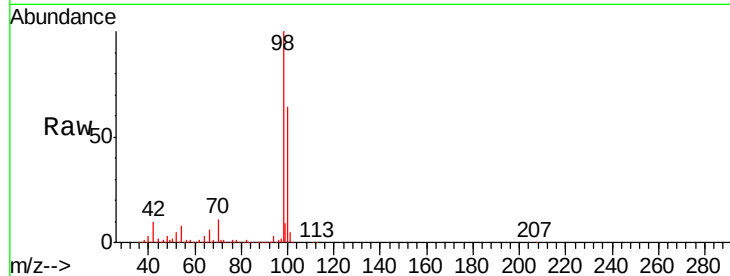

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

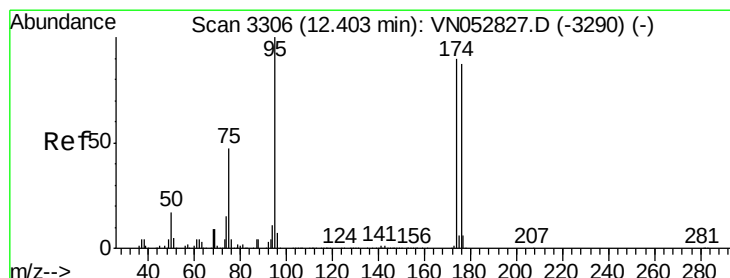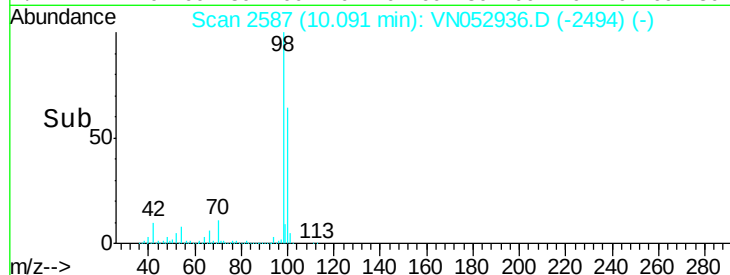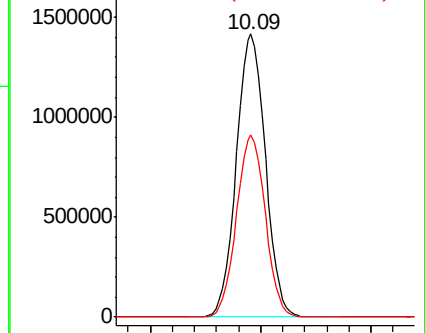

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN052936.D

Acq: 17 Dec 2018 19:11


Tgt Ion: 95 Resp: 865770

Ion Ratio Lower Upper

95 100

174 88.3 0.0 178.8



176 85.7 0.0 173.8

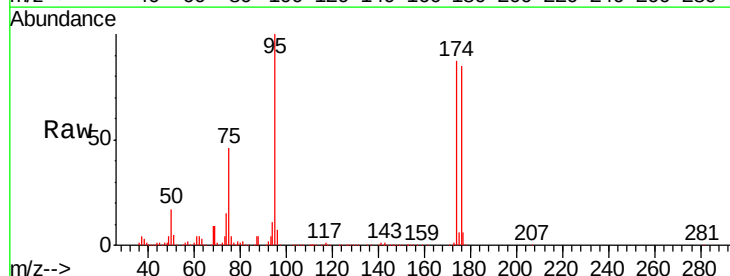


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

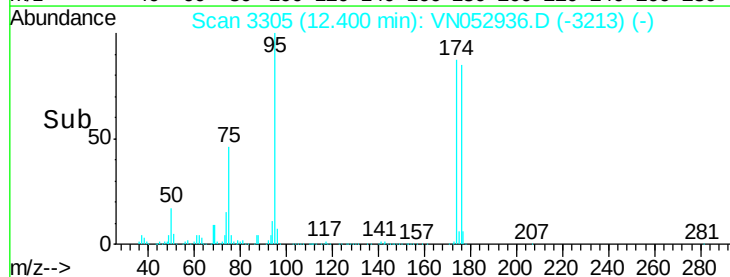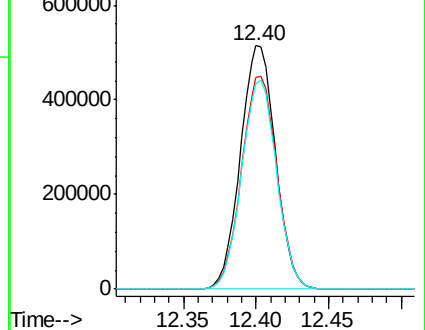


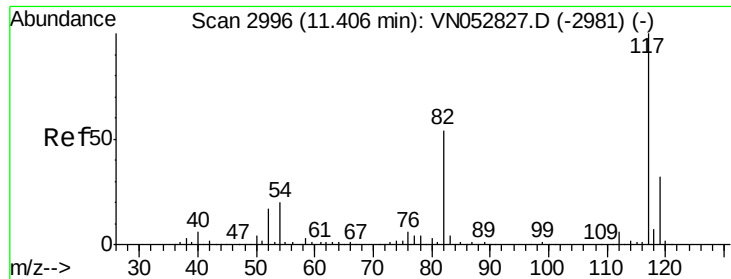




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN052936.D
Acq: 17 Dec 2018 19:11

Instrument :
MSVOA_N
ClientSampleId :
PB115729ZHE#06

Tgt Ion:117 Resp: 1903493
Ion Ratio Lower Upper
117 100
82 53.8 42.8 64.2
119 32.2 25.5 38.3

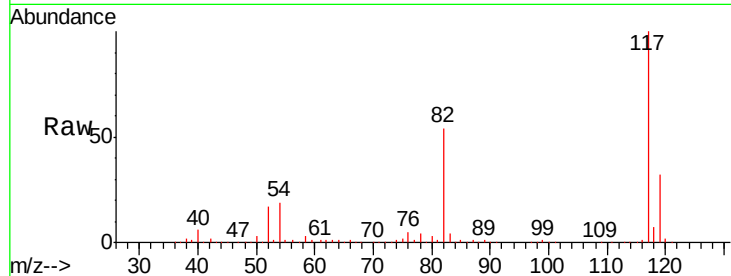


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

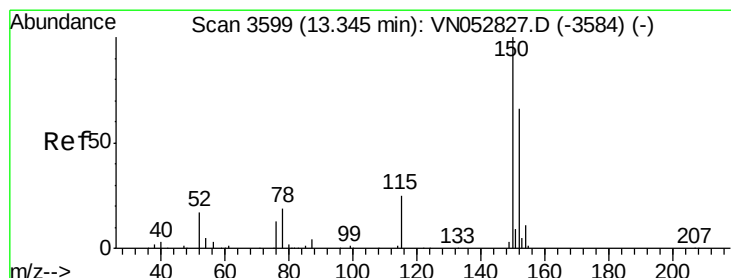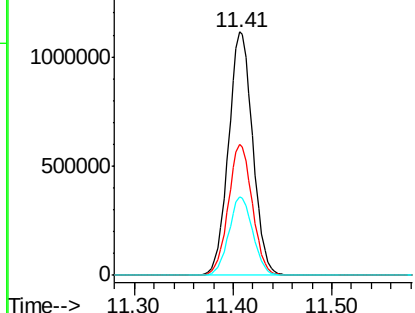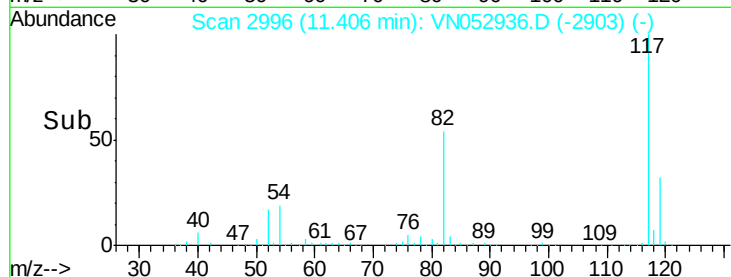

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN052936.D
Acq: 17 Dec 2018 19:11

Tgt Ion:152 Resp: 768570
Ion Ratio Lower Upper
152 100
115 56.8 28.3 85.0
150 158.4 0.0 347.8

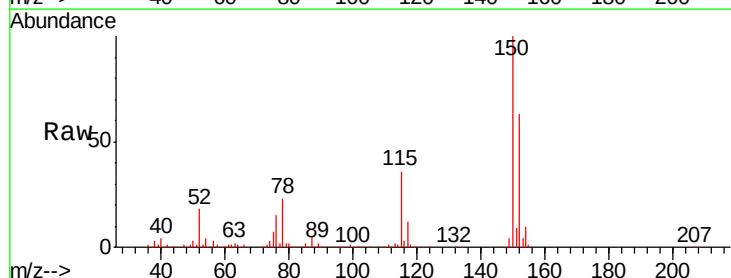

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

