


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121718\
 Data File : VN052914.D
 Acq On : 17 Dec 2018 8:59
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121218W.M
 Title : SW846 8260
 Last Update : Thu Dec 13 01:08:35 2018

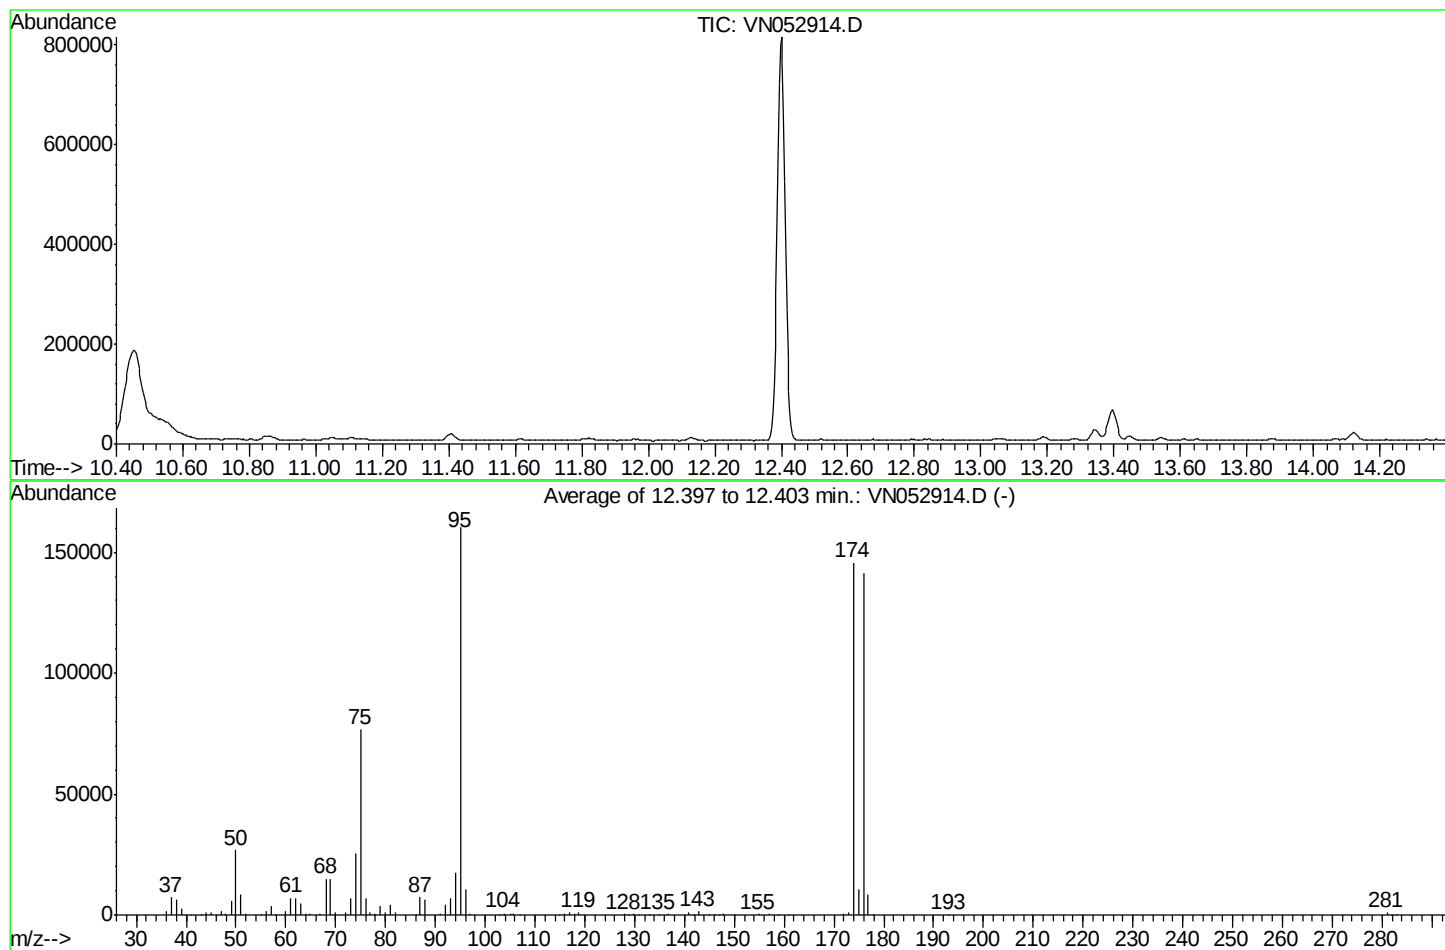

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	26760	PASS
75	95	30	60	47.9	76717	PASS
95	95	100	100	100.0	160298	PASS
96	95	5	9	6.7	10819	PASS
173	174	0.00	2	0.7	1053	PASS
174	95	50	100	90.9	145706	PASS
175	174	5	9	7.3	10580	PASS
176	174	95	101	97.0	141269	PASS
177	176	5	9	5.9	8372	PASS