


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121718\
Data File : VN052941.D
Acq On : 17 Dec 2018 21:25
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121218W.M
Title : SW846 8260
Last Update : Thu Dec 13 01:08:35 2018

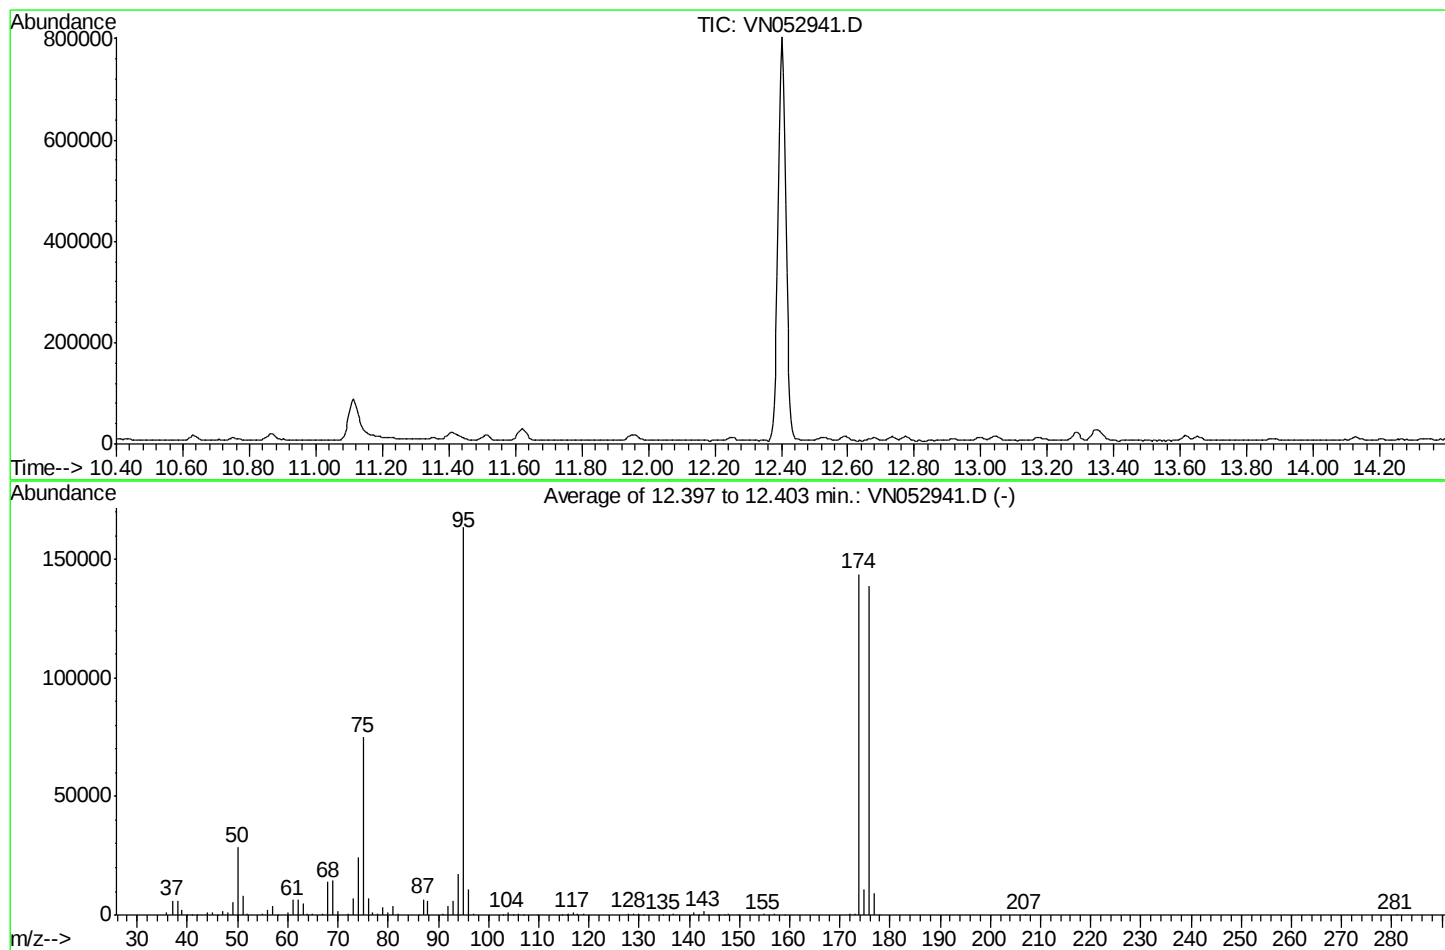

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	28389	PASS
75	95	30	60	45.8	74973	PASS
95	95	100	100	100.0	163605	PASS
96	95	5	9	6.6	10737	PASS
173	174	0.00	2	0.3	395	PASS
174	95	50	100	87.8	143701	PASS
175	174	5	9	7.4	10648	PASS
176	174	95	101	96.6	138792	PASS
177	176	5	9	6.5	9019	PASS