

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN121719\
 Data File : VN059621.D
 Acq On : 17 Dec 2019 13:38
 Operator : JC/SP
 Sample : VN1217WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1217WBL01

Quant Time: Dec 18 06:00:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 13 23:17:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	228714	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	364856	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	321255	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	123042	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	165660	49.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.56%	
35) Dibromofluoromethane	7.57	113	116680	51.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.22%	
50) Toluene-d8	10.08	98	450466	49.84	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.68%	
62) 4-Bromofluorobenzene	12.40	95	144173	43.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.44%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN121719\
Data File : VN059621.D
Acq On : 17 Dec 2019 13:38
Operator : JC/SP
Sample : VN1217WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1217WBL01

Quant Time: Dec 18 06:00:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 13 23:17:39 2019
Response via : Initial Calibration

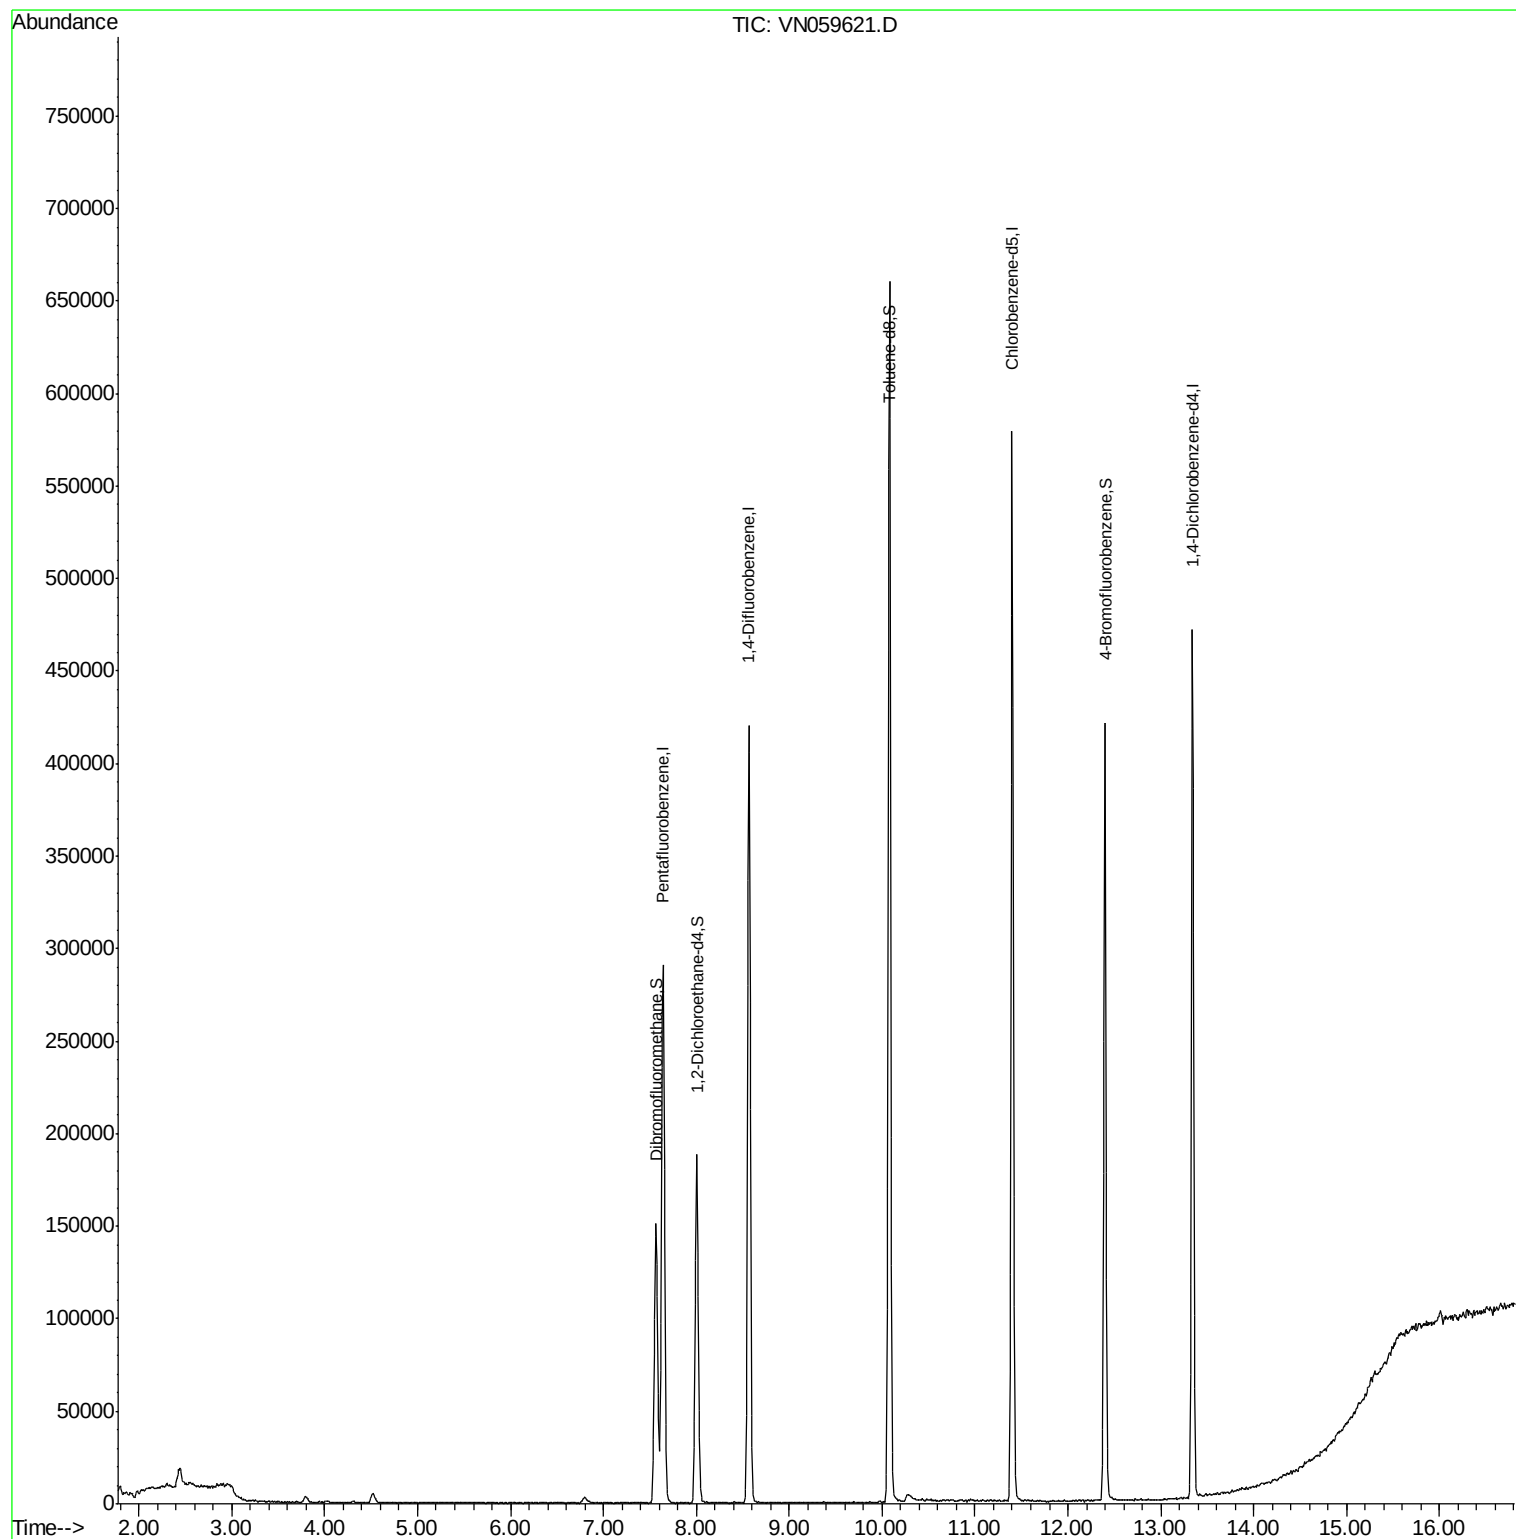

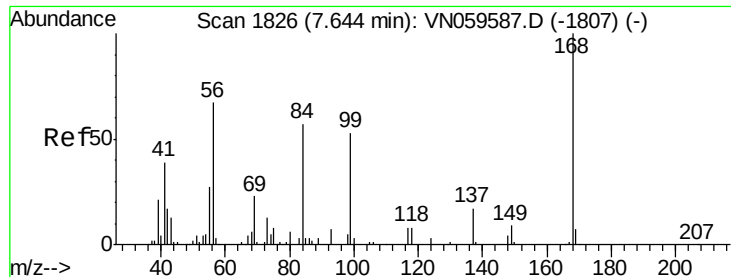

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.00 min

Lab File: VN059621.D

Acq: 17 Dec 2019 13:38

Instrument :

MSVOA_N

ClientSampled :


VN1217WBL01

Tot Ion:168 Resp: 228714

Ion Ratio Lower Upper

168 100

99 59.4 48.2 72.4

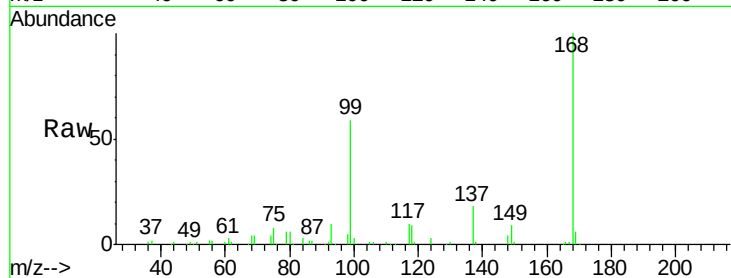

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.64

100000

80000

60000


40000

20000


0

7.60

7.70

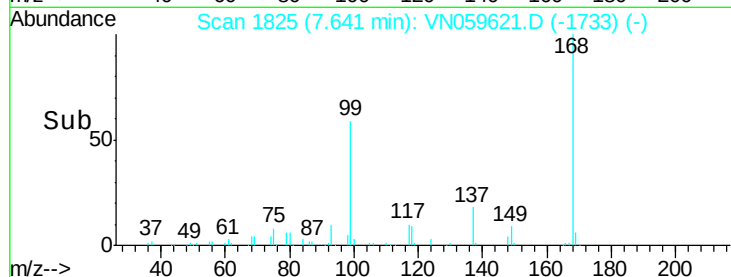

Time-->

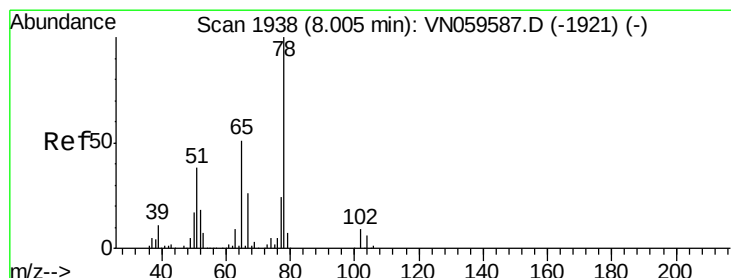

#33

1,2-Dichloroethane-d4

Concen: 49.776 ug/l

RT: 8.00 min Scan# 1938

Delta R.T. 0.00 min

Lab File: VN059621.D


Acq: 17 Dec 2019 13:38

Tgt Ion: 65 Resp: 165660

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.0

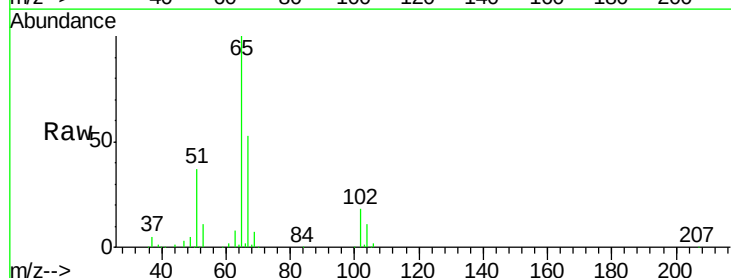

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

8.00

80000

60000


40000

20000


0

7.90

8.10

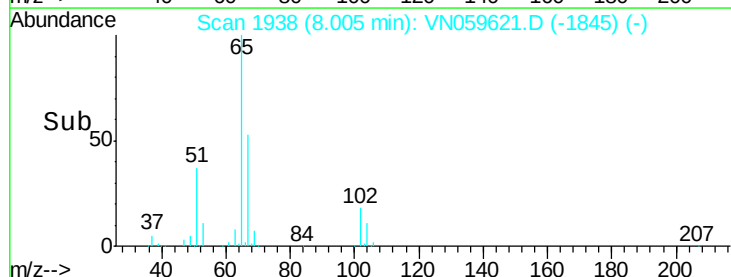


Time-->

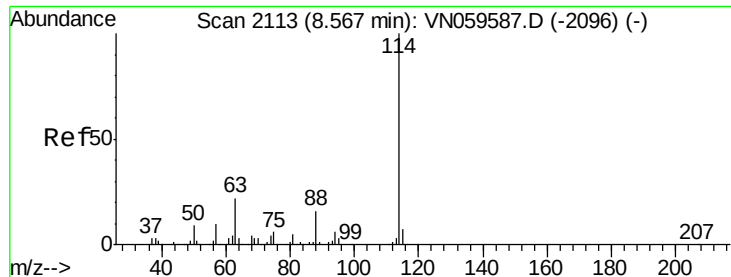




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN059621.D
 Acq: 17 Dec 2019 13:38

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1217WBL01

Tot Ion	Ratio	Lower	Upper
114	100		
63	22.6	0.0	43.6
88	16.0	0.0	31.4

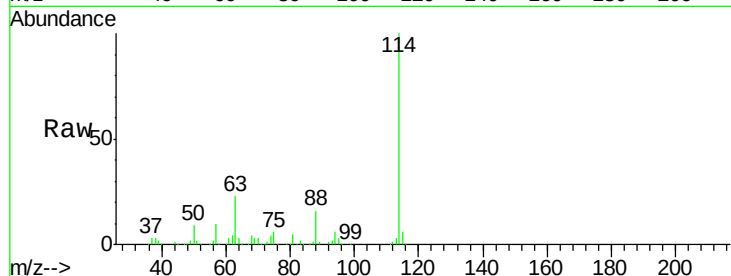


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

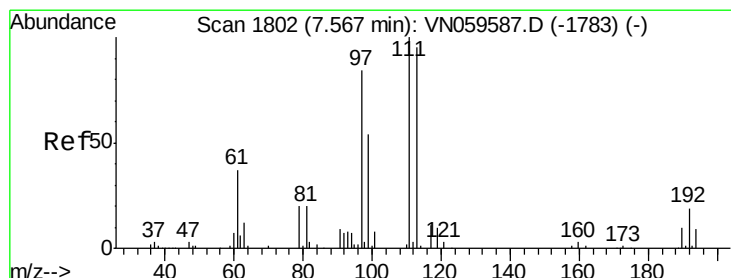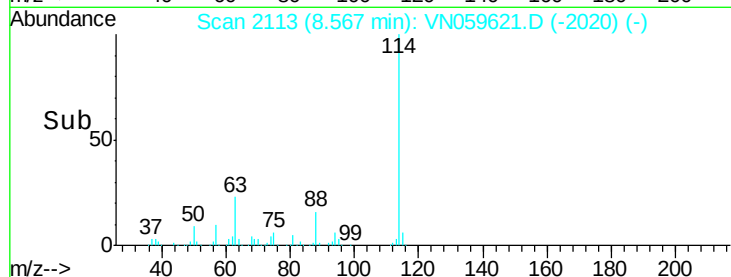
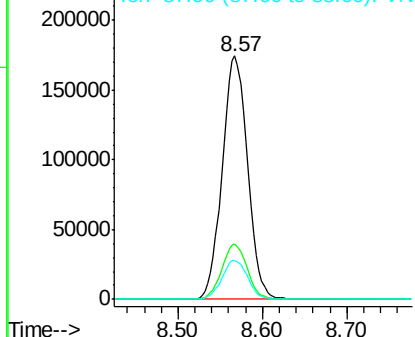



#35
 Dibromofluoromethane
 Concen: 51.111 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN059621.D
 Acq: 17 Dec 2019 13:38

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.4	83.5	125.3
192	18.8	15.4	23.2

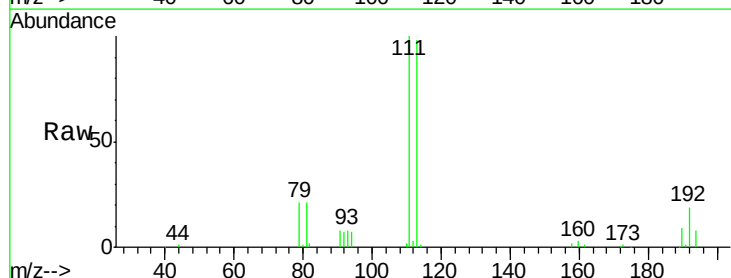

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



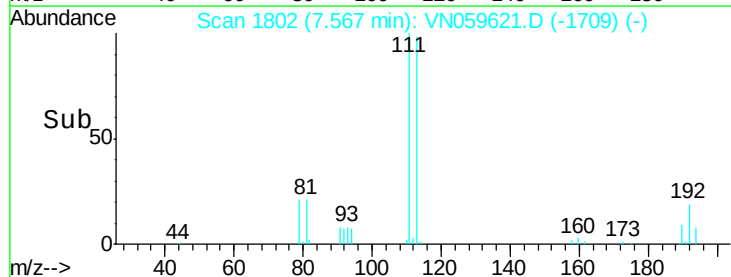
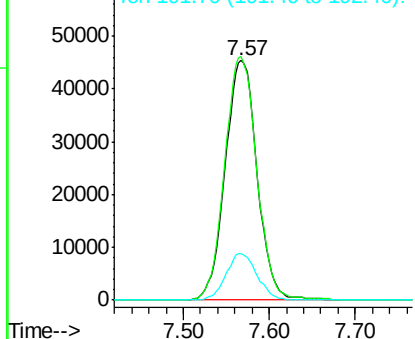


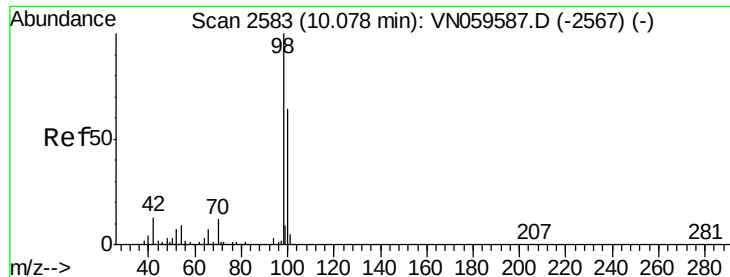

#50
Toluene-d8
Concen: 49.840 ug/l
RT: 10.08 min Scan# 2583
Delta R.T. 0.00 min
Lab File: VN059621.D
Acq: 17 Dec 2019 13:38




Instrument :
MSVOA_N
ClientSampled :
VN1217WBL01


Tot Ion: 98 Resp: 450466
Ion Ratio Lower Upper
98 100
100 63.1 51.2 76.8

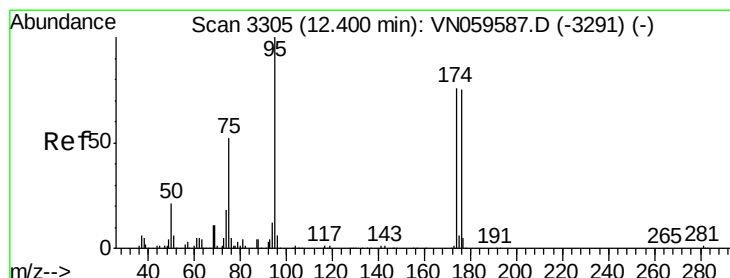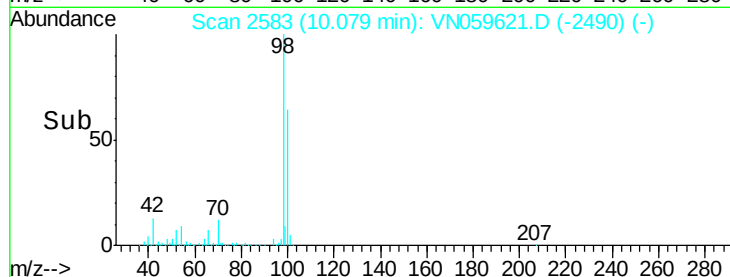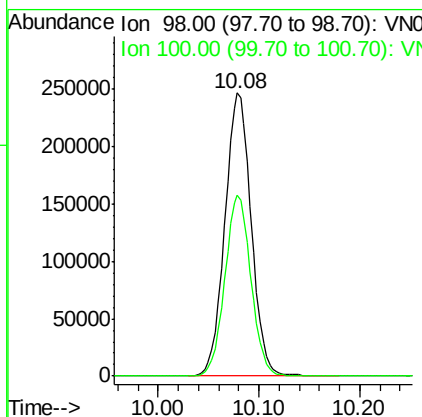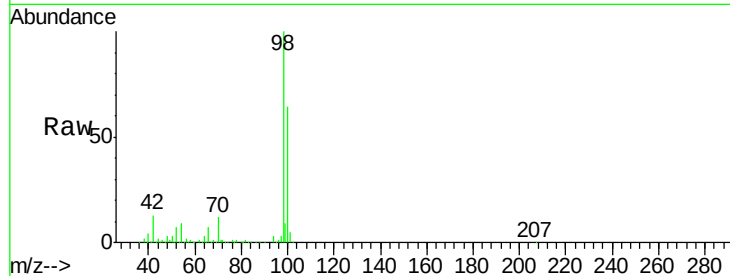

#62
4-Bromofluorobenzene
Concen: 43.716 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. -0.00 min
Lab File: VN059621.D
Acq: 17 Dec 2019 13:38

Tgt Ion: 95 Resp: 144173
Ion Ratio Lower Upper
95 100
174 76.7 0.0 151.4
176 73.6 0.0 146.0

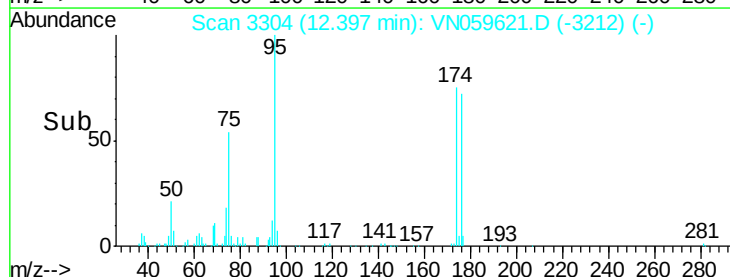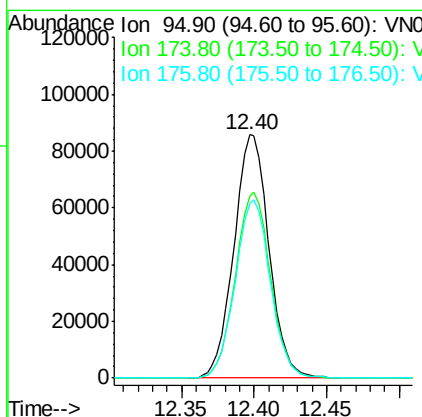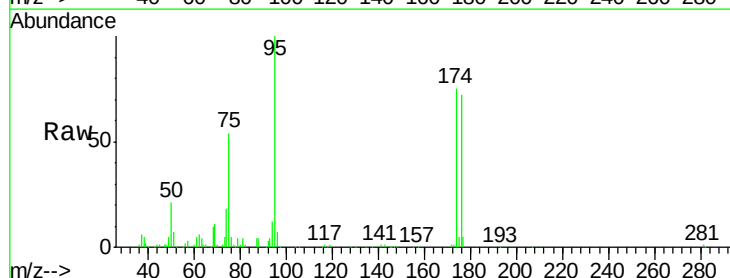

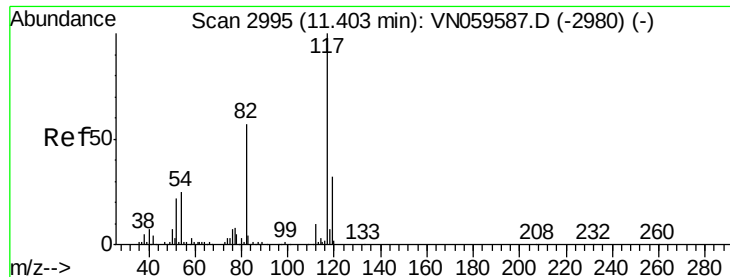

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2994

Delta R.T. -0.00 min

Lab File: VN059621.D

Acq: 17 Dec 2019 13:38

Instrument :

MSVOA_N

ClientSampleId :

VN1217WBL01


Tot Ion:117 Resp: 321255

Ion Ratio Lower Upper

117 100

82 58.4 45.9 68.9




119 32.1 25.5 38.3

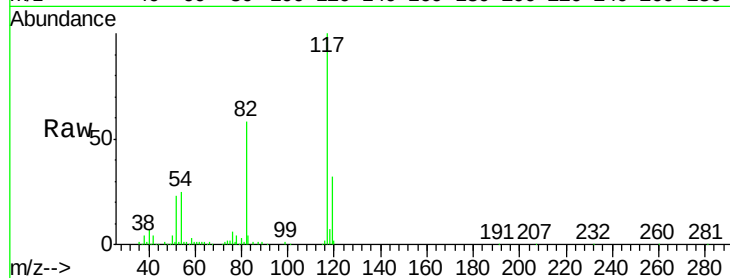

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

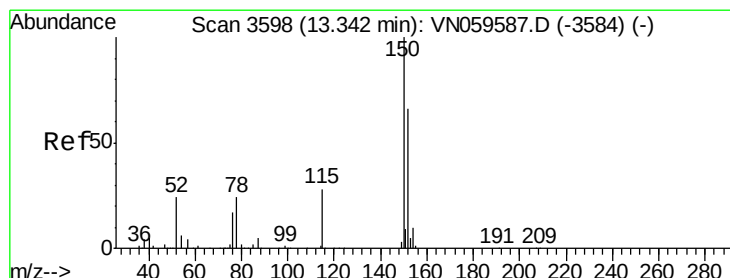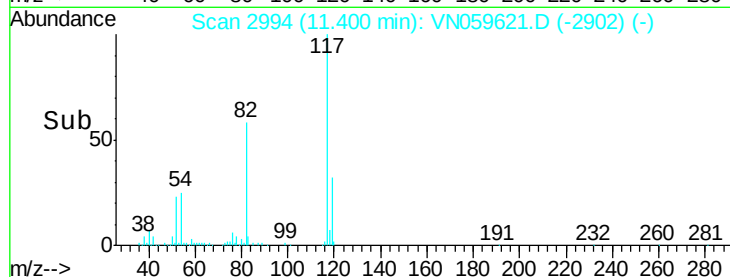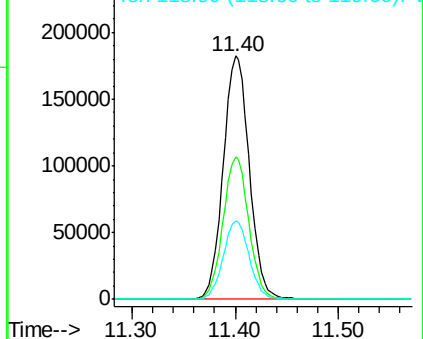

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN059621.D

Acq: 17 Dec 2019 13:38


Tgt Ion:152 Resp: 123042

Ion Ratio Lower Upper

152 100

115 60.6 30.3 90.9

150 156.5 0.0 345.2

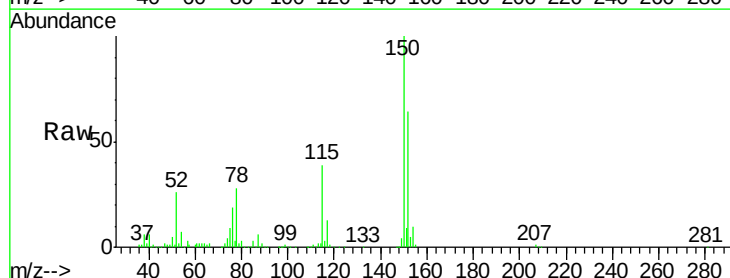

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

