
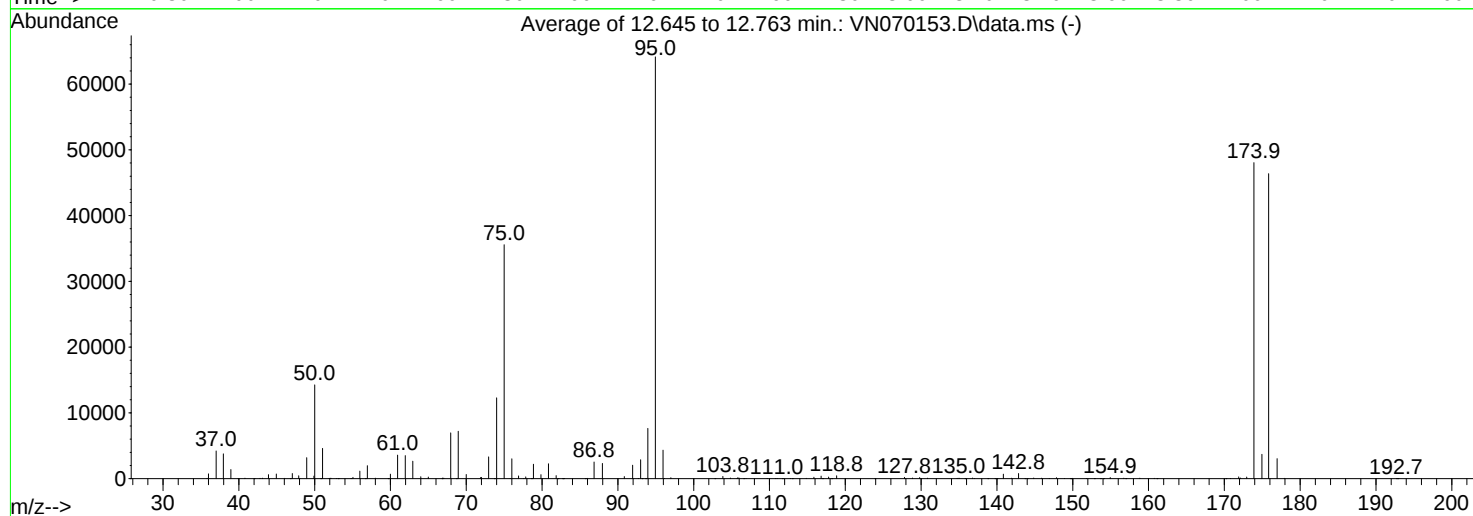


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
 Data File : VN070153.D
 Acq On : 17 Dec 2021 9:25
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N121321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Dec 14 00:59:04 2021

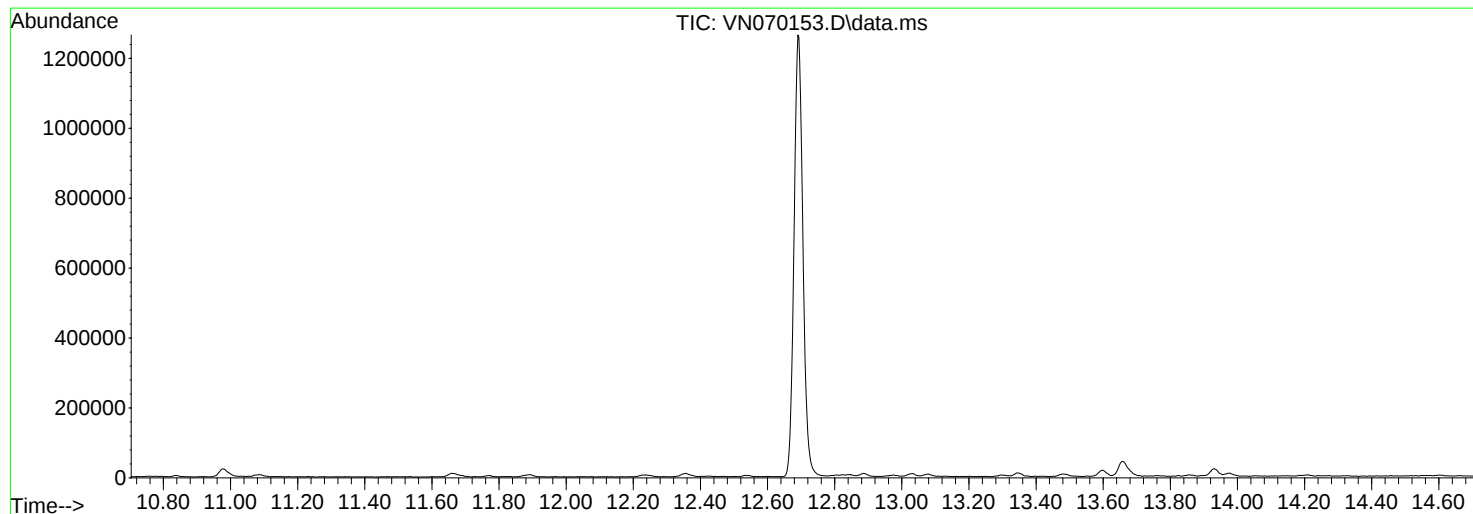

AutoFind: Averaged scan 3973 to 4017; Bkg corrected with scan 3972

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	14248	PASS
75	95	30	60	55.5	35574	PASS
95	95	100	100	100.0	64146	PASS
96	95	5	9	6.7	4323	PASS
173	174	0.00	2	0.5	258	PASS
174	95	50	100	74.9	48056	PASS
175	174	5	9	7.7	3694	PASS
176	174	95	101	96.5	46377	PASS
177	176	5	9	6.5	3033	PASS