
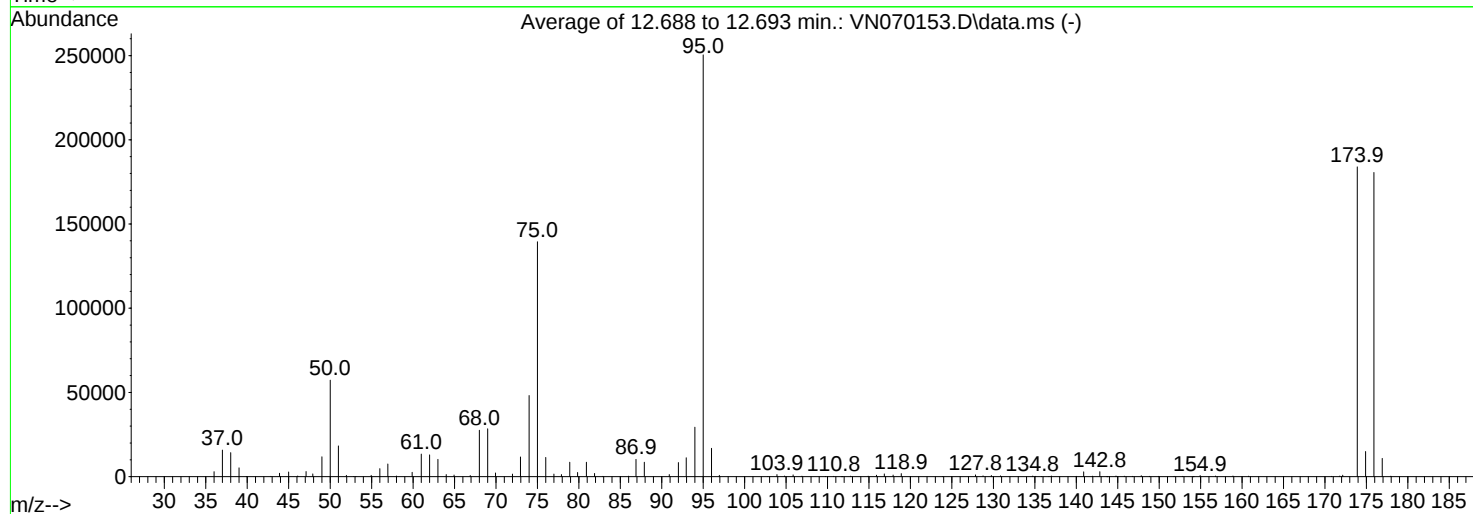


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070153.D
Acq On : 17 Dec 2021 9:25
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

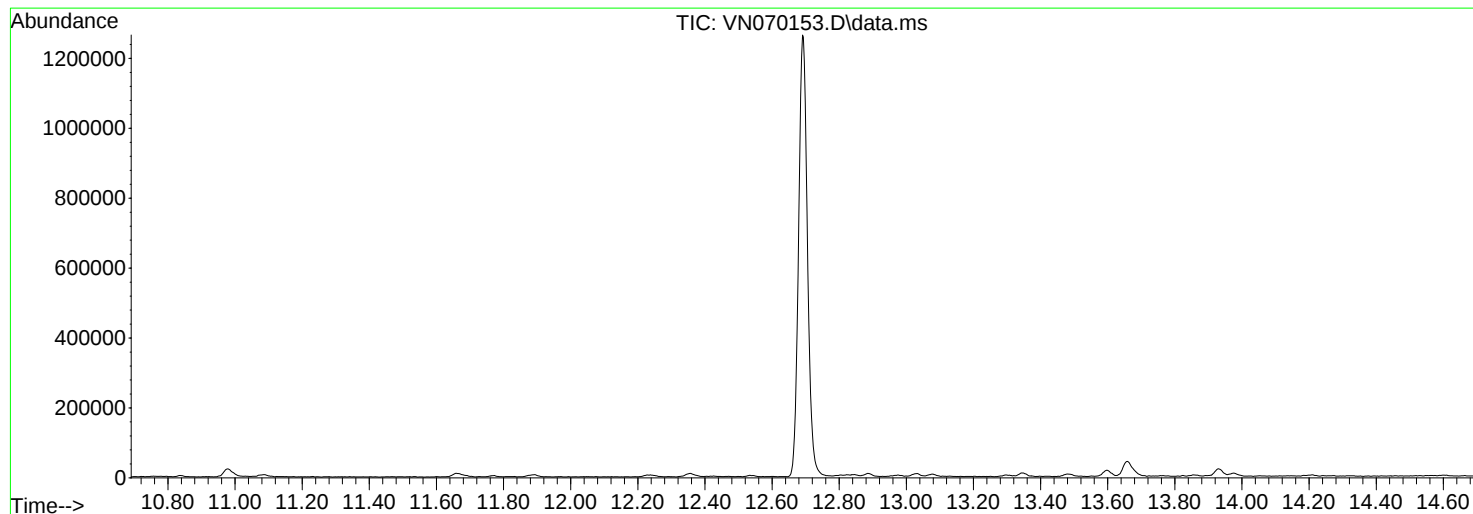

AutoFind: Scans 3989, 3990, 3991; Background Corrected with Scan 3971

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	57333	PASS
75	95	30	60	55.7	139435	PASS
95	95	100	100	100.0	250453	PASS
96	95	5	9	6.7	16792	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.4	183915	PASS
175	174	5	9	8.1	14916	PASS
176	174	95	101	98.2	180587	PASS
177	176	5	9	6.0	10845	PASS