

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
 Data File : VN070191.D
 Acq On : 18 Dec 2021 3:41
 Operator : JC/MD
 Sample : M5132-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260

Signal : TIC: VN070191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	155	171	193	rVB	959296	1612519	19.97%	2.760%
2	3.022	375	385	403	rVB5	132739	306858	3.80%	0.525%
3	3.438	528	540	561	rVB3	61953	141666	1.75%	0.242%
4	3.923	698	721	736	rBV2	80198	226257	2.80%	0.387%
5	4.181	791	817	846	rBV	1078461	3052632	37.81%	5.225%
6	4.594	951	971	996	rBV2	26552	87538	1.08%	0.150%
7	6.391	1618	1641	1671	rVB	125891	406191	5.03%	0.695%
8	7.327	1967	1990	2016	rBV2	191131	531645	6.58%	0.910%
9	8.024	2226	2250	2261	rBV	860376	2100381	26.01%	3.595%
10	8.086	2261	2273	2302	rVB	1455305	3365190	41.68%	5.760%
11	8.440	2382	2405	2423	rBV	1022402	2407028	29.81%	4.120%
12	8.536	2423	2441	2476	rVV	2415968	5697009	70.56%	9.752%
13	8.968	2582	2602	2634	rBV	2514162	5234729	64.84%	8.960%
14	9.236	2680	2702	2719	rBV6	83769	193691	2.40%	0.332%
15	9.569	2805	2826	2852	rBV	1151560	2507312	31.05%	4.292%
16	9.848	2918	2930	2953	rVB2	55174	109502	1.36%	0.187%
17	10.202	3047	3062	3086	rBV2	135585	298981	3.70%	0.512%
18	10.443	3133	3152	3188	rBV	4078476	7694394	95.30%	13.171%
19	11.092	3375	3394	3421	rBV3	122641	322978	4.00%	0.553%
20	11.248	3438	3452	3464	rBV3	73351	129527	1.60%	0.222%
21	11.401	3497	3509	3524	rVB3	55485	94307	1.17%	0.161%
22	11.661	3589	3606	3620	rBV	291084	522544	6.47%	0.894%
23	11.747	3620	3638	3669	rBV	4455069	8073911	100.00%	13.820%
24	12.731	3988	4005	4035	rBV	3555336	6340352	78.53%	10.853%
25	13.675	4339	4357	4385	rBV	3875741	6772199	83.88%	11.592%
26	14.933	4812	4826	4841	rVB3	110555	191879	2.38%	0.328%




Sum of corrected areas: 58421220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070191.D
Acq On : 18 Dec 2021 3:41
Operator : JC/MD
Sample : M5132-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

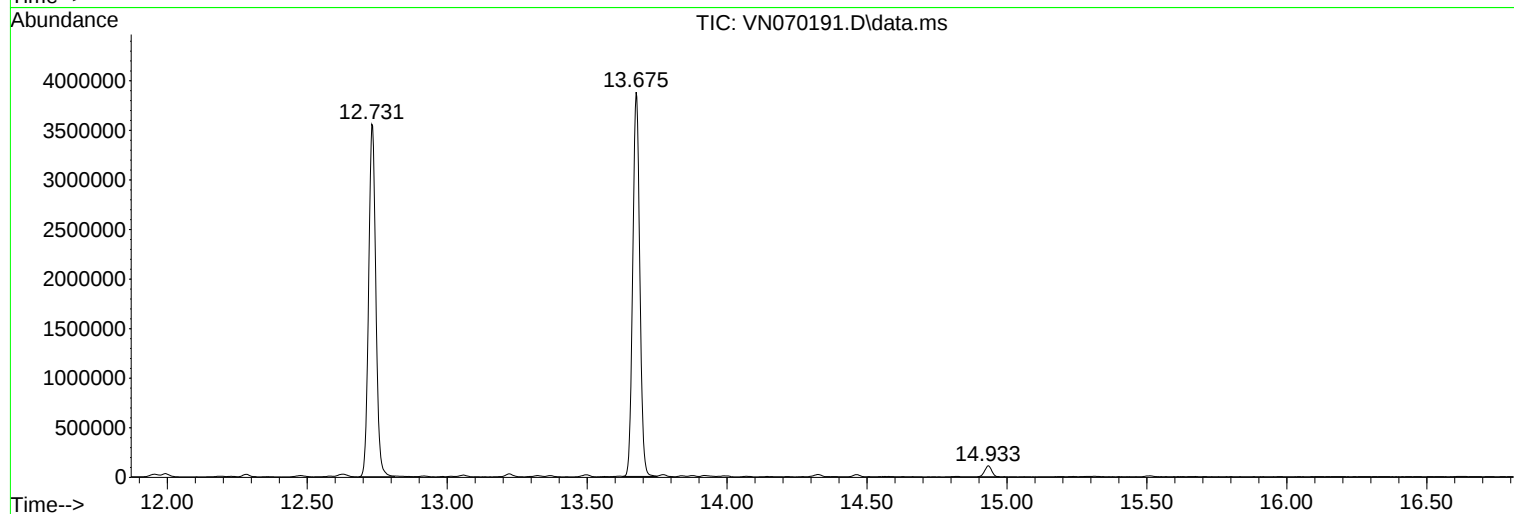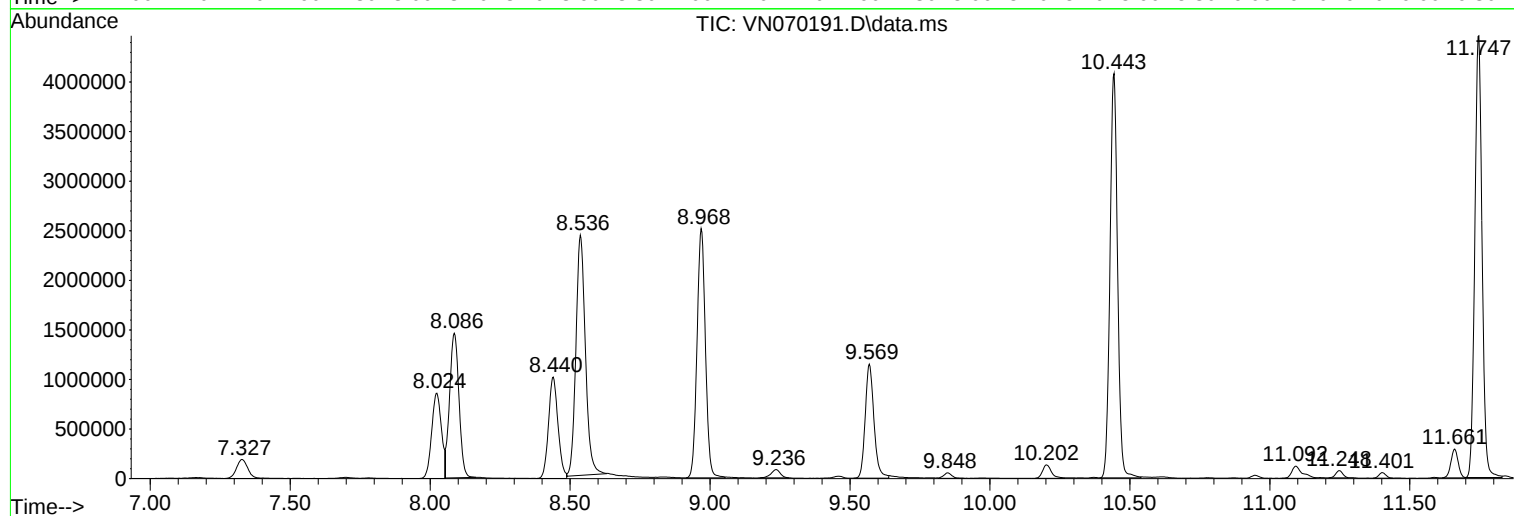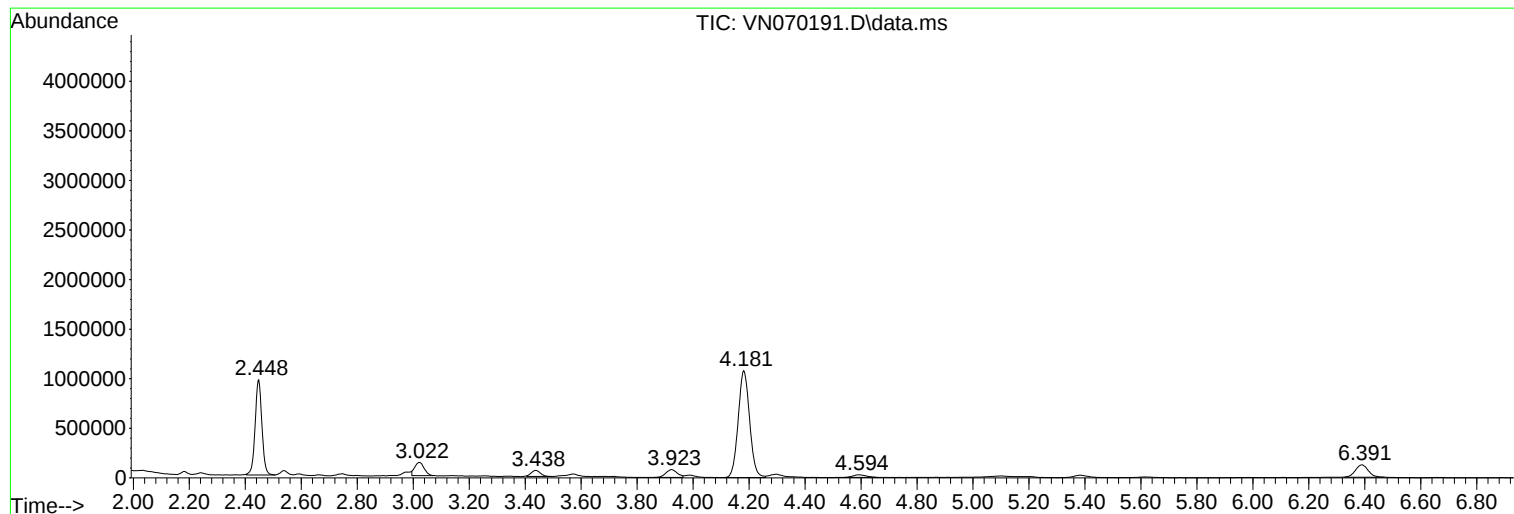

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070191.D
Acq On : 18 Dec 2021 3:41
Operator : JC/MD
Sample : M5132-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070191.D
Acq On : 18 Dec 2021 3:41
Operator : JC/MD
Sample : M5132-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc