

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
 Data File : VN070198.D
 Acq On : 18 Dec 2021 6:40
 Operator : JC/MD
 Sample : M5115-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260

Signal : TIC: VN070198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.024	2227	2250	2261	rBV2	838596	2054915	24.95%	4.508%
2	8.086	2261	2273	2314	rVB	1498157	3410251	41.40%	7.481%
3	8.440	2384	2405	2432	rBV	1007300	2334012	28.33%	5.120%
4	8.968	2578	2602	2630	rBV	2559474	5249412	63.73%	11.516%
5	10.443	3132	3152	3192	rBV	4128458	7809666	94.81%	17.132%
6	11.744	3618	3637	3665	rBV	4516739	8237272	100.00%	18.070%
7	12.731	3988	4005	4028	rBV	3641974	6408114	77.79%	14.057%
8	13.675	4340	4357	4380	rBV	4120785	7121089	86.45%	15.621%
9	13.771	4382	4393	4405	rVV2	121992	214986	2.61%	0.472%
10	13.839	4408	4418	4424	rVV2	80866	129226	1.57%	0.283%
11	13.876	4425	4432	4441	rVV	106716	174484	2.12%	0.383%
12	13.919	4442	4448	4459	rVB2	55209	82909	1.01%	0.182%
13	14.278	4573	4582	4591	rBV	58743	95983	1.17%	0.211%
14	14.466	4641	4652	4662	rBV2	117218	183852	2.23%	0.403%
15	14.657	4714	4723	4739	rVB2	95461	166291	2.02%	0.365%
16	14.823	4771	4785	4797	rBV4	115662	210138	2.55%	0.461%
17	15.316	4946	4969	4984	rVB3	575596	1319684	16.02%	2.895%
18	15.641	5073	5090	5108	rBV4	111651	280855	3.41%	0.616%
19	16.338	5336	5350	5365	rBV6	47367	102072	1.24%	0.224%


Sum of corrected areas: 45585211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070198.D
Acq On : 18 Dec 2021 6:40
Operator : JC/MD
Sample : M5115-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

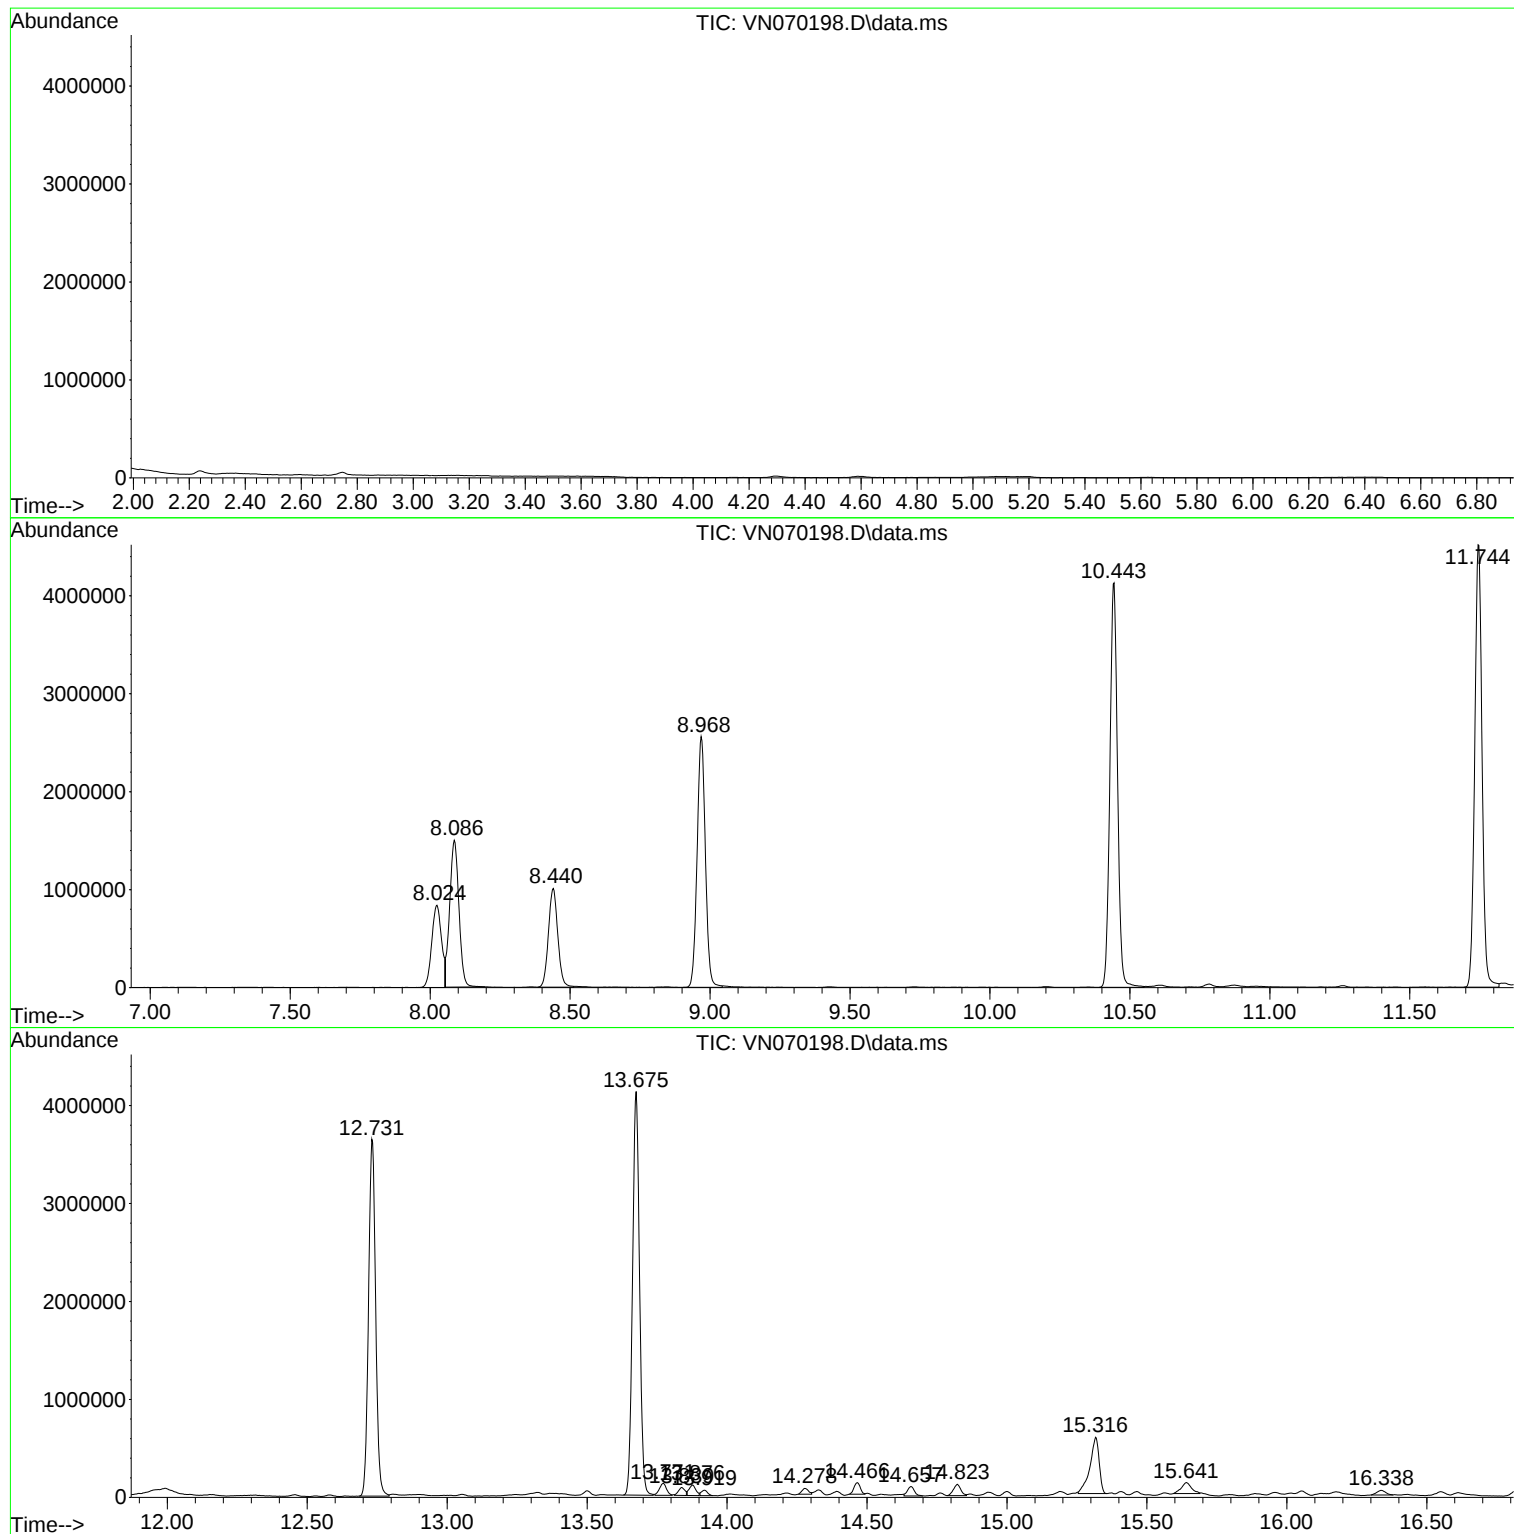

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070198.D
Acq On : 18 Dec 2021 6:40
Operator : JC/MD
Sample : M5115-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1H-Indene, 2,3-dihydro-1,6-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.316	9.27 ug/l	1319680	1,4-Dichlorobenzene-d4	13.675

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1H-Indene, 2,3-dihydro-1,6-dimet...	146	C11H14	017059-48-2	94		
2	1H-Indene, 2,3-dihydro-1,1-dimet...	146	C11H14	004912-92-9	91		
3	1H-Indene, 2,3-dihydro-1,3-dimet...	146	C11H14	004175-53-5	91		
4	1H-Indene, 2,3-dihydro-4,7-dimet...	146	C11H14	006682-71-9	91		
5	Benzene, (1-methyl-1-butenyl)-	146	C11H14	053172-84-2	91		

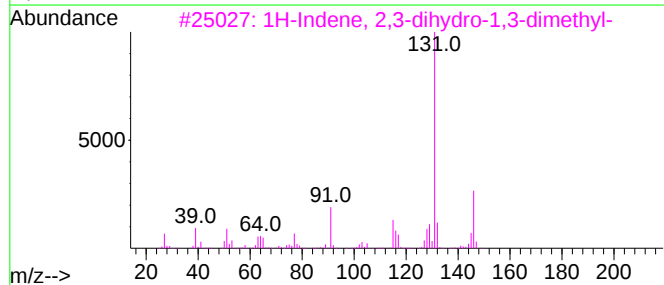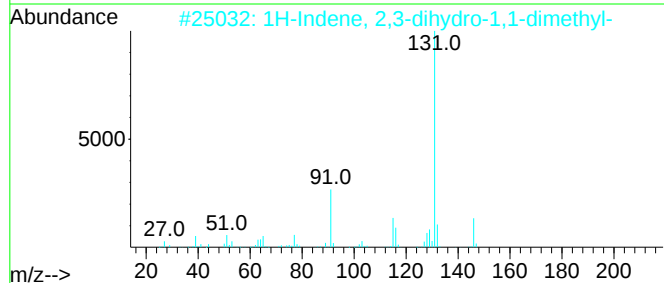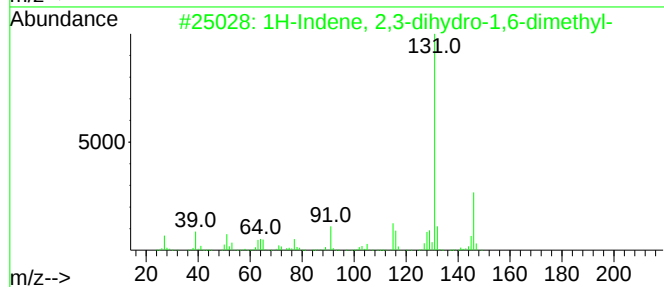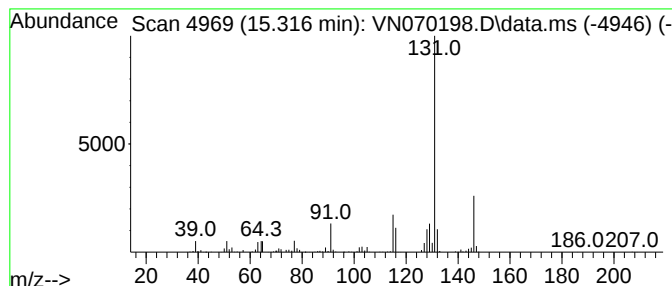

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070198.D
Acq On : 18 Dec 2021 6:40
Operator : JC/MD
Sample : M5115-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 2,3-...	15.316	9.3	ug/l	1319680	4	13.675	7121090	50.0