


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121721\
Data File : VN070179.D
Acq On : 17 Dec 2021 22:08
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

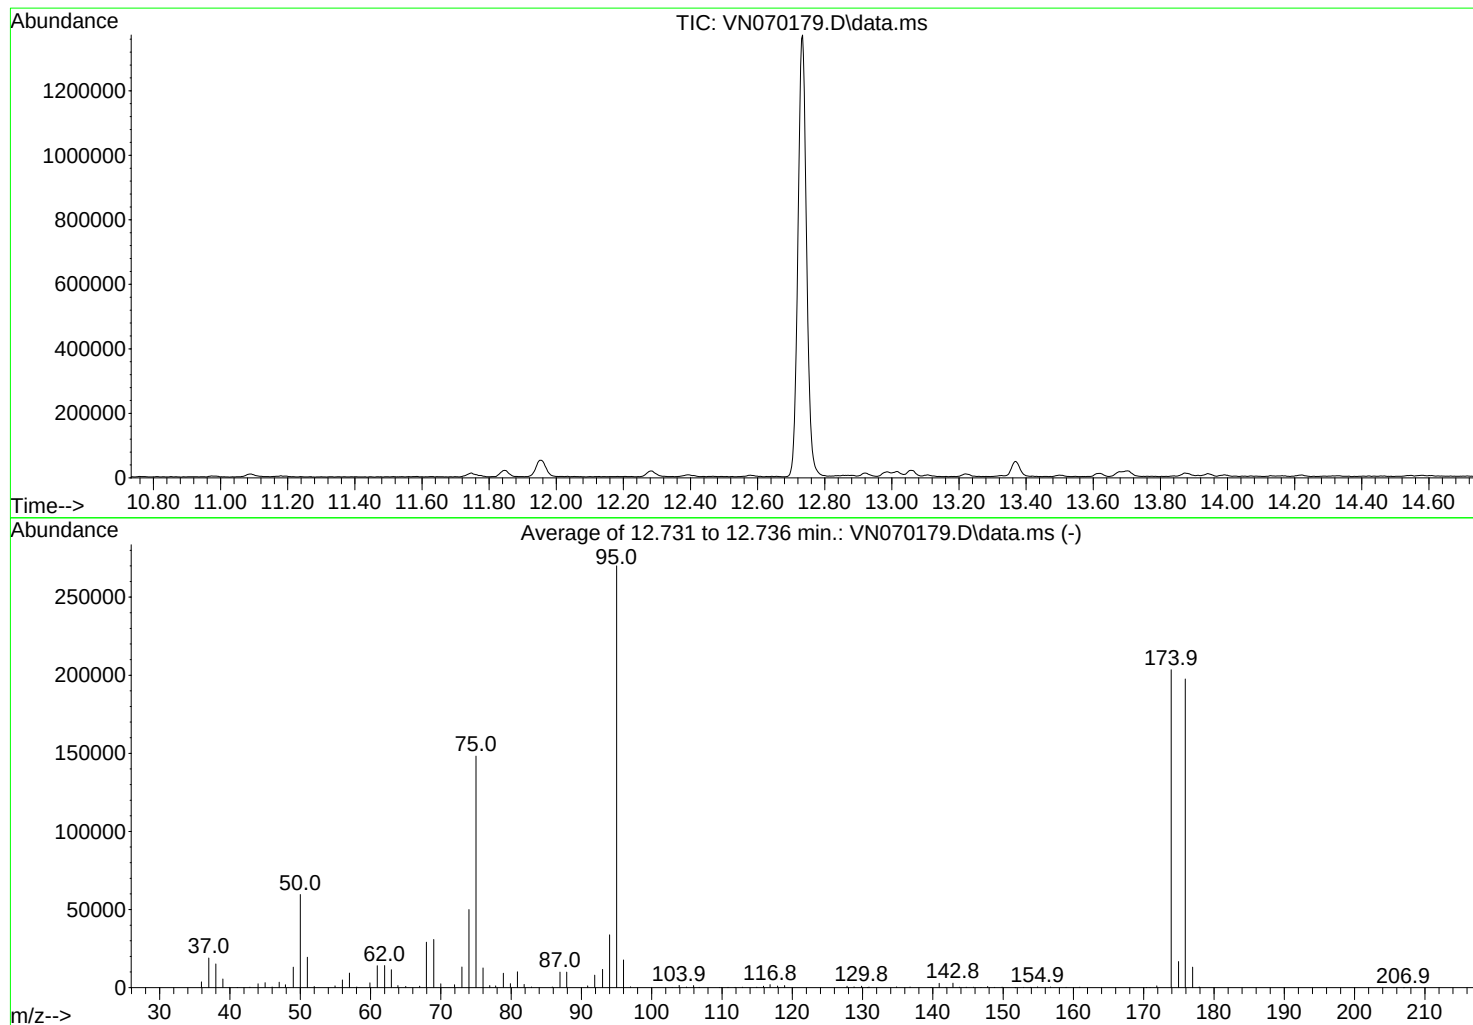

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	59621	PASS
75	95	30	60	54.9	148203	PASS
95	95	100	100	100.0	270037	PASS
96	95	5	9	6.6	17691	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.4	203520	PASS
175	174	5	9	8.2	16728	PASS
176	174	95	101	97.1	197611	PASS
177	176	5	9	6.6	13108	PASS