
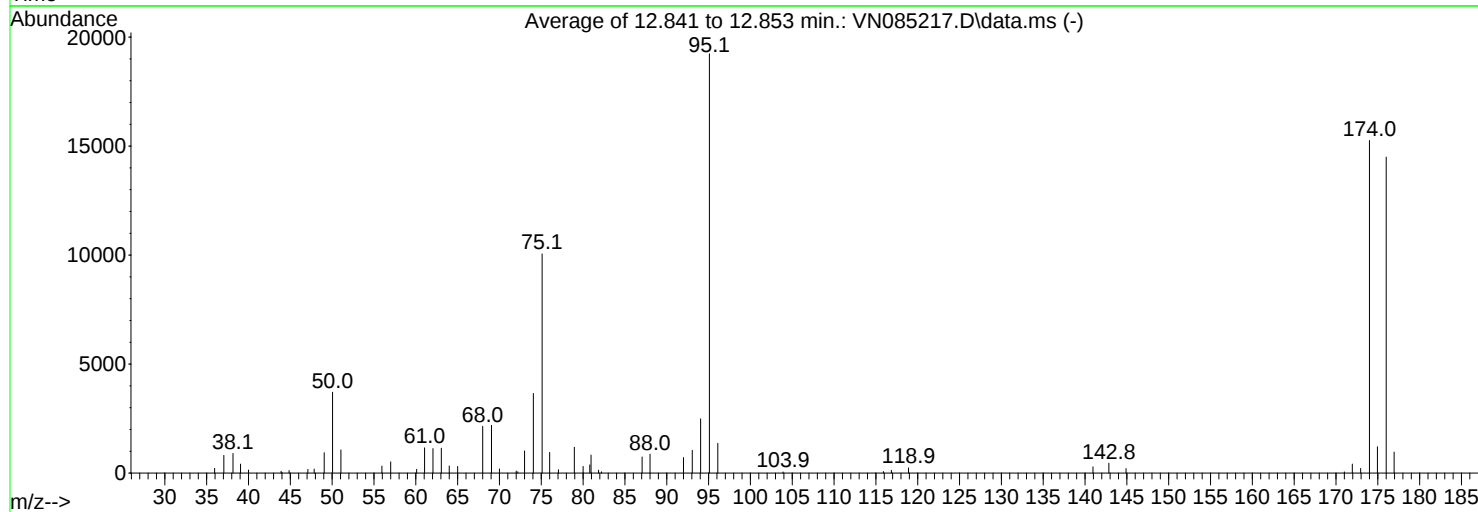


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121724\
Data File : VN085217.D
Acq On : 17 Dec 2024 11:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112224W.M
Title : SW846 8260
Last Update : Sat Nov 23 02:54:10 2024

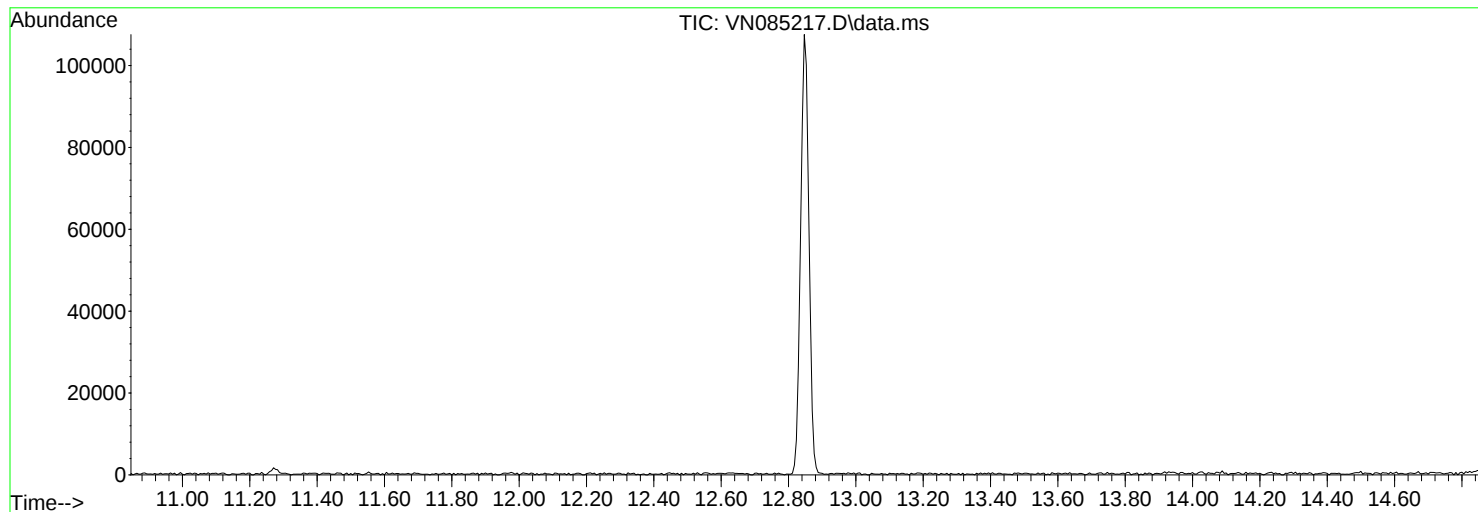

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	3708	PASS
75	95	30	60	52.3	10056	PASS
95	95	100	100	100.0	19237	PASS
96	95	5	9	7.1	1368	PASS
173	174	0.00	2	1.4	213	PASS
174	95	50	100	79.3	15256	PASS
175	174	5	9	7.9	1207	PASS
176	174	95	101	95.0	14496	PASS
177	176	5	9	6.7	964	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	219	50.05	3708	69.05	2191	80.80	377
37.05	813	51.05	1062	70.00	192	80.95	829
38.15	901	55.95	320	72.00	94	81.85	136
39.05	411	57.00	516	72.20	61	82.20	60
40.00	142	60.10	171	73.00	1018	87.05	741
43.90	87	61.05	1158	74.05	3656	88.00	868
44.00	30	62.05	1125	75.10	10056	92.00	711
44.85	118	63.05	1141	76.00	950	93.05	1044
47.10	167	64.00	325	77.05	152	94.05	2489
47.85	186	65.00	305	78.95	1188	95.10	19237
49.05	936	68.00	2144	80.00	307	96.10	1368

Average of 12.841 to 12.853 min.: VN085217.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	52	174.95	1207				
115.90	71	176.00	14496				
116.85	130	176.95	964				
118.90	238						
140.95	286						
142.85	453						
144.90	208						
171.00	55						
171.95	413						
172.95	213						
174.00	15256						

Instrument :

MSVOA_N

ClientSampleId :

BFB