



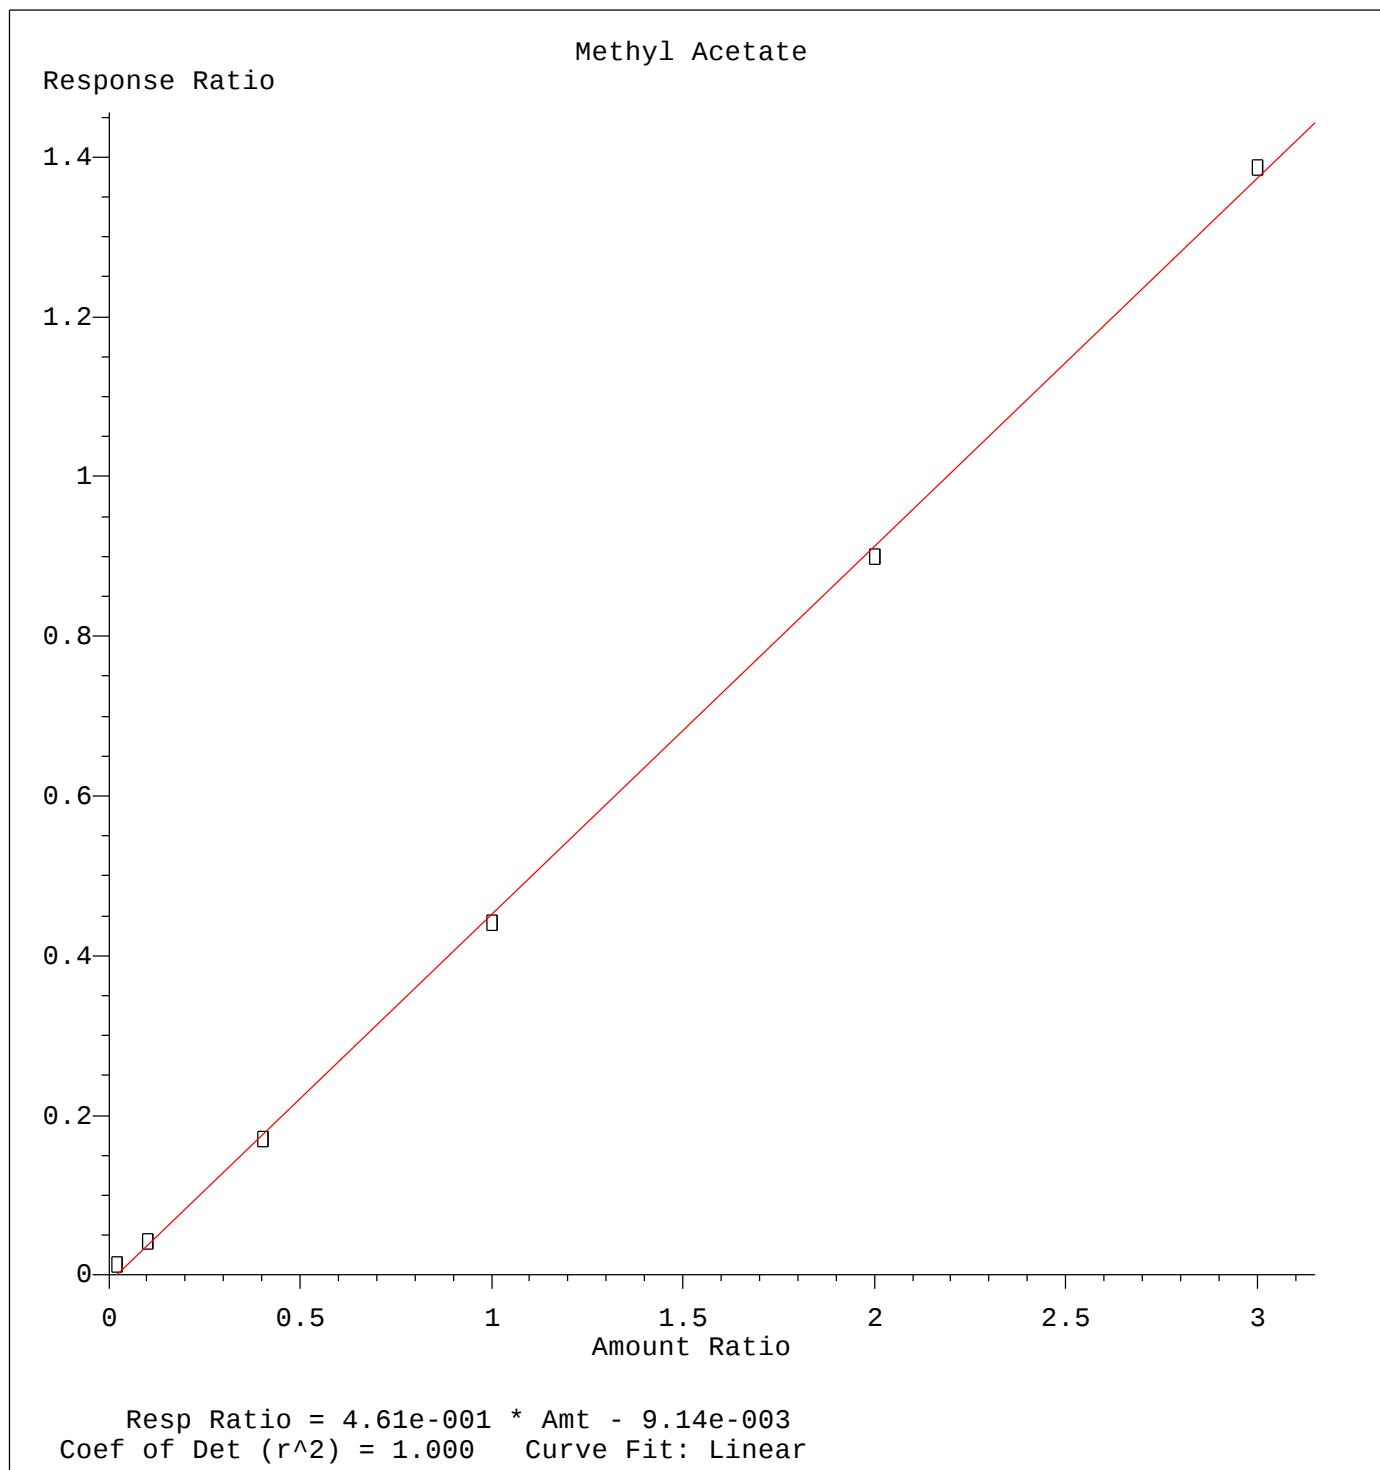

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018


Isopropyl Acetate

Response Ratio

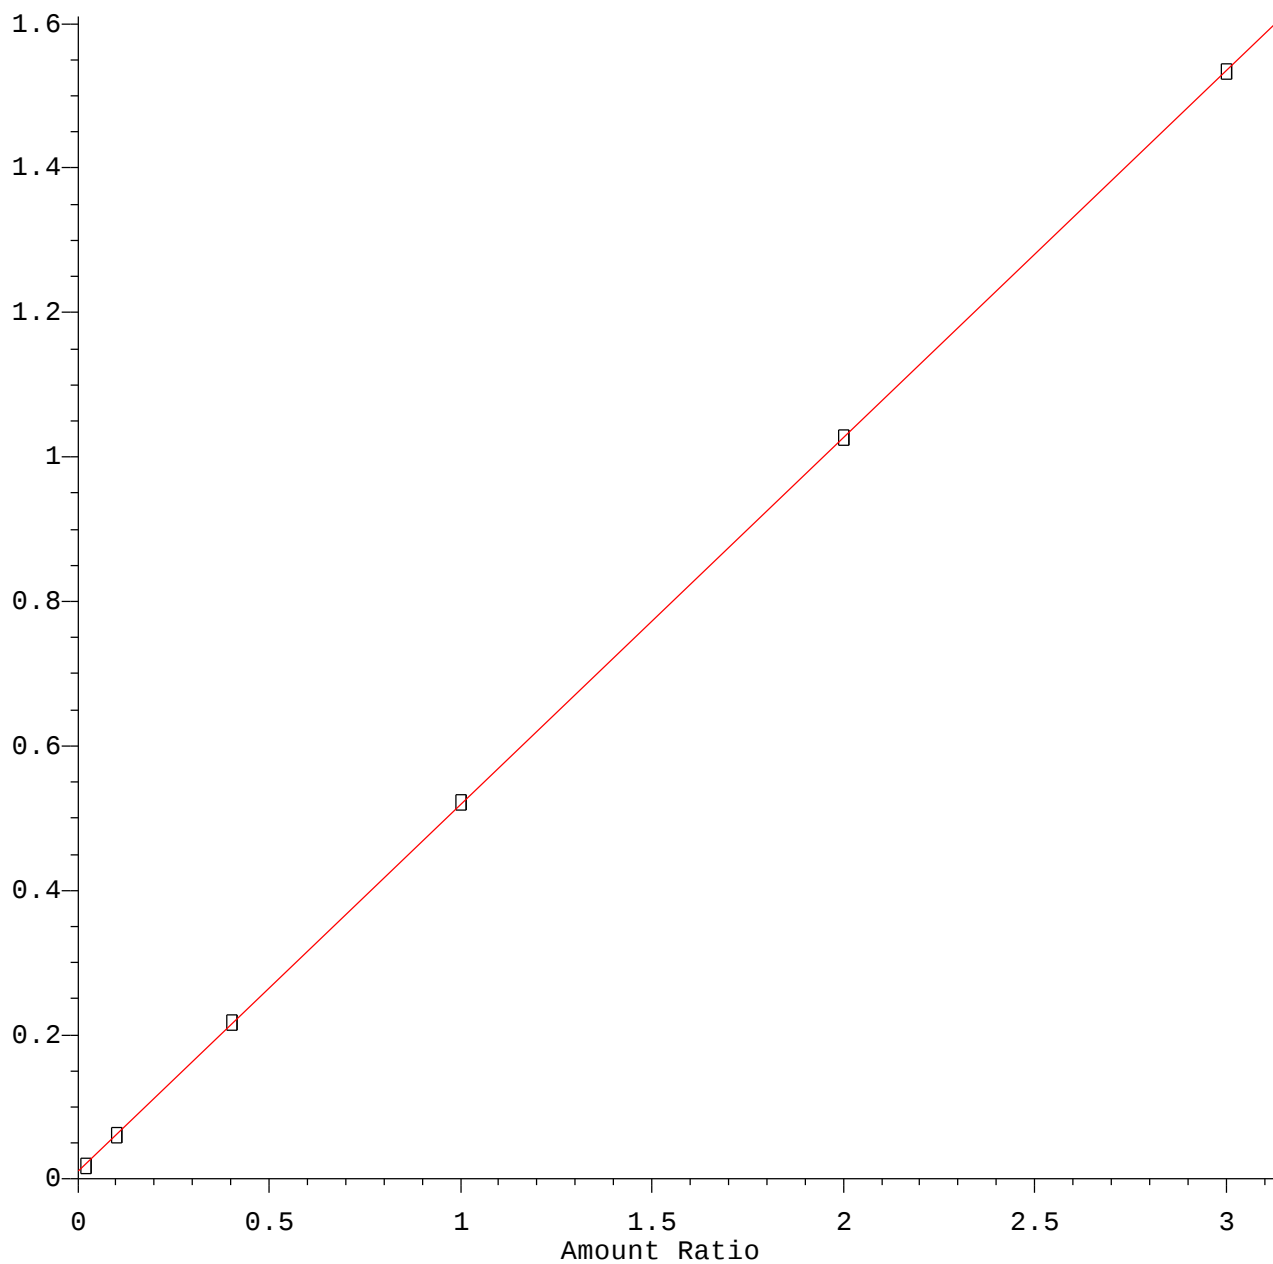

Resp Ratio = 5.08e-001 * Amt + 1.08e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018

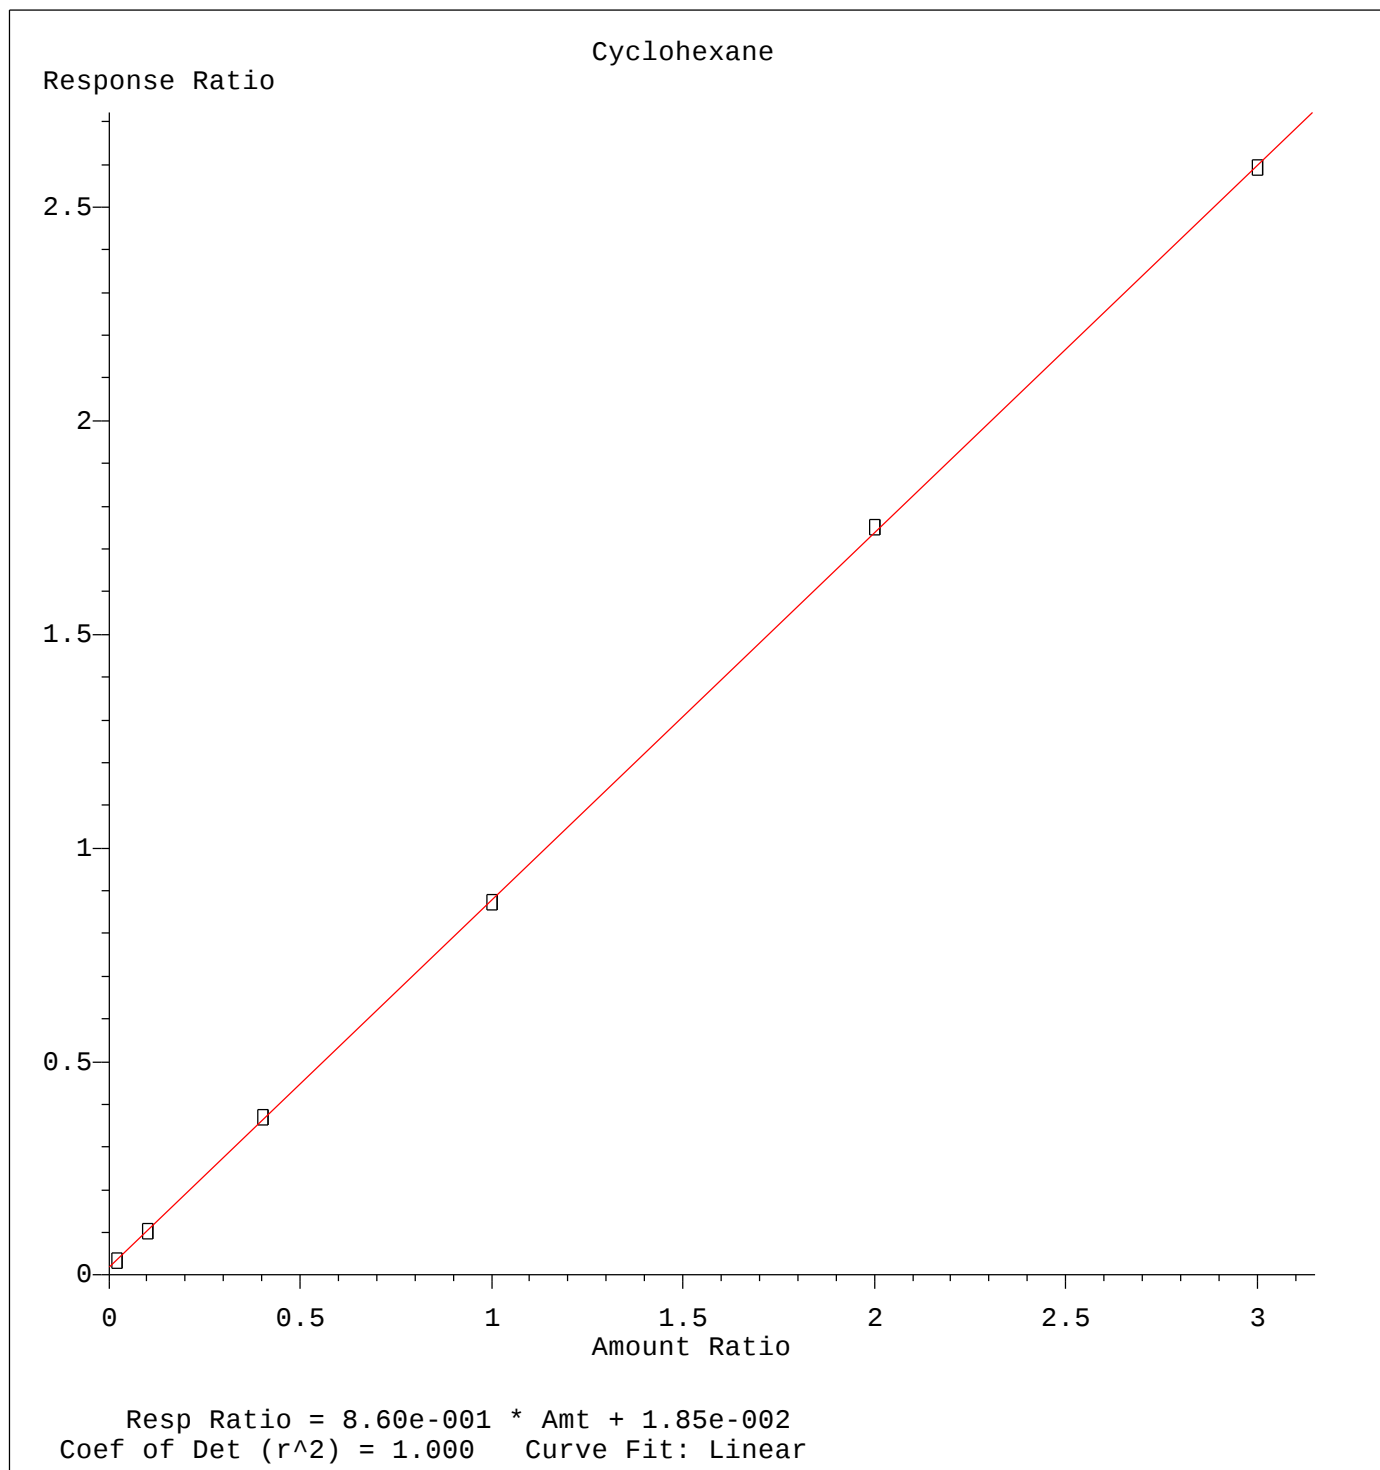

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018

1,2,3-Trichlorobenzene

Response Ratio

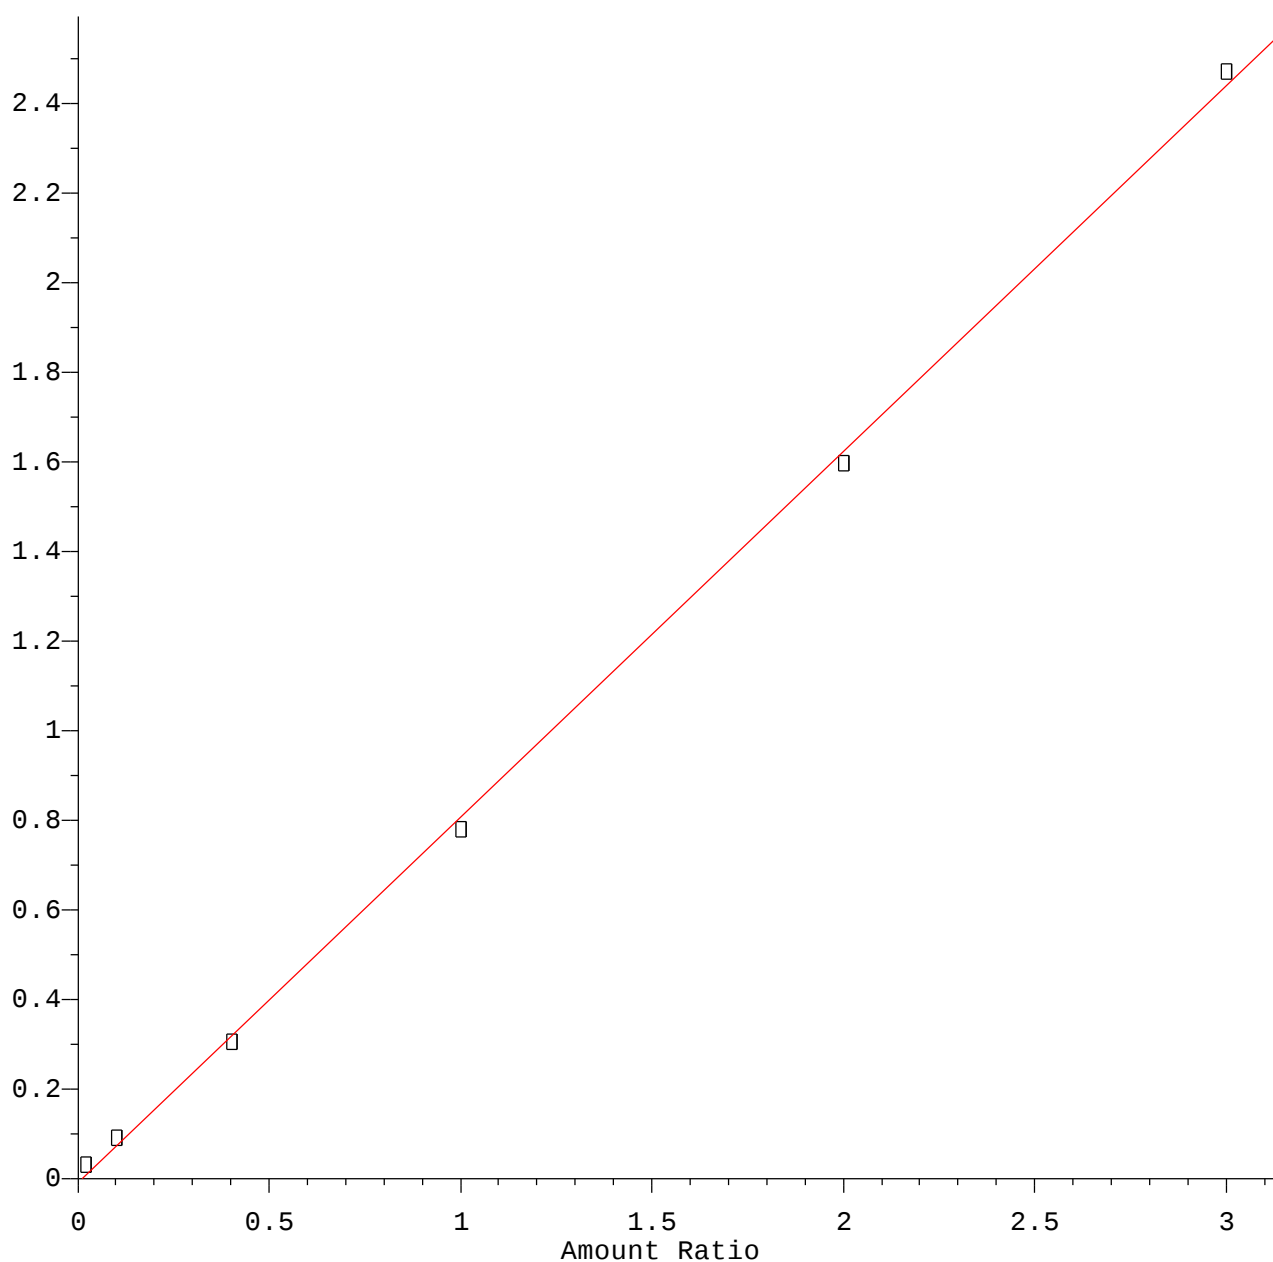


Resp Ratio = $8.16 \times 10^{-1} \times \text{Amt} - 8.29 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018


Naphthalene

Response Ratio

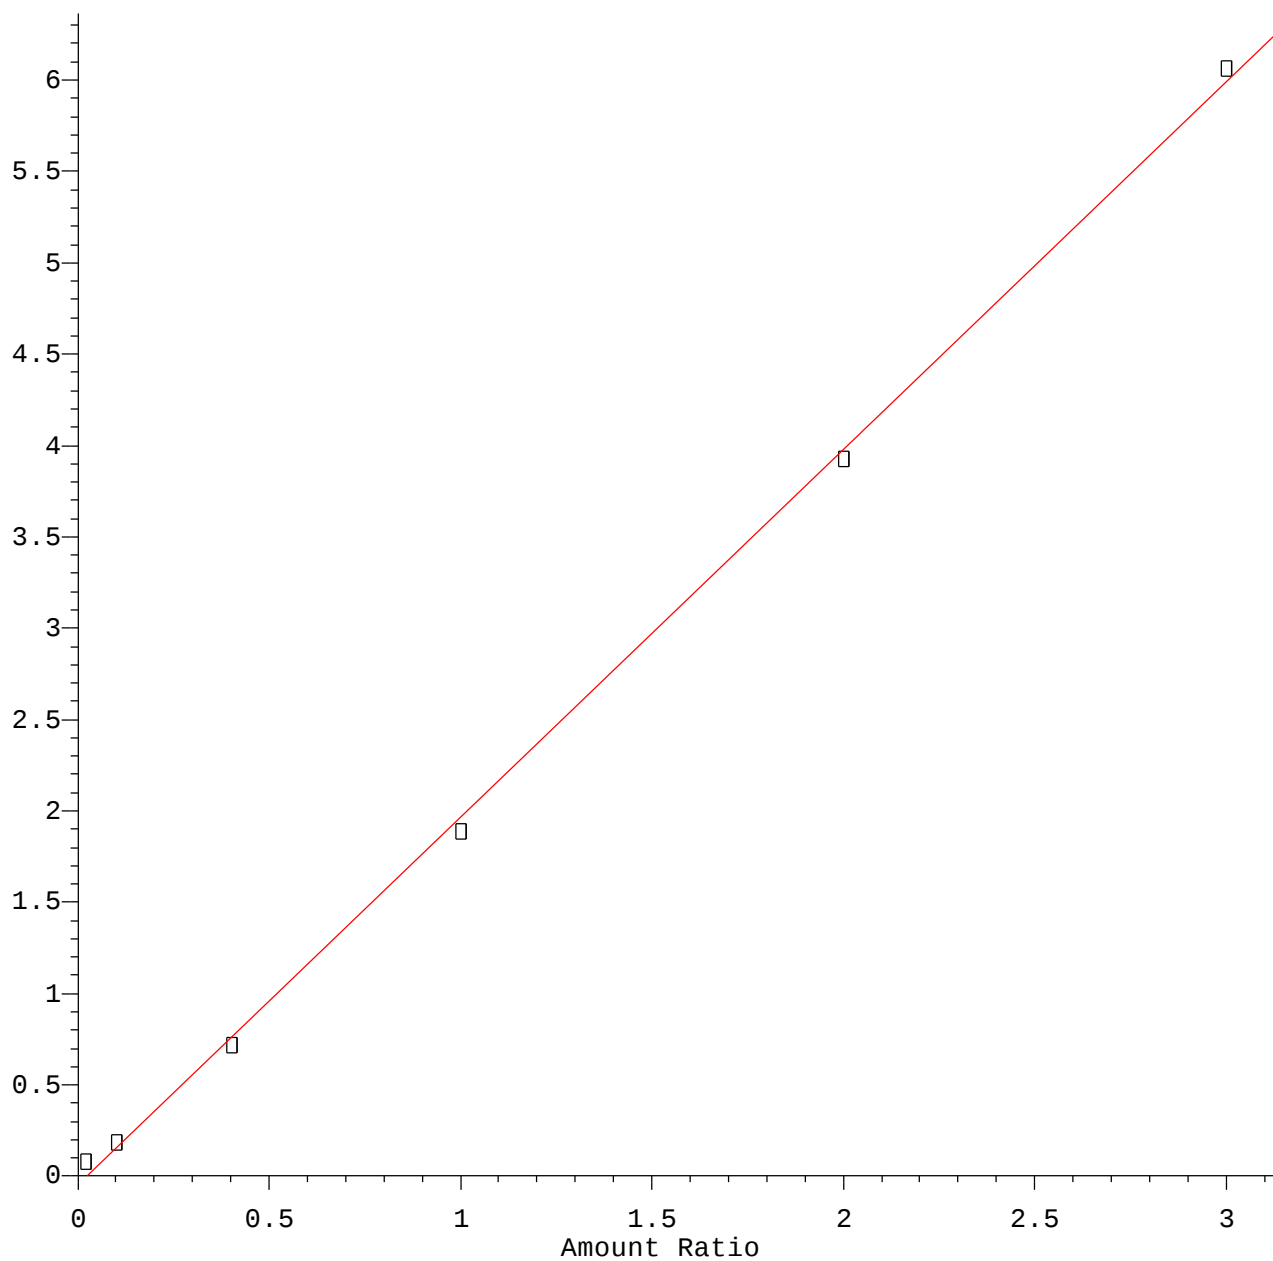

Resp Ratio = 2.01e+000 * Amt - 4.61e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018

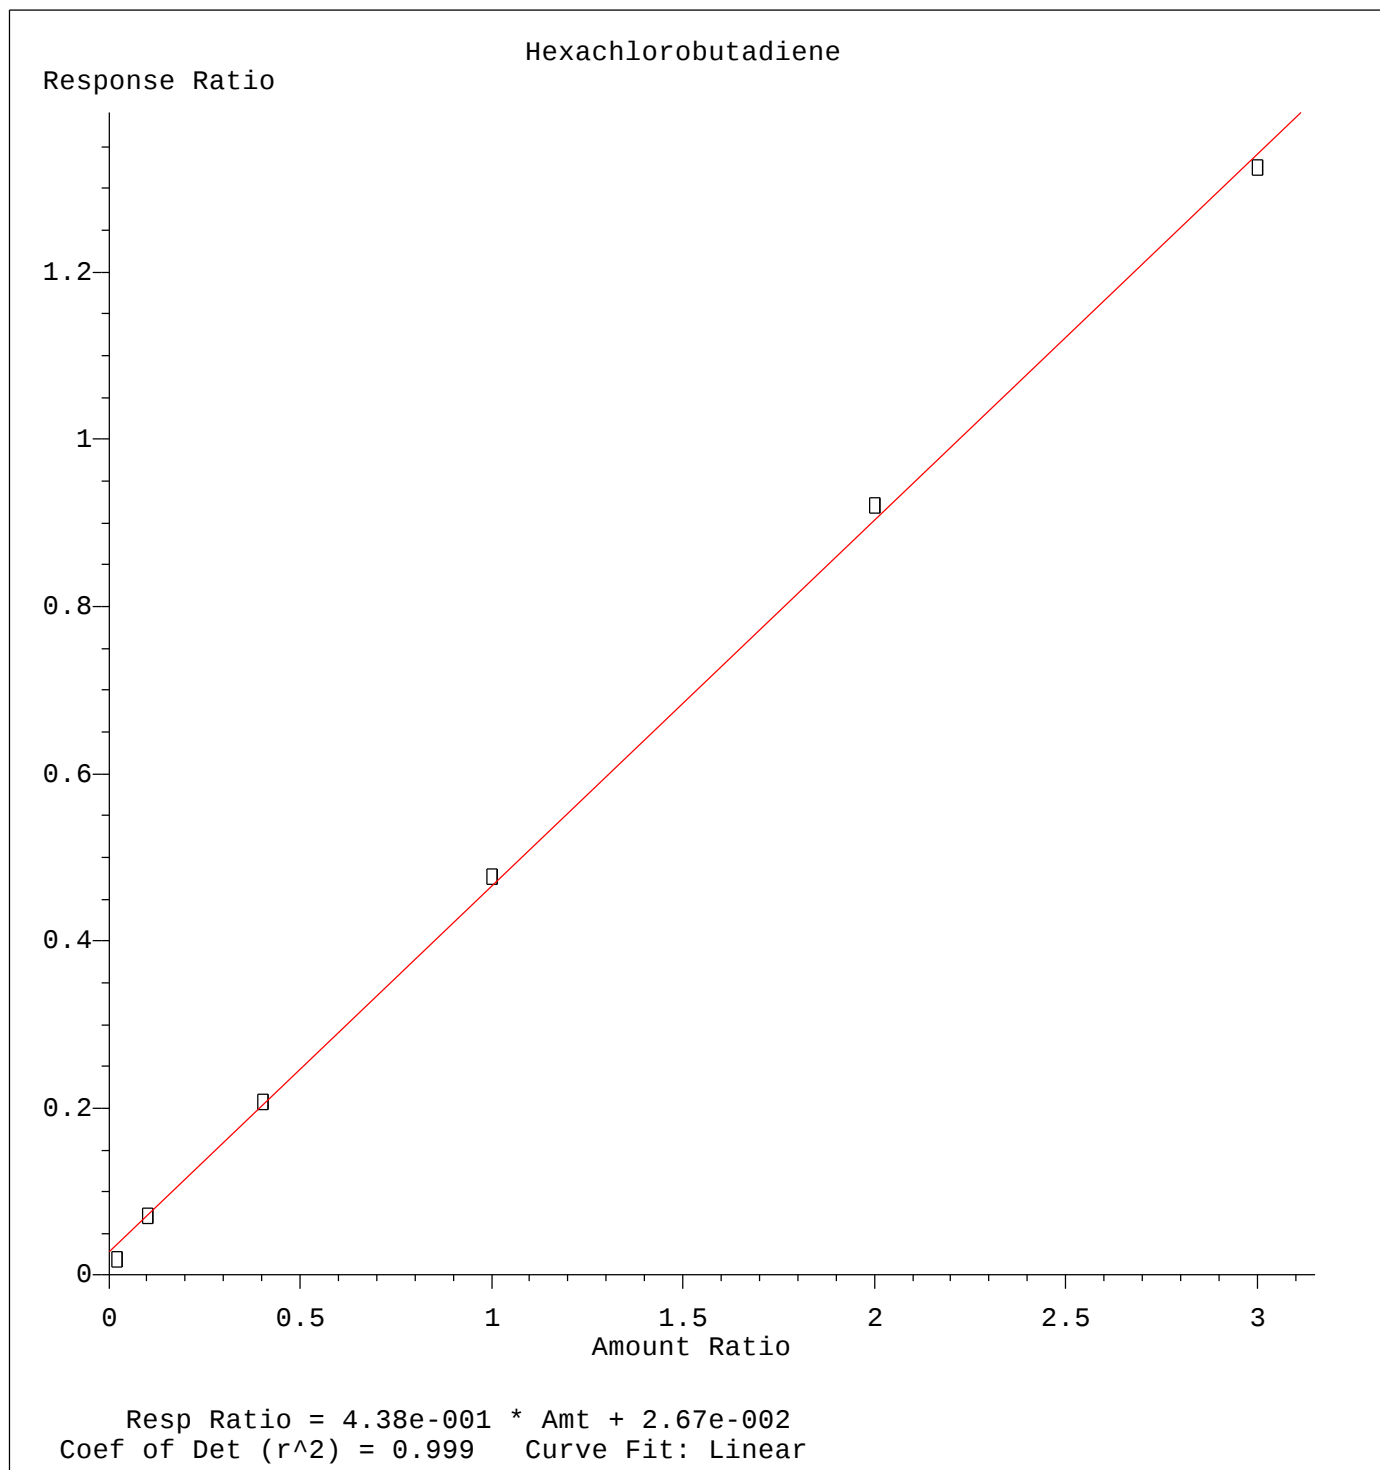

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018

1,2,4-Trichlorobenzene

Response Ratio

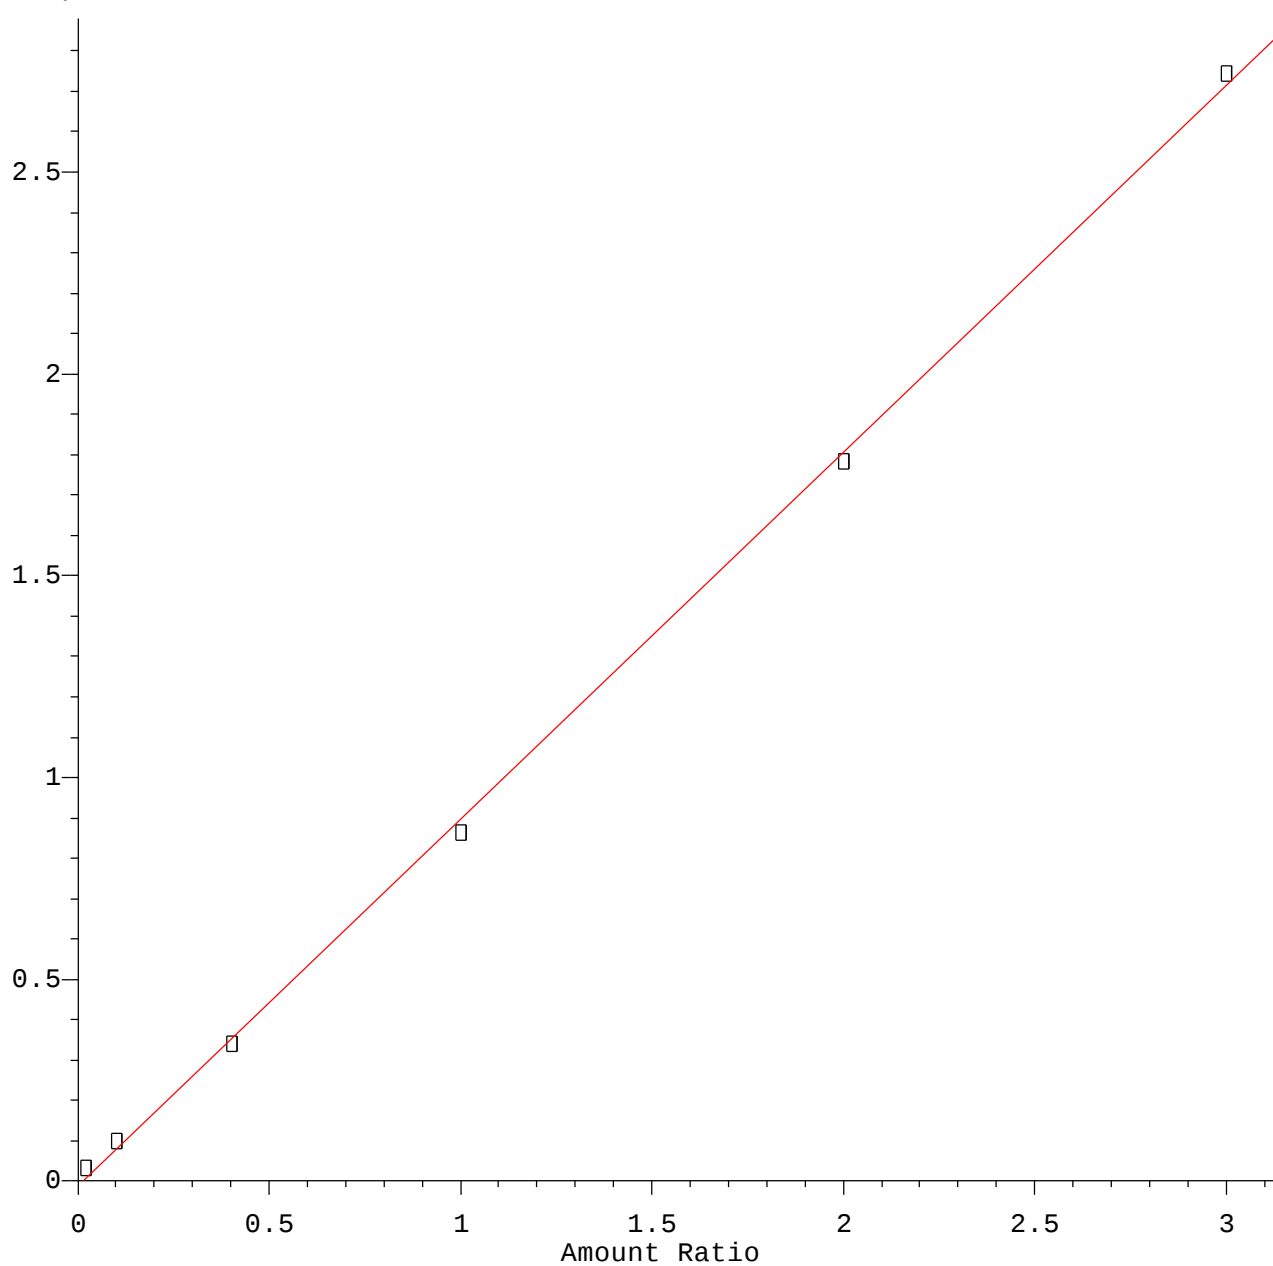

Resp Ratio = 9.08e-001 * Amt - 1.08e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Calibration Table Last Updated: Tue Dec 18 13:03:37 2018