

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN121818\
 Data File : VN052958.D
 Acq On : 18 Dec 2018 13:50
 Operator : MD\SY
 Sample : VN1218MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 9 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1218MBL01

Quant Time: Dec 18 14:41:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 18 13:03:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1434402	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	2198863	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1936681	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	734880	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	700127	48.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.20%	
35) Dibromofluoromethane	7.59	113	545544	54.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.62%	
50) Toluene-d8	10.09	98	2666316	49.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.90%	
62) 4-Bromofluorobenzene	12.40	95	851698	44.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.98%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN121818\
Data File : VN052958.D
Acq On : 18 Dec 2018 13:50
Operator : MD\SY
Sample : VN1218MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 9 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN1218MBL01

Quant Time: Dec 18 14:41:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 18 13:03:37 2018
Response via : Initial Calibration

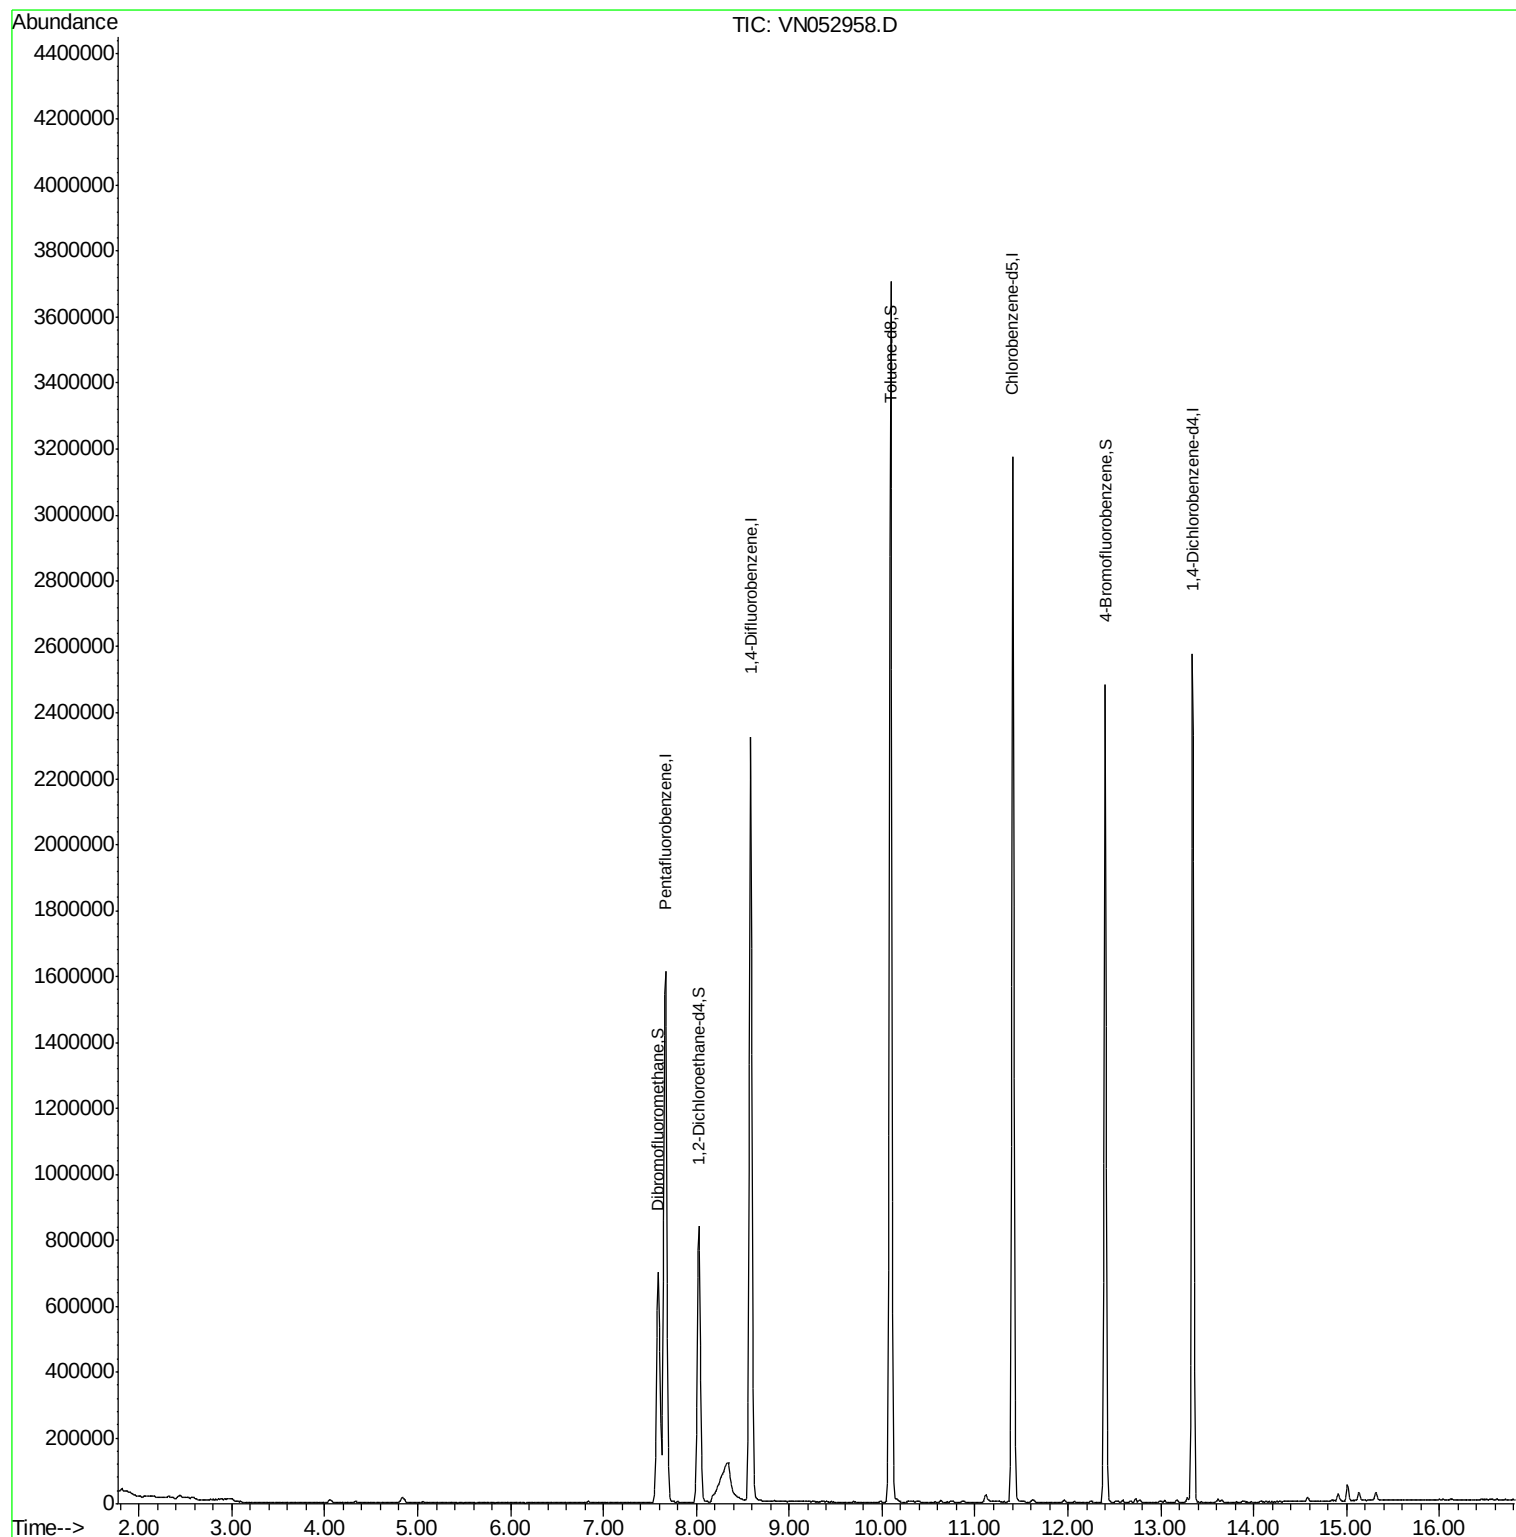

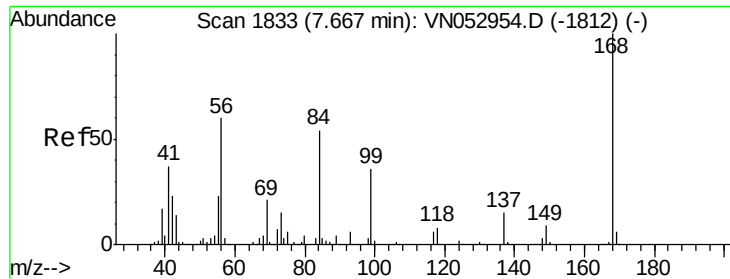

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052958.D

Acq: 18 Dec 2018 13:50

Instrument :

MSVOA_N

ClientSampleId :


VN1218MBL01

Tgt Ion:168 Resp: 1434402

Ion Ratio Lower Upper

168 100

99 49.4 40.2 60.2

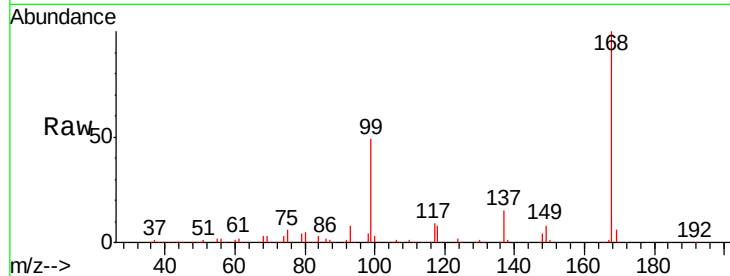

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67



600000

400000

200000

0

Time-->

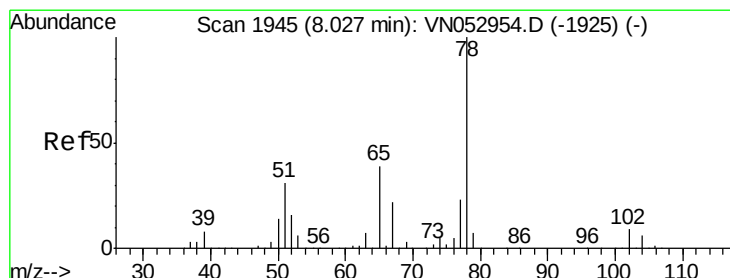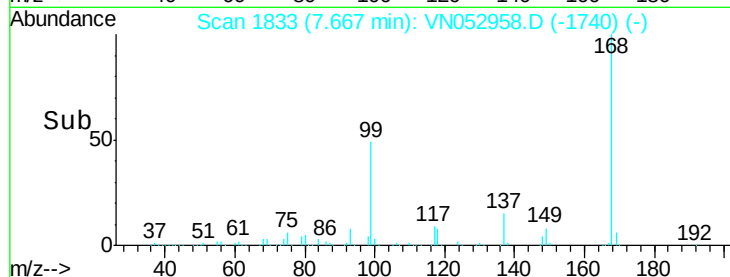

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN052958.D


Acq: 18 Dec 2018 13:50

Tgt Ion: 65 Resp: 700127

Ion Ratio Lower Upper

65 100

67 54.6 0.0 110.4

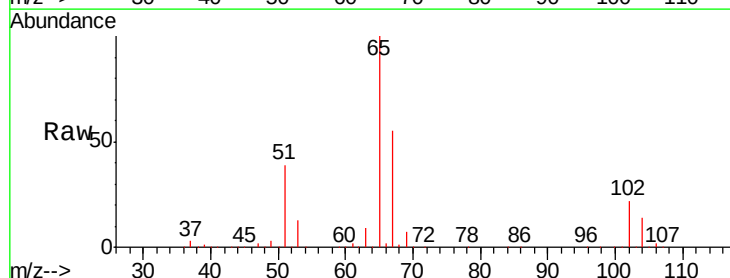

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03


300000


200000

100000

0

Time-->

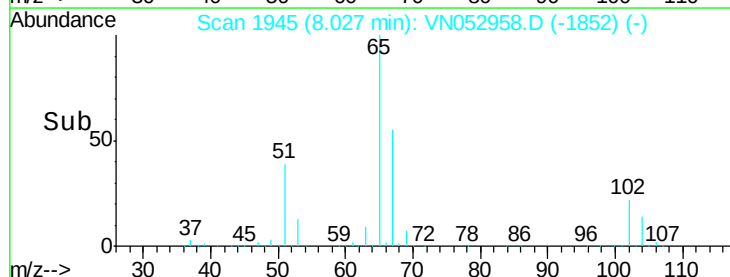


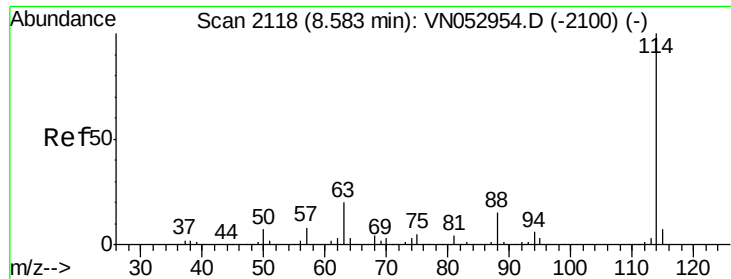




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN052958.D
 Acq: 18 Dec 2018 13:50

Instrument :
 MSVOA_N
 ClientSampled :
 VN1218MBL01

Tgt Ion:114 Resp: 2198863
 Ion Ratio Lower Upper
 114 100
 63 19.4 0.0 39.8
 88 15.5 0.0 31.0

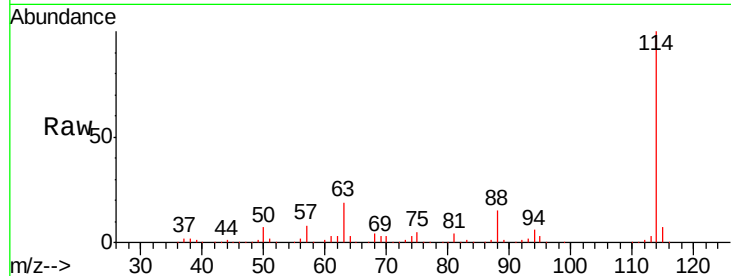


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN0
 Ion 87.90 (87.60 to 88.60): VN0

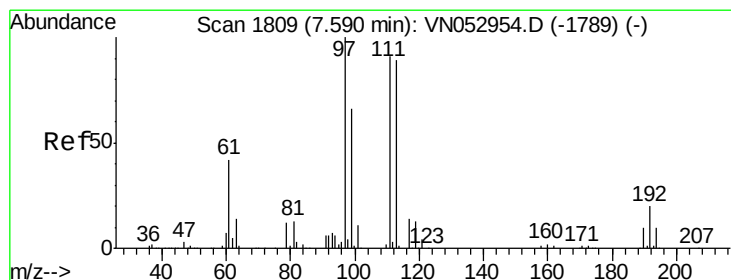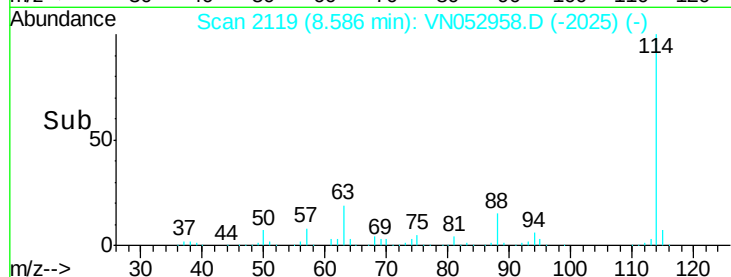
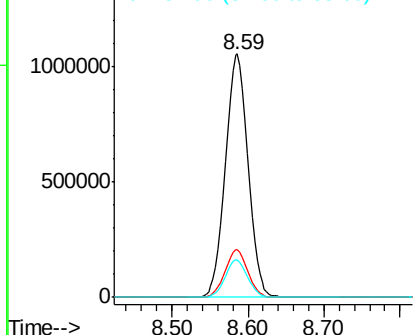



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. -0.00 min
 Lab File: VN052958.D
 Acq: 18 Dec 2018 13:50

Tgt Ion:113 Resp: 545544
 Ion Ratio Lower Upper
 113 100
 111 102.4 83.0 124.4
 192 22.5 17.5 26.3

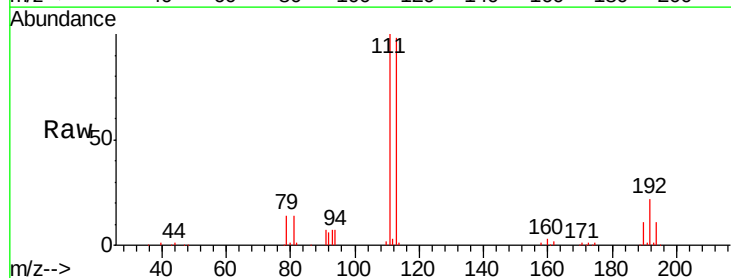

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

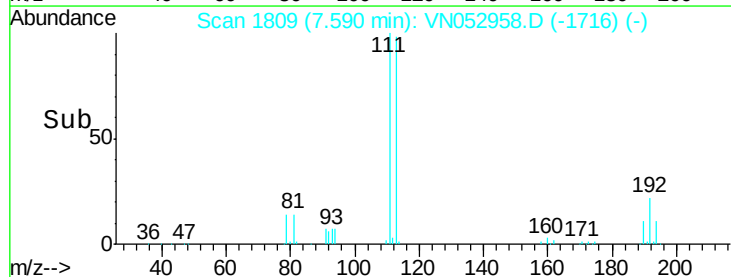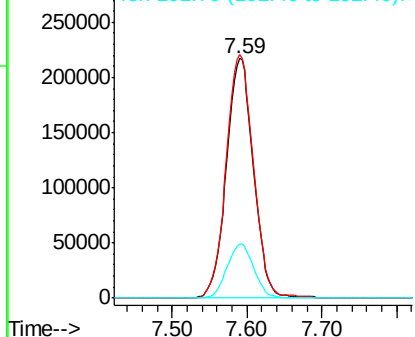

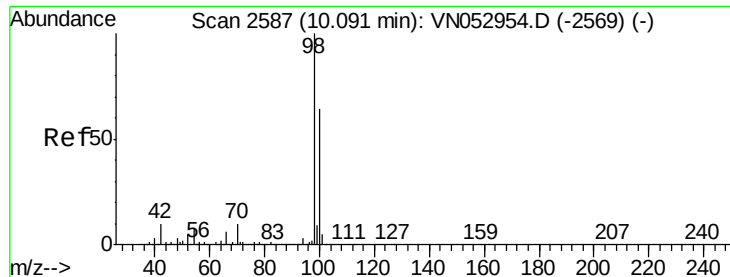

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052958.D

Acq: 18 Dec 2018 13:50

Instrument :

MSVOA_N

ClientSampleId :


VN1218MBL01

Tgt Ion: 98 Resp: 2666316

Ion Ratio Lower Upper

98 100

100 64.5 51.6 77.4

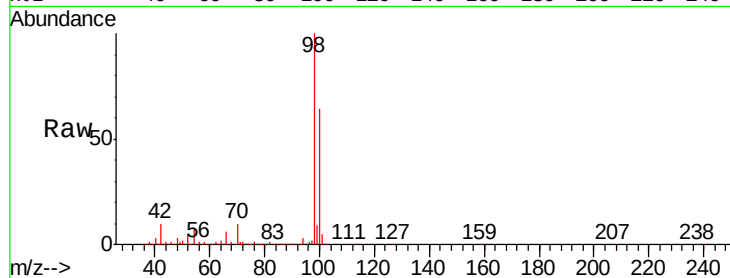

Abundance Ion 98.00 (97.70 to 98.70): VN052954.D (-2569) (-)

Ion 100.00 (99.70 to 100.70): VN052954.D (-2569) (-)

10.09

1500000



1000000

500000

0

Time-->

10.00 10.10 10.20

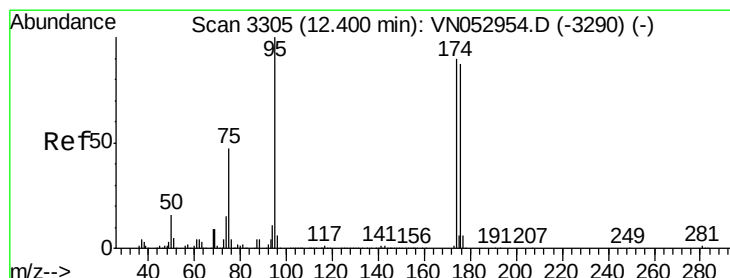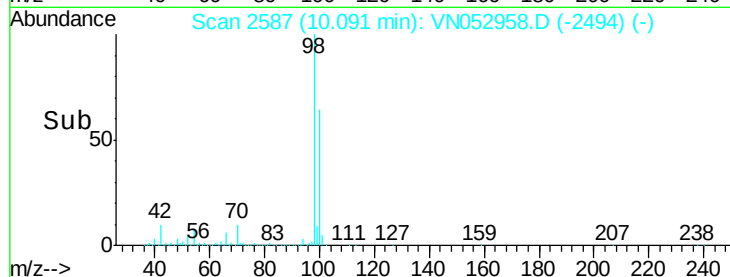

#62

4-Bromofluorobenzene

Concen: Below ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN052958.D

Acq: 18 Dec 2018 13:50


Tgt Ion: 95 Resp: 851698

Ion Ratio Lower Upper

95 100

174 89.8 0.0 178.8

176 87.2 0.0 173.8

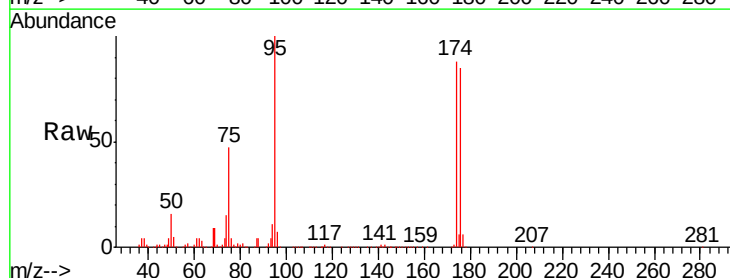

Abundance Ion 94.90 (94.60 to 95.60): VN052954.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN052954.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN052954.D (-3290) (-)

12.40

600000


400000


200000

0

Time-->

12.30 12.40 12.50




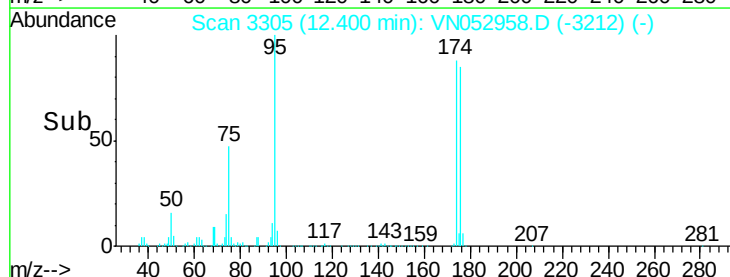


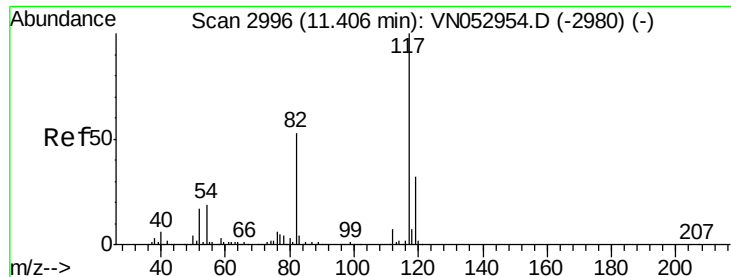

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN052958.D
Acq: 18 Dec 2018 13:50

Instrument :
MSVOA_N
ClientSampled :
VN1218MBL01

Tgt Ion:117 Resp: 1936681
Ion Ratio Lower Upper
117 100
82 53.0 42.8 64.2
119 32.1 25.5 38.3

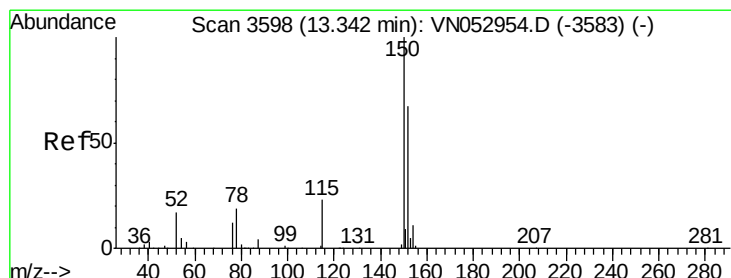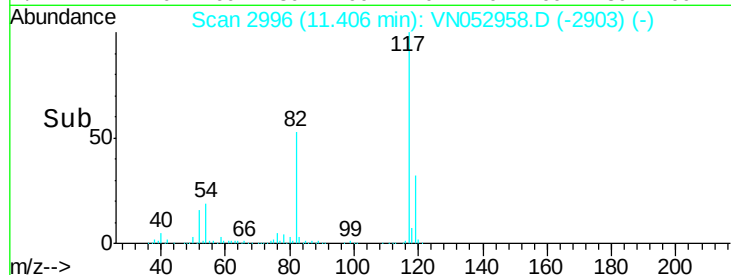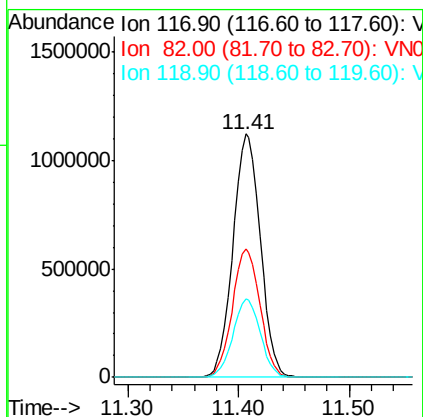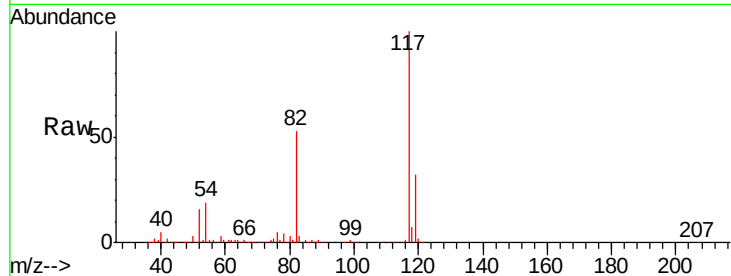

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN052958.D
Acq: 18 Dec 2018 13:50

Tgt Ion:152 Resp: 734880
Ion Ratio Lower Upper
152 100
115 56.3 28.3 85.0
150 157.1 0.0 347.8

