


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN121818\
 Data File : VN052950.D
 Acq On : 18 Dec 2018 8:28
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Title : SW846 8260
 Last Update : Tue Dec 18 13:03:37 2018

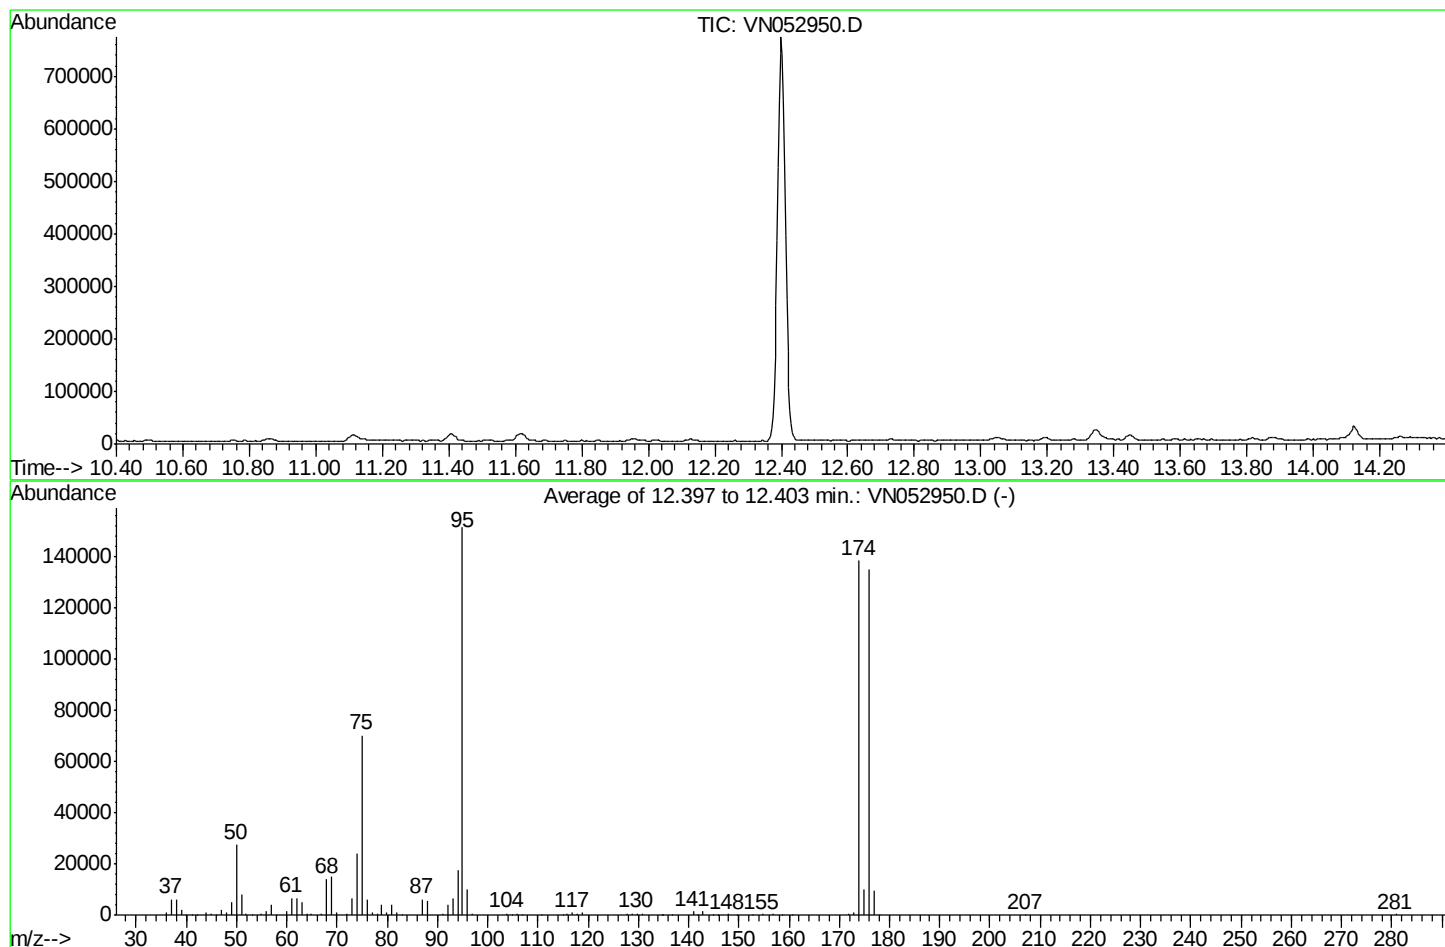

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	27466	PASS
75	95	30	60	46.2	70117	PASS
95	95	100	100	100.0	151616	PASS
96	95	5	9	6.6	9988	PASS
173	174	0.00	2	0.8	1144	PASS
174	95	50	100	91.3	138496	PASS
175	174	5	9	7.3	10101	PASS
176	174	95	101	97.5	134976	PASS
177	176	5	9	7.1	9537	PASS