


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN121818\
Data File : VN052973.D
Acq On : 18 Dec 2018 21:04
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Title : SW846 8260
Last Update : Tue Dec 18 13:03:37 2018

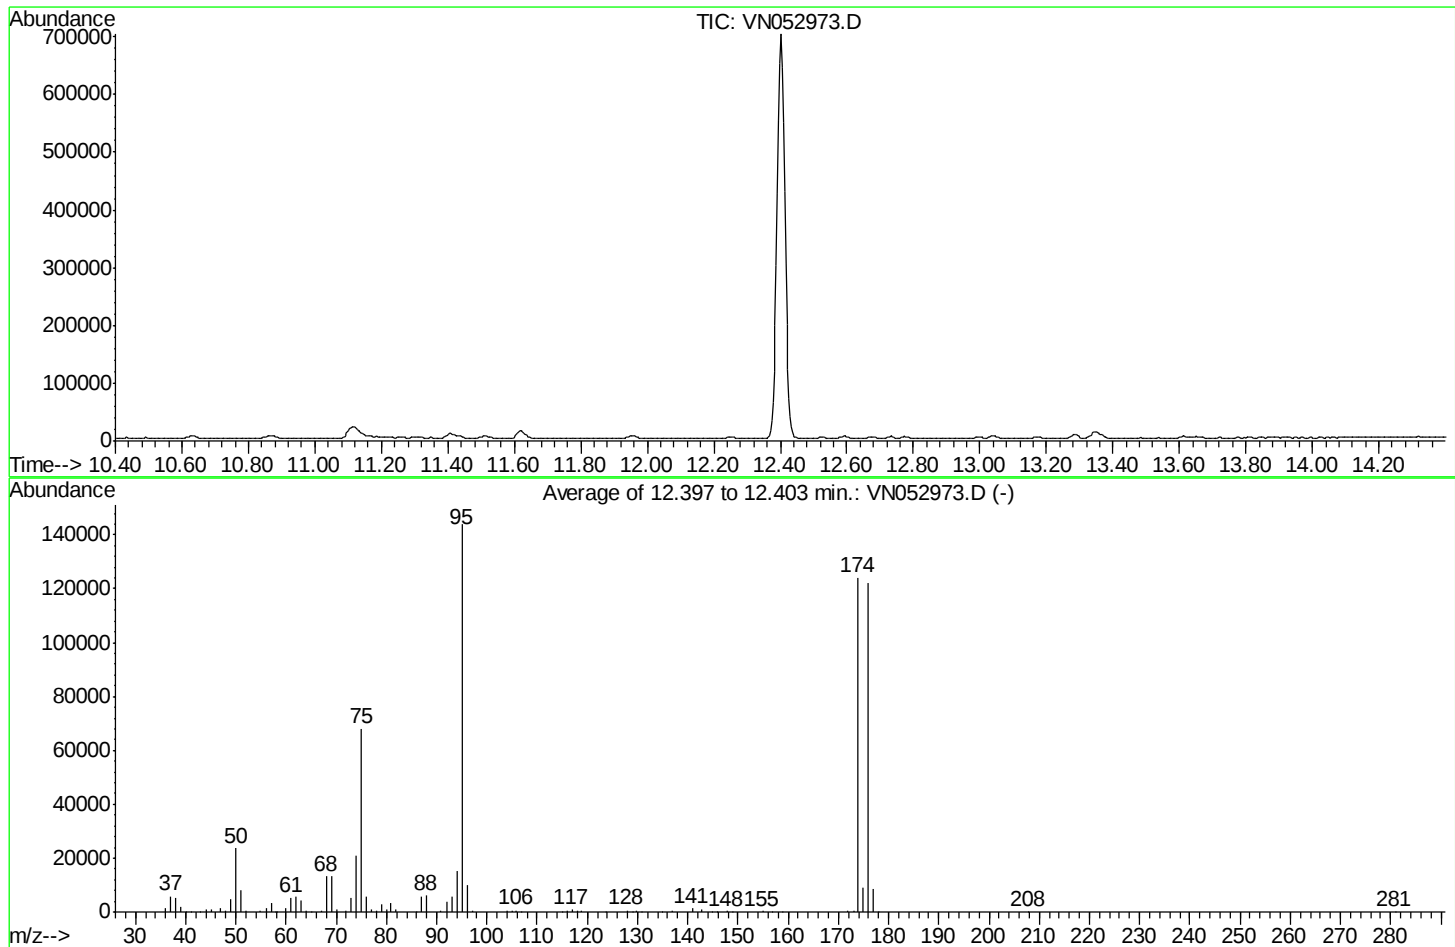

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	23714	PASS
75	95	30	60	47.4	68189	PASS
95	95	100	100	100.0	143914	PASS
96	95	5	9	6.8	9774	PASS
173	174	0.00	2	0.6	707	PASS
174	95	50	100	86.2	124101	PASS
175	174	5	9	7.4	9220	PASS
176	174	95	101	98.6	122328	PASS
177	176	5	9	6.8	8355	PASS