


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121819\
Data File : VN059644.D
Acq On : 18 Dec 2019 10:04
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
Title : SW846 8260
Last Update : Fri Dec 13 23:17:39 2019

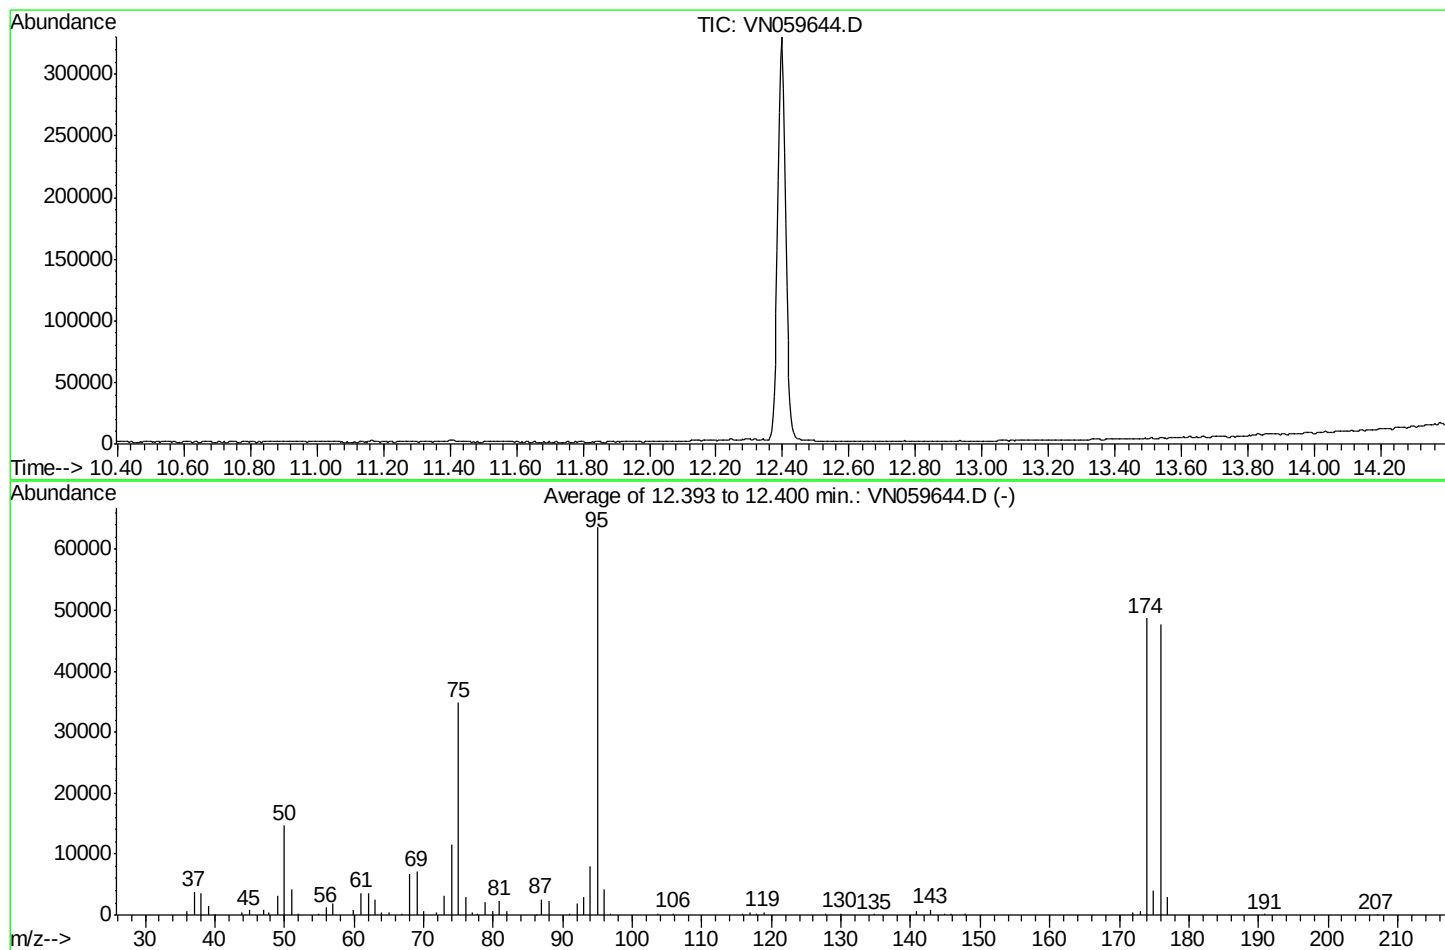

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	14634	PASS
75	95	30	60	54.7	34805	PASS
95	95	100	100	100.0	63600	PASS
96	95	5	9	6.7	4292	PASS
173	174	0.00	2	1.1	548	PASS
174	95	50	100	76.5	48642	PASS
175	174	5	9	8.3	4058	PASS
176	174	95	101	98.1	47736	PASS
177	176	5	9	6.3	3030	PASS