

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121821\
 Data File : VN070213.D
 Acq On : 18 Dec 2021 15:10
 Operator : JC/MD
 Sample : M5044-04 10X
 Misc : 5.64g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 9 Sample Multiplier: 1


Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 19 08:46:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 03 08:46:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.083	168	1169614	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2253005	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2789322	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	1239856	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	928071	51.391	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 102.780%			
35) Dibromofluoromethane	8.021	113	648559	45.957	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 91.920%			
50) Toluene-d8	10.440	98	3082607	54.400	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 108.800%			
62) 4-Bromofluorobenzene	12.731	95	1487429	72.456	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 144.920%#			
Target Compounds						
					Qvalue	
5) Bromomethane	2.821	94	2925	0.343	ug/l #	54
11) Tert butyl alcohol	5.312	59	15718	4.605	ug/l #	71
16) Acetone	4.291	43	8478	0.780	ug/l	94
25) 2-Butanone	7.340	43	7179	0.486	ug/l #	79
31) Cyclohexane	8.078	56	51946	2.067	ug/l #	56
36) 1,1-Dichloropropene	8.083	75	98204	4.579	ug/l #	49
38) Carbon Tetrachloride	8.083	117	118205	5.620	ug/l #	16
39) Methylcyclohexane	9.459	83	36491	1.430	ug/l #	36
43) Isopropyl Acetate	8.558	43	15789	0.334	ug/l #	55
48) Methyl methacrylate	9.593	41	19544	0.887	ug/l #	27
49) 1,4-Dioxane	9.585	88	152	0.384	ug/l #	1
51) 4-Methyl-2-Pentanone	10.371	43	69585	2.271	ug/l #	81
53) t-1,3-Dichloropropene	10.711	75	254	2.803	ug/l #	43
54) cis-1,3-Dichloropropene	10.194	75	106	2.002	ug/l #	1
55) 1,1,2-Trichloroethane	10.878	97	35862	2.221	ug/l #	39
56) Ethyl methacrylate	10.778	69	5597	2.454	ug/l #	48
58) 2-Chloroethyl Vinyl ether	10.017	63	1070	18.509	ug/l #	45
59) 2-Hexanone	11.052	43	54057	2.332	ug/l #	26
60) Dibromochloromethane	11.140	129	78	2.381	ug/l	87
67) Ethyl Benzene	11.843	91	22151	0.215	ug/l	100
71) Bromoform	12.709	173	502	2.759	ug/l #	29
74) N-amyl acetate	12.366	43	46776	0.959	ug/l #	67
76) 1,2,3-Trichloropropane	12.731	75	813764	22.887	ug/l #	1
78) n-propylbenzene	12.919	91	66621	0.543	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.731	75	813764	72.882	ug/l #	5
85) sec-Butylbenzene	13.501	105	47085	0.442	ug/l #	49
89) n-Butylbenzene	13.940	91	57845	0.855	ug/l	95
90) Hexachloroethane	14.217	117	19670	1.344	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.268	180	3123	3.023	ug/l #	1
95) Naphthalene	15.507	128	18834	4.271	ug/l #	90
96) 1,2,3-Trichlorobenzene	15.708	180	3277	2.593	ug/l #	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed



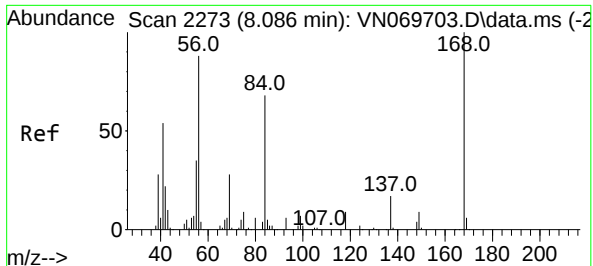


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Instrument :
MSVOA_N
ClientSampleId :



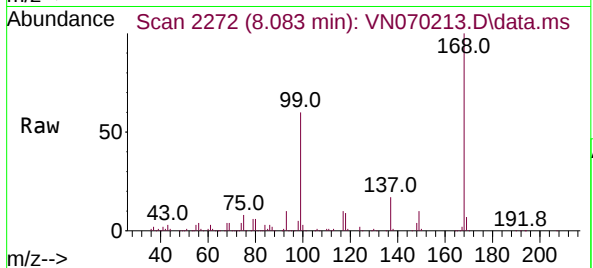



Tgt Ion:168 Resp: 1169614
Ion Ratio Lower Upper
168 100
99 60.2 41.3 61.9

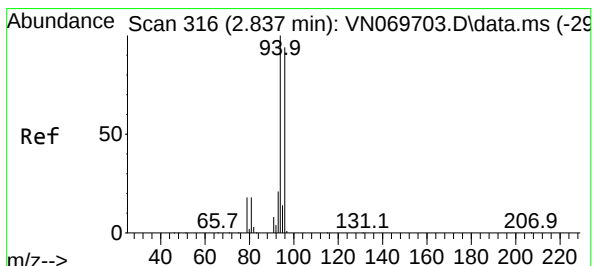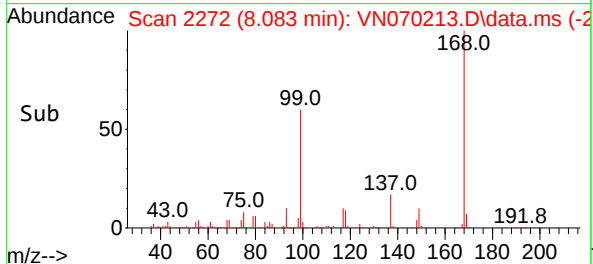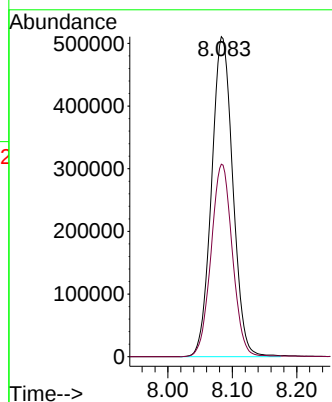

#5
Bromomethane
Concen: 0.343 ug/l
RT: 2.821 min Scan# 310
Delta R.T. -0.016 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 94 Resp: 2925
Ion Ratio Lower Upper
94 100
96 48.4 73.8 110.8#


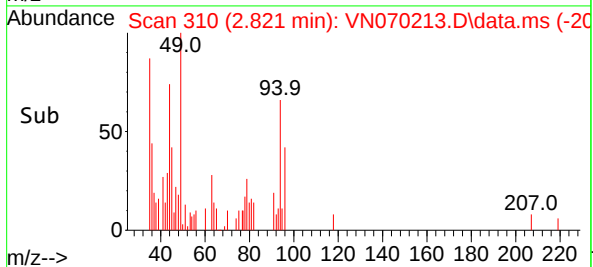
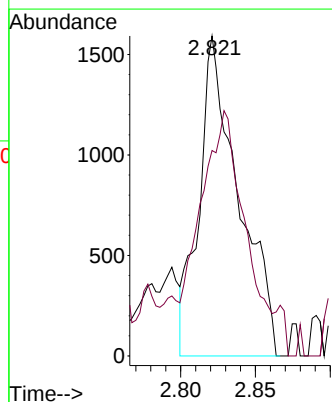
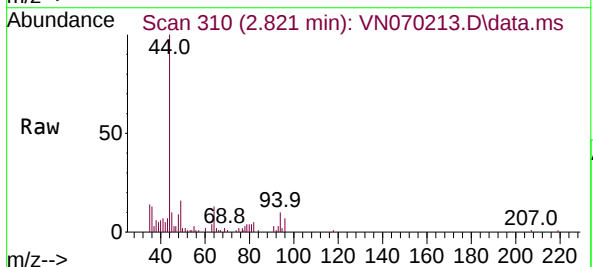




#11
Tert butyl alcohol
Concen: 4.605 ug/l
RT: 5.312 min Scan# 11
Delta R.T. -0.078 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 15718
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

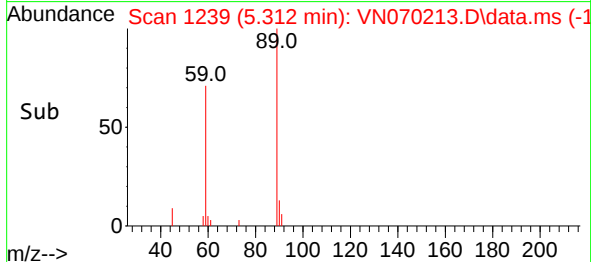

#16
Acetone
Concen: 0.780 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.000 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 43 Resp: 8478
Ion Ratio Lower Upper
43 100
58 32.3 23.1 34.7

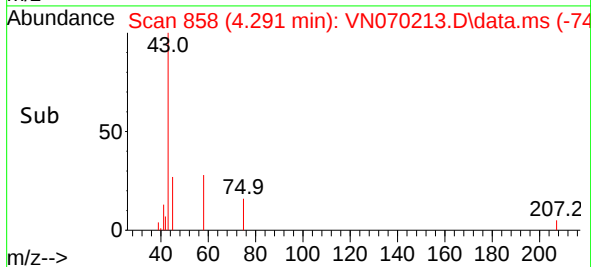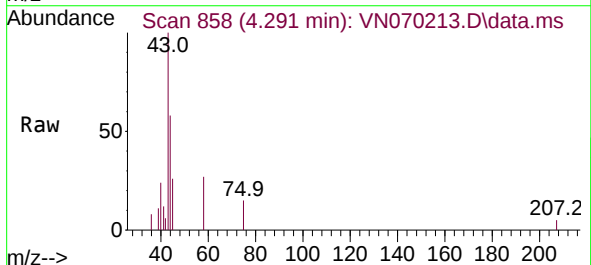



#25

2-Butanone

Concen: 0.486 ug/l

RT: 7.340 min Scan# 1994

Delta R.T. 0.003 min

Lab File: VN070213.D

Acq: 18 Dec 2021 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 7179

Ion Ratio Lower Upper

43 100

72 16.1 21.7 32.5#

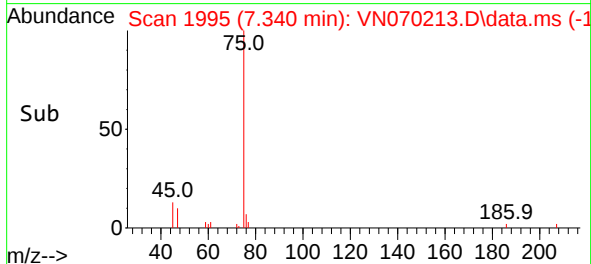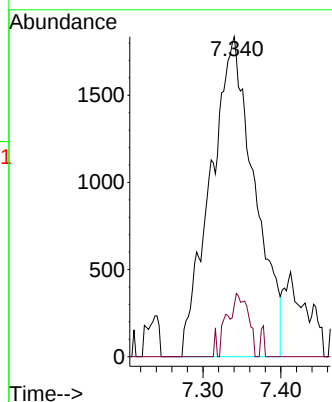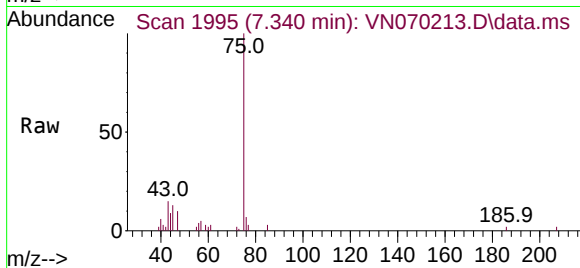

#31

Cyclohexane

Concen: 2.067 ug/l

RT: 8.078 min Scan# 2270

Delta R.T. -0.016 min

Lab File: VN070213.D

Acq: 18 Dec 2021 15:10




Tgt Ion: 56 Resp: 51946


Ion Ratio Lower Upper

56 100

69 100.3 27.1 40.7#

84 75.0 73.4 110.0

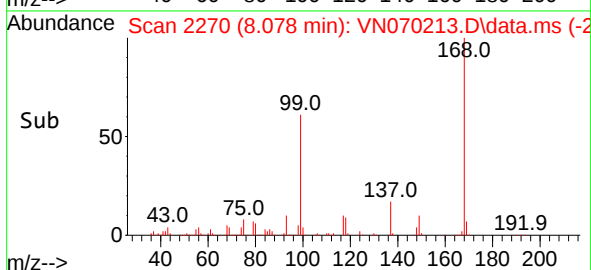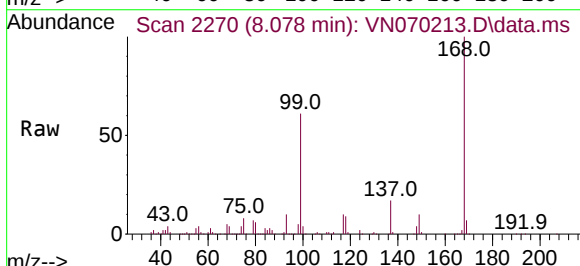



#33

1,2-Dichloroethane-d4

Concen: 51.391 ug/l

RT: 8.437 min Scan# 2404

Delta R.T. 0.000 min

Lab File: VN070213.D

Acq: 18 Dec 2021 15:10

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 928071

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.0

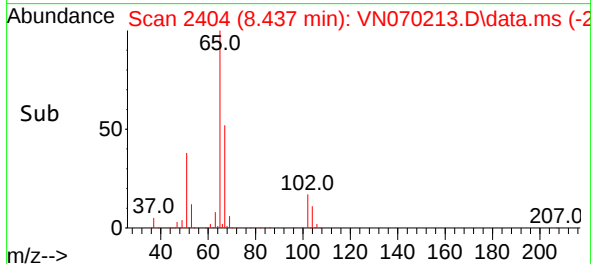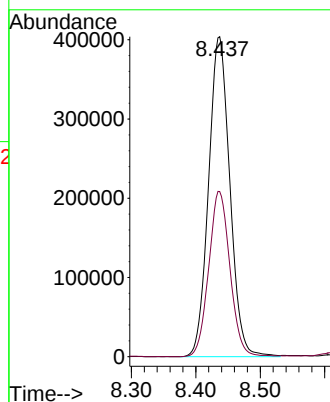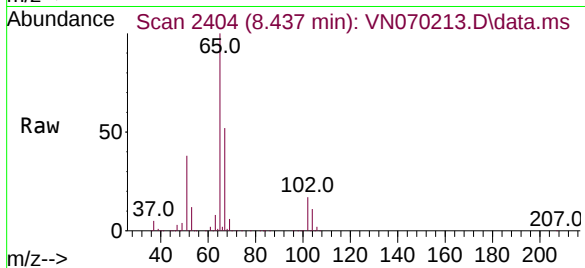

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. 0.000 min

Lab File: VN070213.D

Acq: 18 Dec 2021 15:10




Tgt Ion: 114 Resp: 2253005


Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.6 0.0 27.4


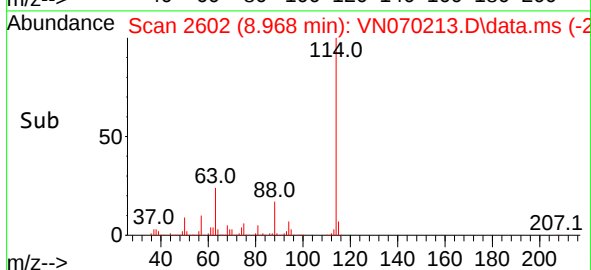
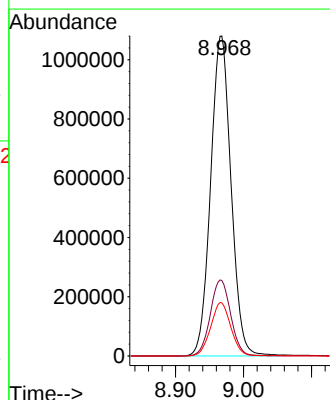
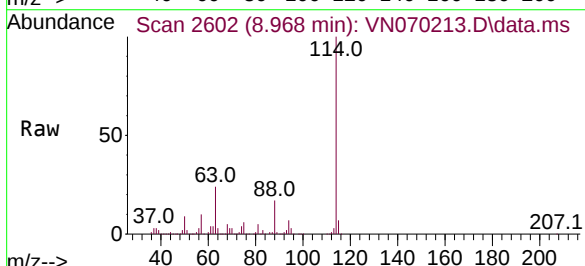




#35
 Dibromofluoromethane
 Concen: 45.957 ug/l
 RT: 8.021 min Scan# 2113
 Delta R.T. -0.003 min
 Lab File: VN070213.D
 Acq: 18 Dec 2021 15:10




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:113 Resp: 648559
 Ion Ratio Lower Upper
 113 100
 111 103.6 82.2 123.2
 192 18.9 16.9 25.3

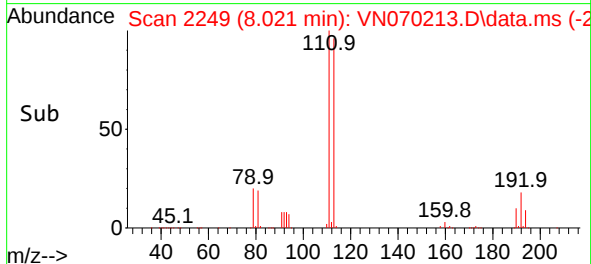

#36
 1,1-Dichloropropene
 Concen: 4.579 ug/l
 RT: 8.083 min Scan# 2272
 Delta R.T. -0.139 min
 Lab File: VN070213.D
 Acq: 18 Dec 2021 15:10


Tgt Ion: 75 Resp: 98204
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.4 55.2#
 77 0.0 24.4 36.6#

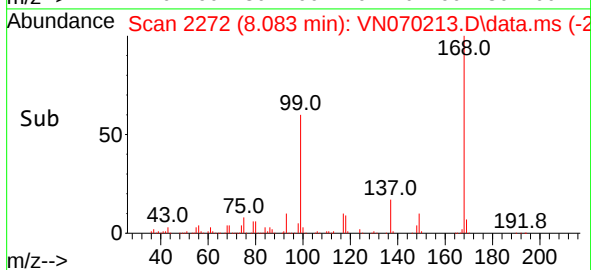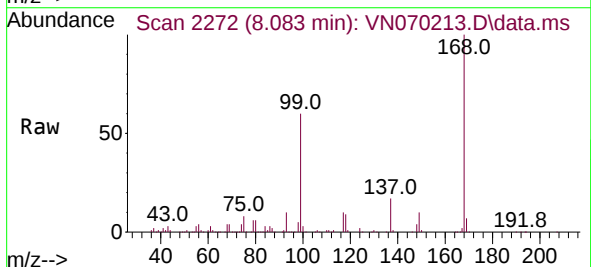






#38
Carbon Tetrachloride
Concen: 5.620 ug/l
RT: 8.083 min Scan# 211
Delta R.T. -0.123 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 118205
Ion Ratio Lower Upper
117 100
119 5.3 76.1 114.1#
121 0.0 24.2 36.2#

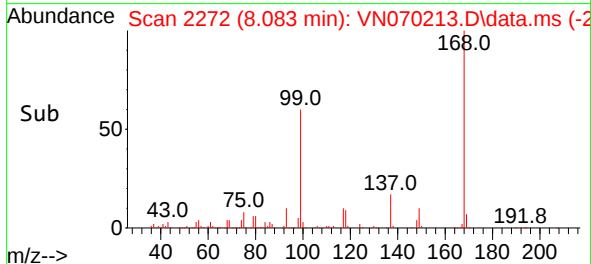

#39
Methylcyclohexane
Concen: 1.430 ug/l
RT: 9.459 min Scan# 2785
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 83 Resp: 36491
Ion Ratio Lower Upper
83 100
55 159.7 58.1 87.1#
98 50.7 38.4 57.6


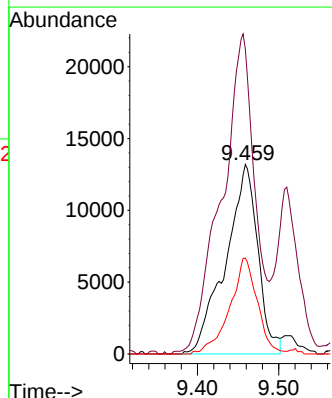
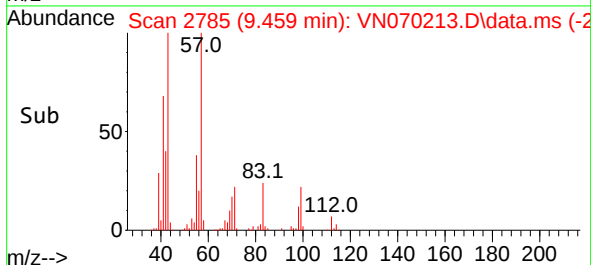
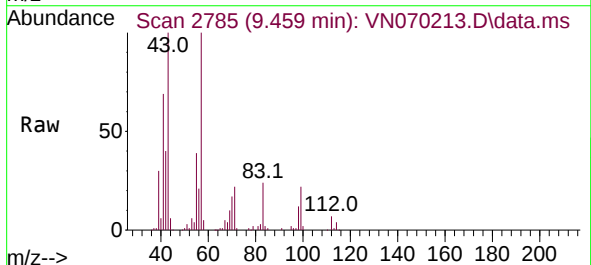


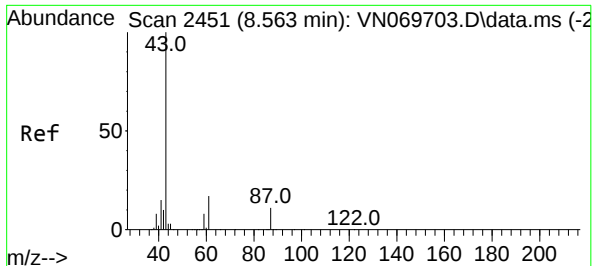

#43
Isopropyl Acetate
Concen: 0.334 ug/l
RT: 8.558 min Scan# 2449
Delta R.T. -0.005 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 15789
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#

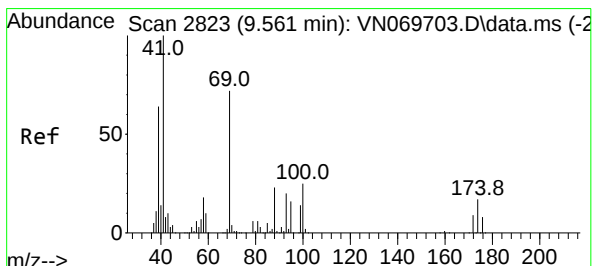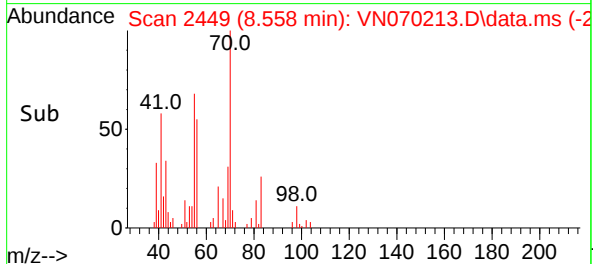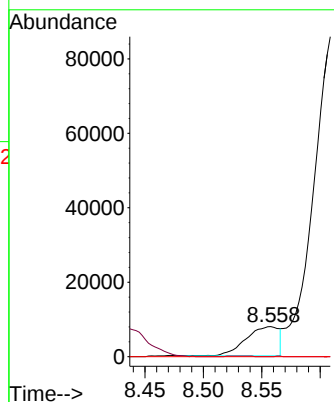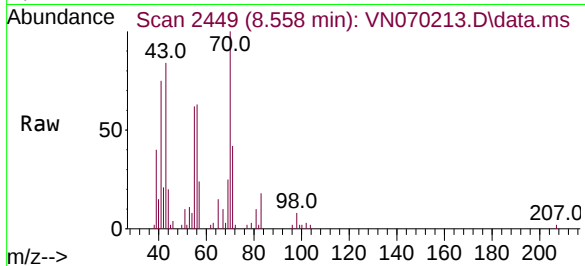

#48
Methyl methacrylate
Concen: 0.887 ug/l
RT: 9.593 min Scan# 2835
Delta R.T. 0.032 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 41 Resp: 19544
Ion Ratio Lower Upper
41 100
69 2.9 72.4 108.6#
39 31.4 58.4 87.6#

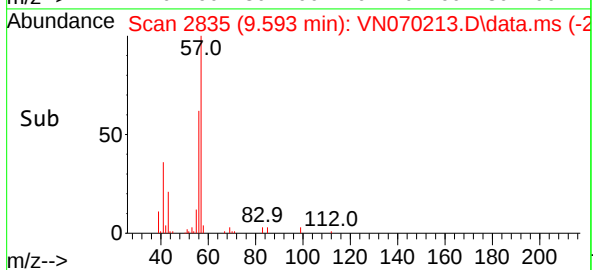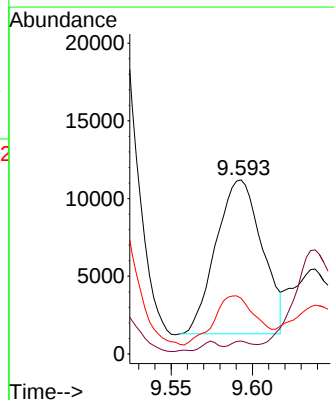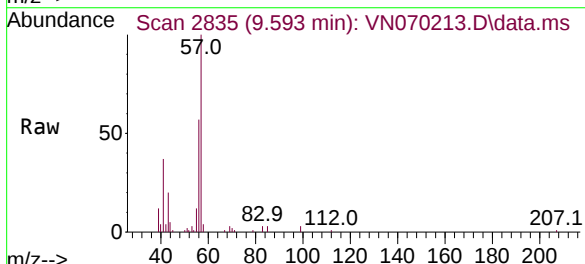



#49

1,4-Dioxane

Concen: 0.384 ug/l

RT: 9.585 min Scan# 21

Delta R.T. 0.014 min

Lab File: VN070213.D

Acq: 18 Dec 2021 15:10





Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion: 88 Resp: 152

Ion	Ratio	Lower	Upper
88	100		
43	8728.3	23.4	35.2#
58	2042.1	50.6	75.8#

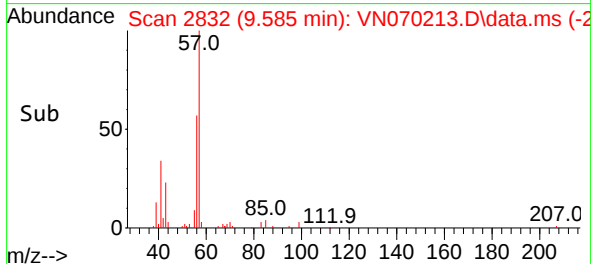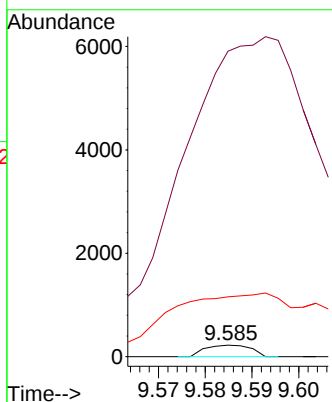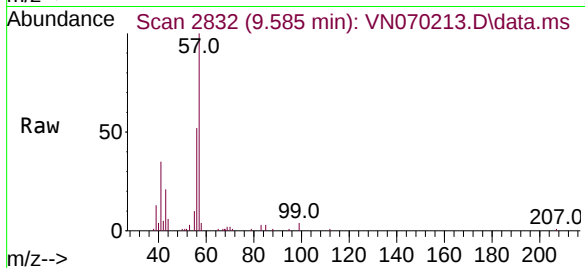

#50

Toluene-d8

Concen: 54.400 ug/l

RT: 10.440 min Scan# 3151




Delta R.T. -0.003 min


Lab File: VN070213.D

Acq: 18 Dec 2021 15:10

Tgt Ion: 98 Resp: 3082607

Ion	Ratio	Lower	Upper
98	100		
100	64.0	50.4	75.6




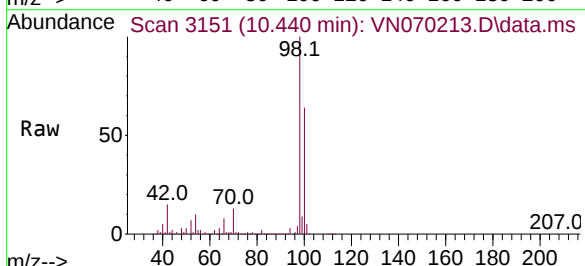




#51
4-Methyl-2-Pentanone
Concen: 2.271 ug/l
RT: 10.371 min Scan# 3111
Delta R.T. 0.038 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 69585
Ion Ratio Lower Upper
43 100
58 26.6 30.4 45.6#

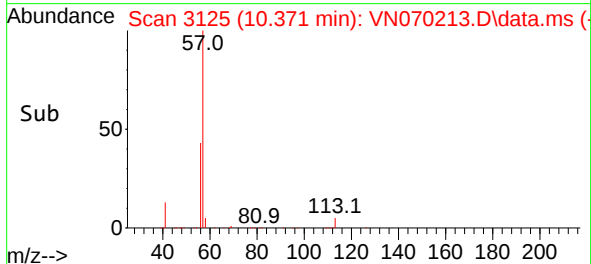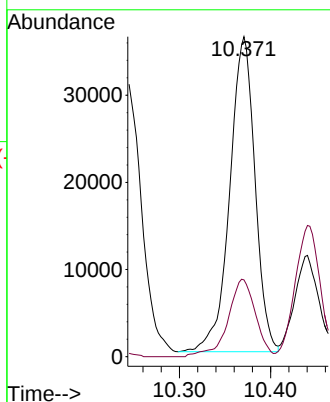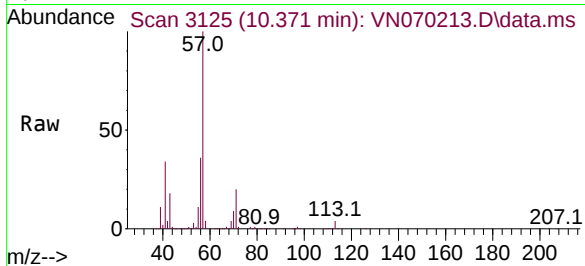

#53
t-1,3-Dichloropropene
Concen: 2.803 ug/l
RT: 10.711 min Scan# 3252
Delta R.T. -0.008 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 75 Resp: 254
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#


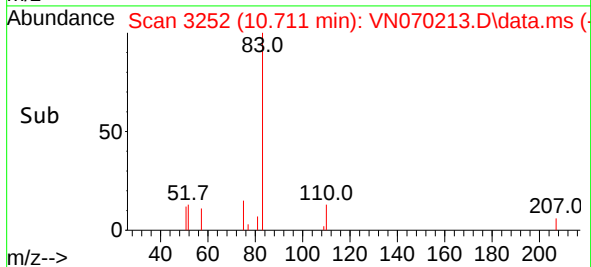
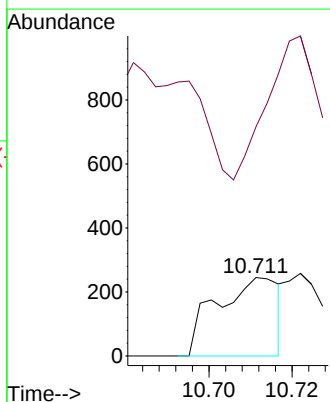
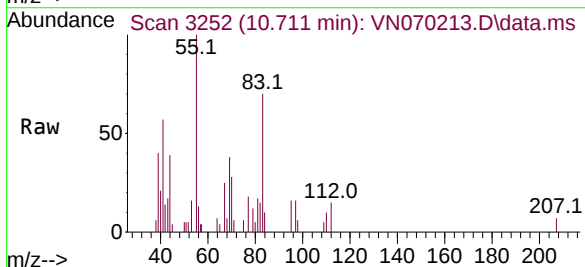




#54
cis-1,3-Dichloropropene
Concen: 2.002 ug/l
RT: 10.194 min Scan# 3058
Delta R.T. 0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 106
Ion Ratio Lower Upper
75 100
77 2.5 26.4 39.6#
39 223.3 42.5 63.7#

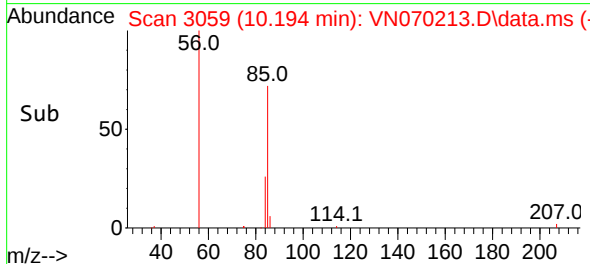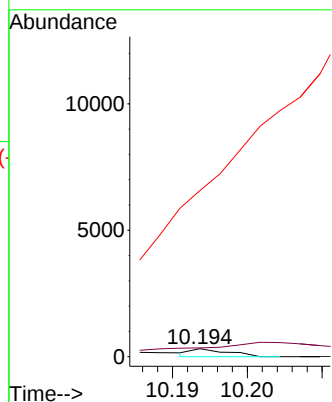

#55
1,1,2-Trichloroethane
Concen: 2.221 ug/l
RT: 10.878 min Scan# 3314
Delta R.T. -0.021 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 97 Resp: 35862
Ion Ratio Lower Upper
97 100
83 10.7 67.8 101.6#
85 50.1 45.4 68.2
99 0.0 49.4 74.0#


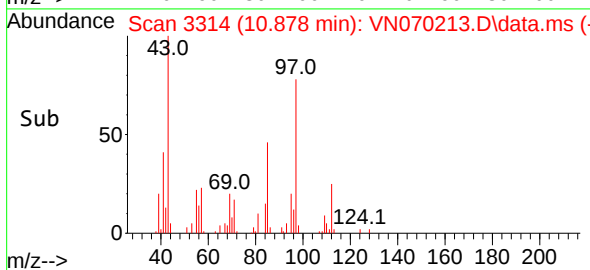

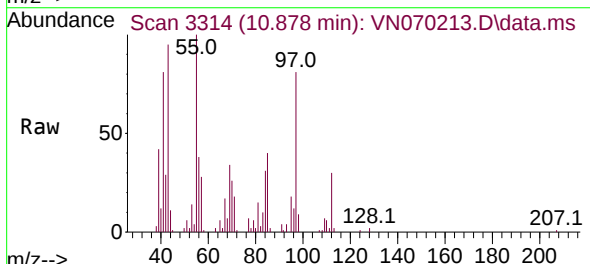




#56
Ethyl methacrylate
Concen: 2.454 ug/l
RT: 10.778 min Scan# 31
Delta R.T. 0.016 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 5597
Ion Ratio Lower Upper
69 100
41 103.7 51.4 77.0#
39 78.5 34.6 52.0#

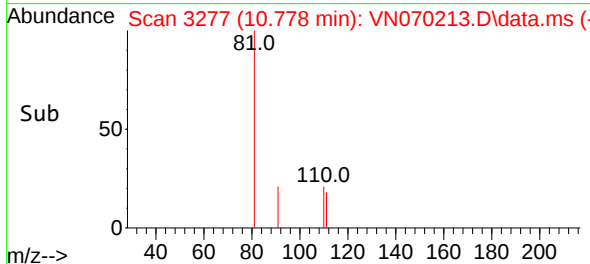

#58
2-Chloroethyl Vinyl ether
Concen: 18.509 ug/l
RT: 10.017 min Scan# 2993
Delta R.T. -0.026 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 63 Resp: 1070
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#




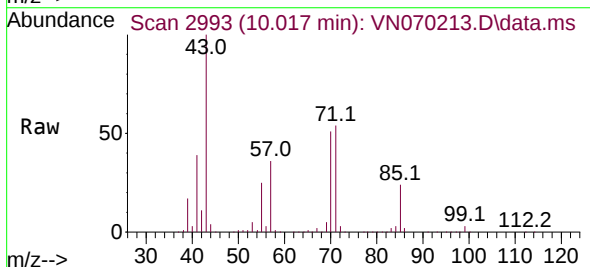




#59
2-Hexanone
Concen: 2.332 ug/l
RT: 11.052 min Scan# 31
Delta R.T. -0.035 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 54057
Ion Ratio Lower Upper
43 100
58 0.6 26.9 80.7#

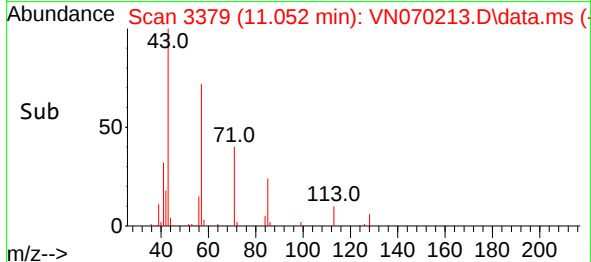

#60
Dibromochloromethane
Concen: 2.381 ug/l
RT: 11.140 min Scan# 3412
Delta R.T. -0.100 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 129 Resp: 78
Ion Ratio Lower Upper
129 100
127 88.5 38.6 116.0


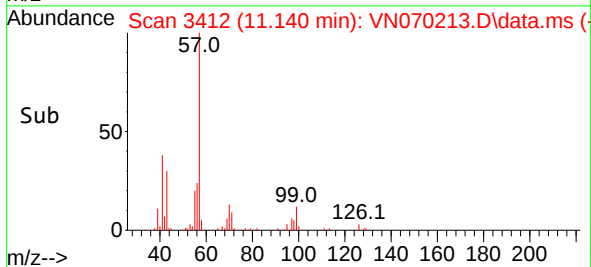

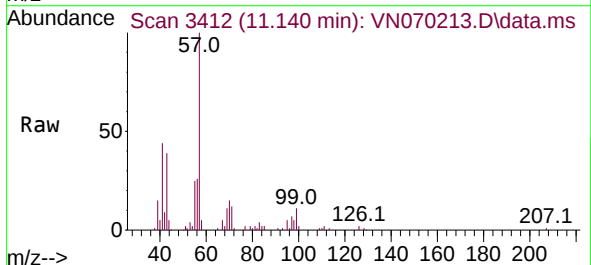




#62
4-Bromofluorobenzene
Concen: 72.456 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 1487429
Ion Ratio Lower Upper
95 100
174 74.7 0.0 187.2
176 72.2 0.0 181.4

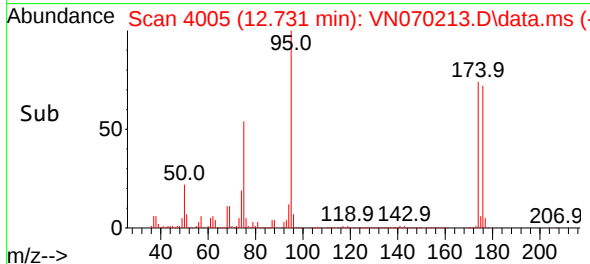

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.002 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 117 Resp: 2789322
Ion Ratio Lower Upper
117 100
82 60.0 42.4 63.6
119 32.1 25.4 38.2


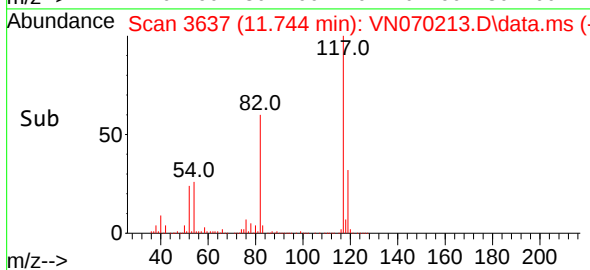

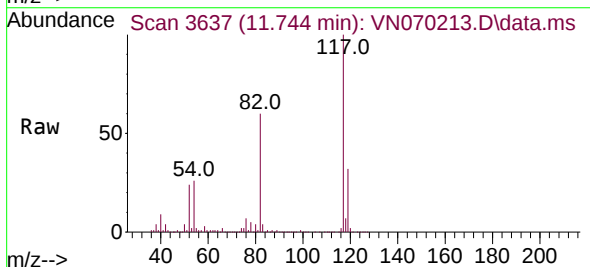




#67
Ethyl Benzene
Concen: 0.215 ug/l
RT: 11.843 min Scan# 30
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 22151
Ion Ratio Lower Upper
91 100
106 32.1 25.7 38.5

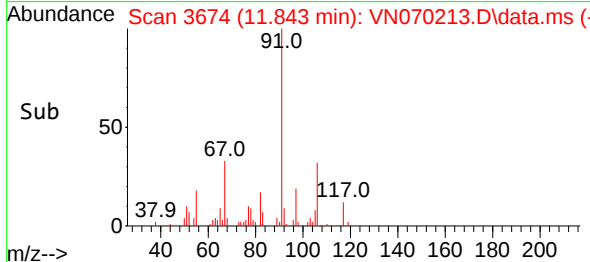

#71
Bromoform
Concen: 2.759 ug/l
RT: 12.709 min Scan# 3997
Delta R.T. 0.249 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10


Tgt Ion:173 Resp: 502
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

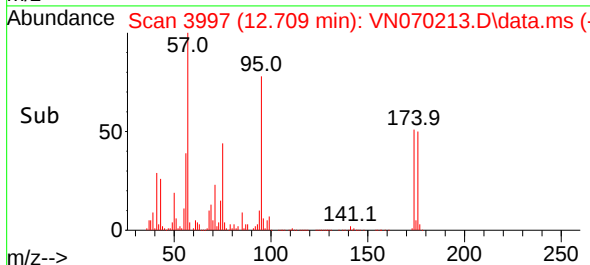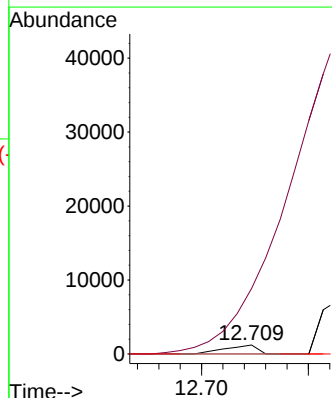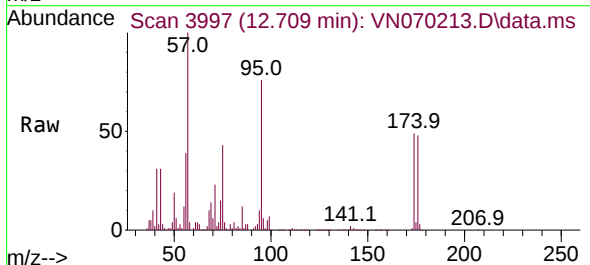






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:152 Resp: 1239856
Ion Ratio Lower Upper
152 100
115 60.8 27.5 82.5
150 155.7 0.0 344.4

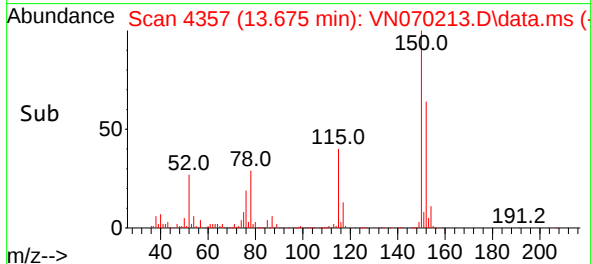

#74
N-ethyl acetate
Concen: 0.959 ug/l
RT: 12.366 min Scan# 3869
Delta R.T. -0.021 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 43 Resp: 46776
Ion Ratio Lower Upper
43 100
70 15.6 33.4 50.0#
55 22.6 19.3 28.9
61 0.0 18.5 27.7#


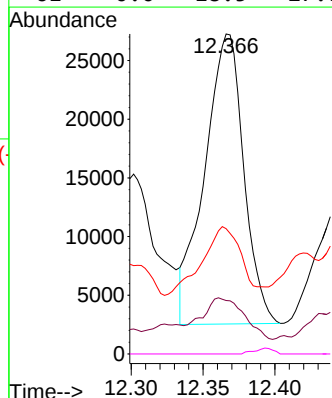
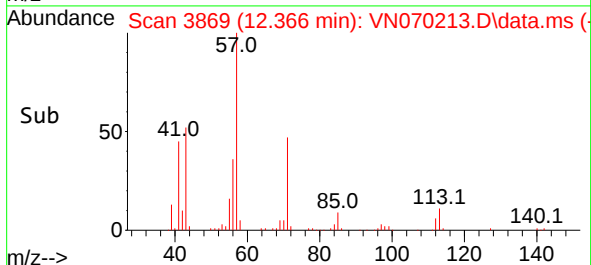
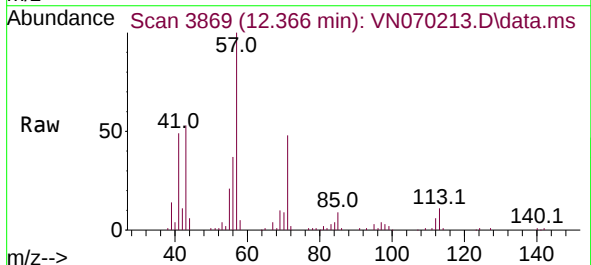




#76
1,2,3-Trichloropropane
Concen: 22.887 ug/l
RT: 12.731 min Scan# 4061
Delta R.T. -0.150 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 813764
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#

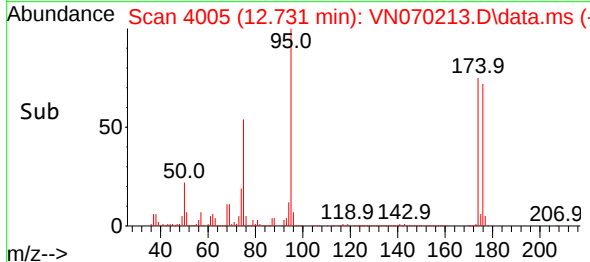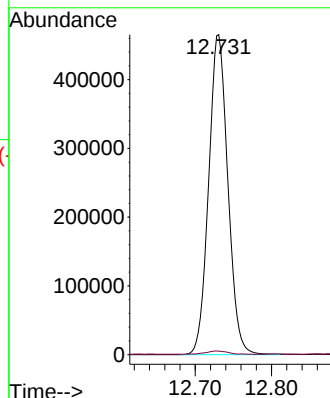

#78
n-propylbenzene
Concen: 0.543 ug/l
RT: 12.919 min Scan# 4075
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10


Tgt Ion: 91 Resp: 66621
Ion Ratio Lower Upper
91 100
120 22.6 11.9 35.9

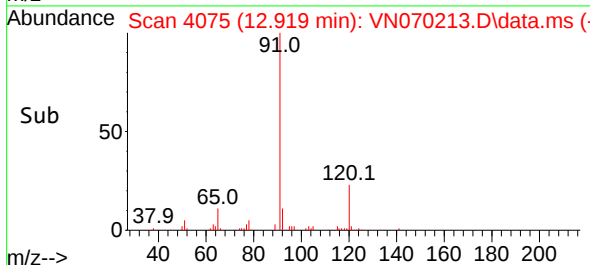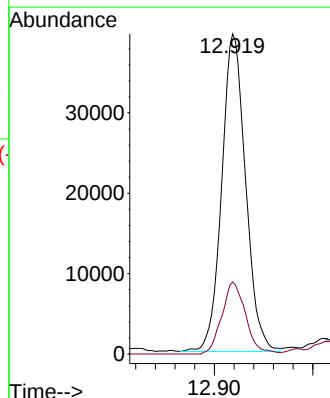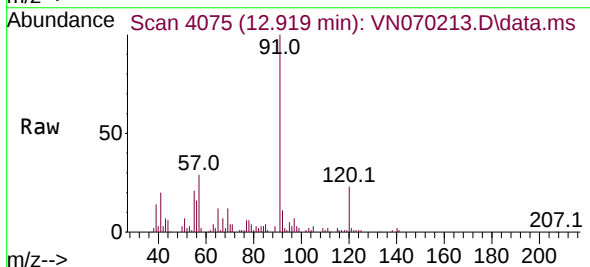






#81
trans-1,4-Dichloro-2-butene
Concen: 72.882 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 813764
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

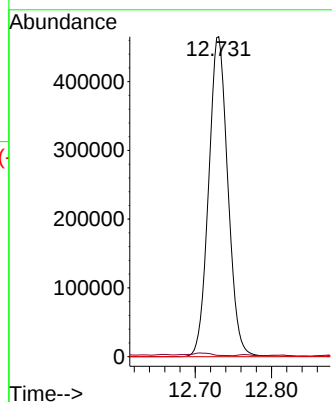

#85
sec-Butylbenzene
Concen: 0.442 ug/l
RT: 13.501 min Scan# 4292
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

Tgt Ion: 105 Resp: 47085
Ion Ratio Lower Upper
105 100
134 44.3 10.4 31.1#



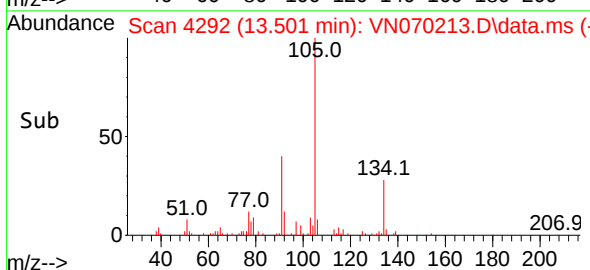





#89
n-Butylbenzene
Concen: 0.855 ug/l
RT: 13.940 min Scan# 4457
Delta R.T. -0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 57845
Ion Ratio Lower Upper
91 100
92 46.0 25.4 76.0
134 26.6 13.6 40.8

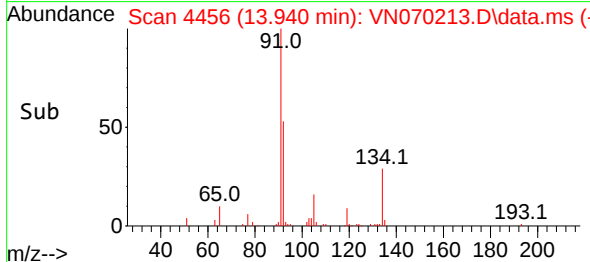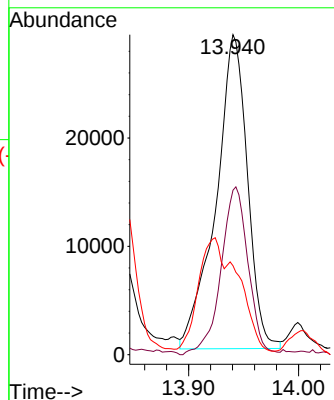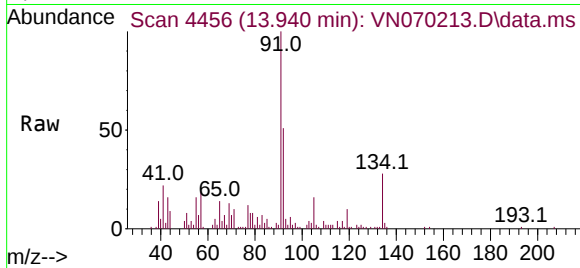

#90
Hexachloroethane
Concen: 1.344 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.005 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10


Tgt Ion: 117 Resp: 19670
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

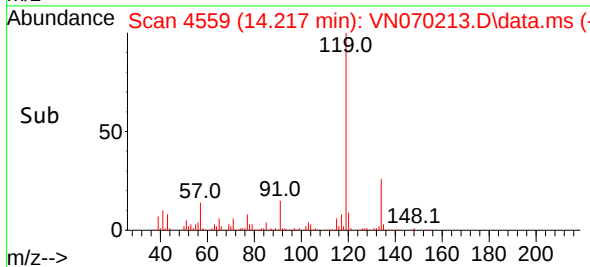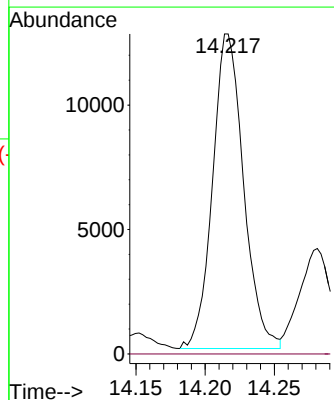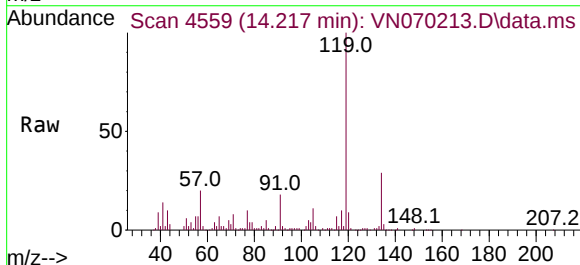






#93
1,2,4-Trichlorobenzene
Concen: 3.023 ug/l
RT: 15.268 min Scan# 4950
Delta R.T. 0.003 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:180 Resp: 3123
Ion Ratio Lower Upper
180 100
182 96.5 48.3 144.9
145 397.1 14.5 43.5#

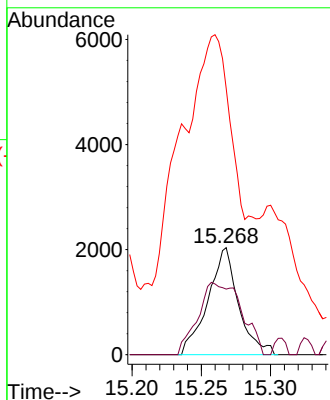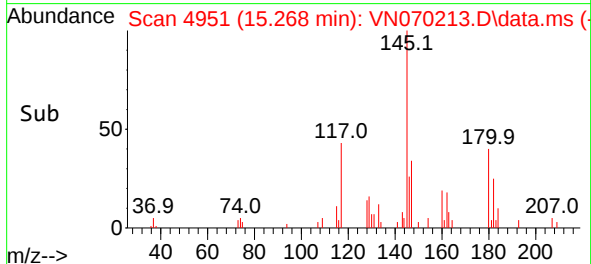


#95
Naphthalene
Concen: 4.271 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN070213.D
Acq: 18 Dec 2021 15:10

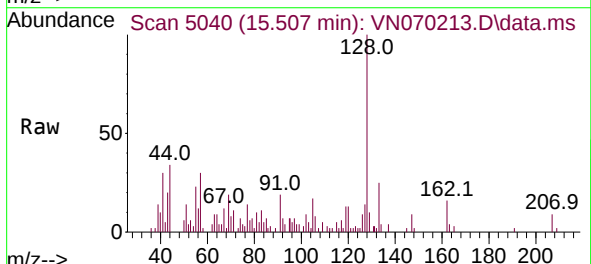

Tgt Ion:128 Resp: 18834
Ion Ratio Lower Upper
128 100
127 15.6 10.5 15.7
129 5.8 8.7 13.1#

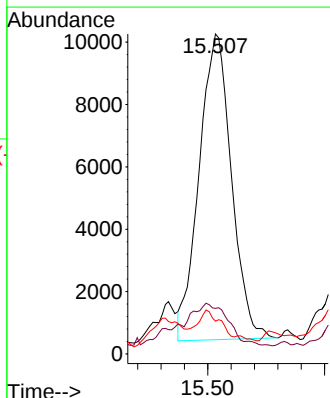



#96

1,2,3-Trichlorobenzene

Concen: 2.593 ug/l

RT: 15.708 min Scan# 51

Delta R.T. 0.006 min


Lab File: VN070213.D

Acq: 18 Dec 2021 15:10

Instrument :

MSVOA_N

ClientSampleId :

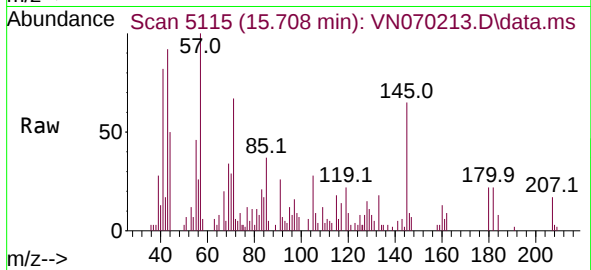

Tgt Ion:180 Resp: 3277

Ion Ratio Lower Upper

180 100

182 59.0 47.4 142.2

145 0.0 15.0 45.1#

