
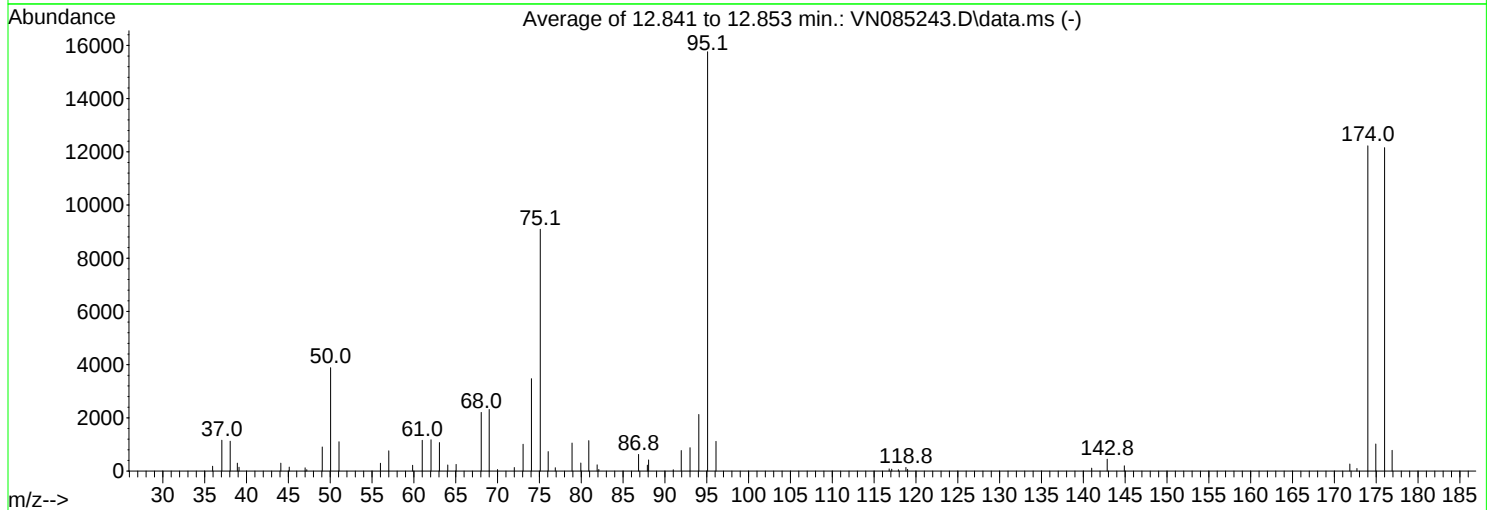


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121824\  
Data File : VN085243.D  
Acq On : 18 Dec 2024 08:37  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121824W.M  
Title : SW846 8260  
Last Update : Thu Dec 19 06:31:00 2024

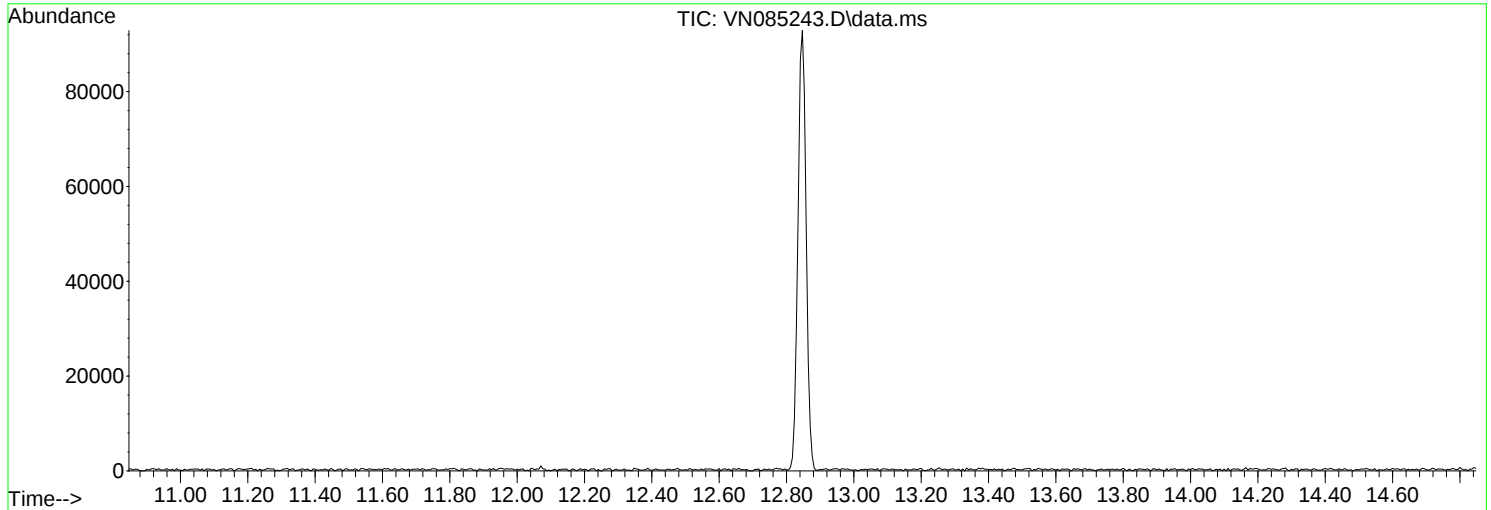

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 24.7         | 3887       | PASS                |
| 75             | 95              | 30              | 60              | 57.7         | 9090       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 15762      | PASS                |
| 96             | 95              | 5               | 9               | 7.1          | 1117       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.8          | 97         | PASS                |
| 174            | 95              | 50              | 100             | 77.6         | 12225      | PASS                |
| 175            | 174             | 5               | 9               | 8.3          | 1018       | PASS                |
| 176            | 174             | 95              | 101             | 99.4         | 12157      | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 780        | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z    | abund. |
|-------|--------|-------|--------|-------|--------|--------|--------|
| 35.95 | 183    | 51.05 | 1103   | 70.00 | 57     | 82.10  | 62     |
| 37.05 | 1160   | 56.00 | 295    | 72.00 | 134    | 86.85  | 627    |
| 38.05 | 1122   | 57.00 | 762    | 73.05 | 1008   | 87.90  | 225    |
| 38.90 | 298    | 59.85 | 218    | 74.05 | 3473   | 88.05  | 418    |
| 39.10 | 144    | 61.00 | 1157   | 75.10 | 9090   | 91.00  | 50     |
| 44.10 | 297    | 62.05 | 1176   | 76.05 | 733    | 91.95  | 772    |
| 45.10 | 149    | 63.05 | 1071   | 76.90 | 126    | 93.00  | 879    |
| 47.00 | 123    | 64.05 | 229    | 78.90 | 1054   | 94.05  | 2127   |
| 47.20 | 52     | 65.05 | 250    | 79.95 | 303    | 95.10  | 15762  |
| 49.05 | 906    | 68.05 | 2205   | 80.90 | 1144   | 96.10  | 1117   |
| 50.05 | 3887   | 69.00 | 2317   | 81.90 | 235    | 116.80 | 83     |

Average of 12.841 to 12.853 min.: VN085243.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z | abund. | m/z | abund. |
|--------|--------|--------|--------|-----|--------|-----|--------|
| 117.10 | 72     | 176.00 | 12157  |     |        |     |        |
| 117.90 | 53     | 176.90 | 780    |     |        |     |        |
| 118.80 | 138    |        |        |     |        |     |        |
| 119.00 | 65     |        |        |     |        |     |        |
| 141.00 | 111    |        |        |     |        |     |        |
| 142.85 | 447    |        |        |     |        |     |        |
| 144.90 | 198    |        |        |     |        |     |        |
| 171.85 | 266    |        |        |     |        |     |        |
| 172.70 | 97     |        |        |     |        |     |        |
| 174.00 | 12225  |        |        |     |        |     |        |
| 174.95 | 1018   |        |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB