


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121918\
 Data File : VN052996.D
 Acq On : 19 Dec 2018 8:21
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Title : SW846 8260
 Last Update : Tue Dec 18 13:03:37 2018

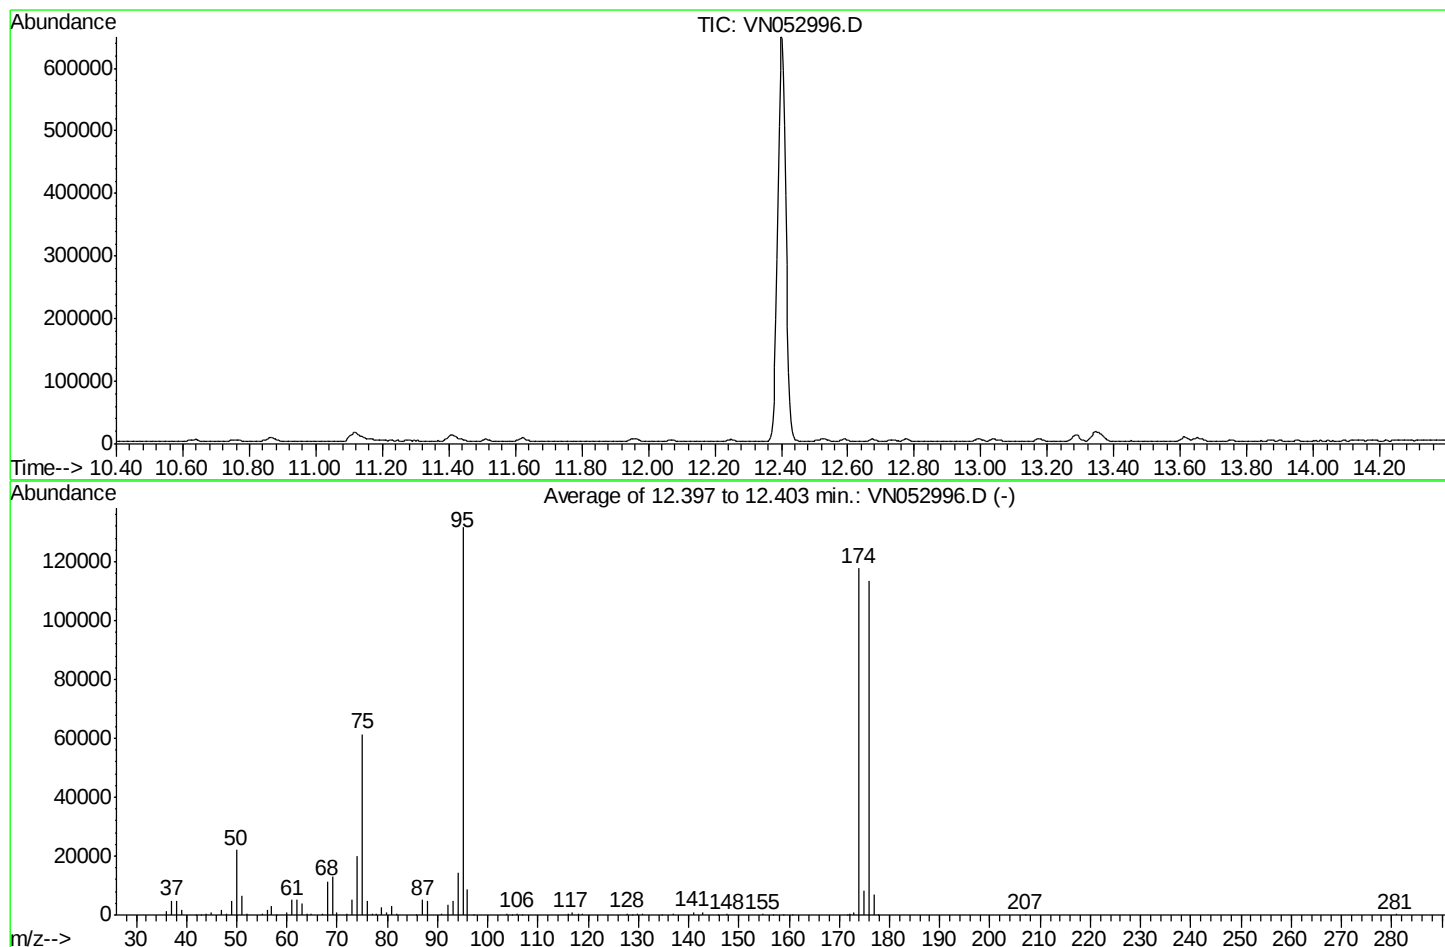

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	22138	PASS
75	95	30	60	46.7	61504	PASS
95	95	100	100	100.0	131661	PASS
96	95	5	9	6.5	8506	PASS
173	174	0.00	2	0.8	931	PASS
174	95	50	100	89.3	117608	PASS
175	174	5	9	6.9	8147	PASS
176	174	95	101	96.7	113677	PASS
177	176	5	9	6.3	7155	PASS