


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN121919\
 Data File : VN059663.D
 Acq On : 19 Dec 2019 9:30
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121319W.M
 Title : SW846 8260
 Last Update : Fri Dec 13 23:17:39 2019

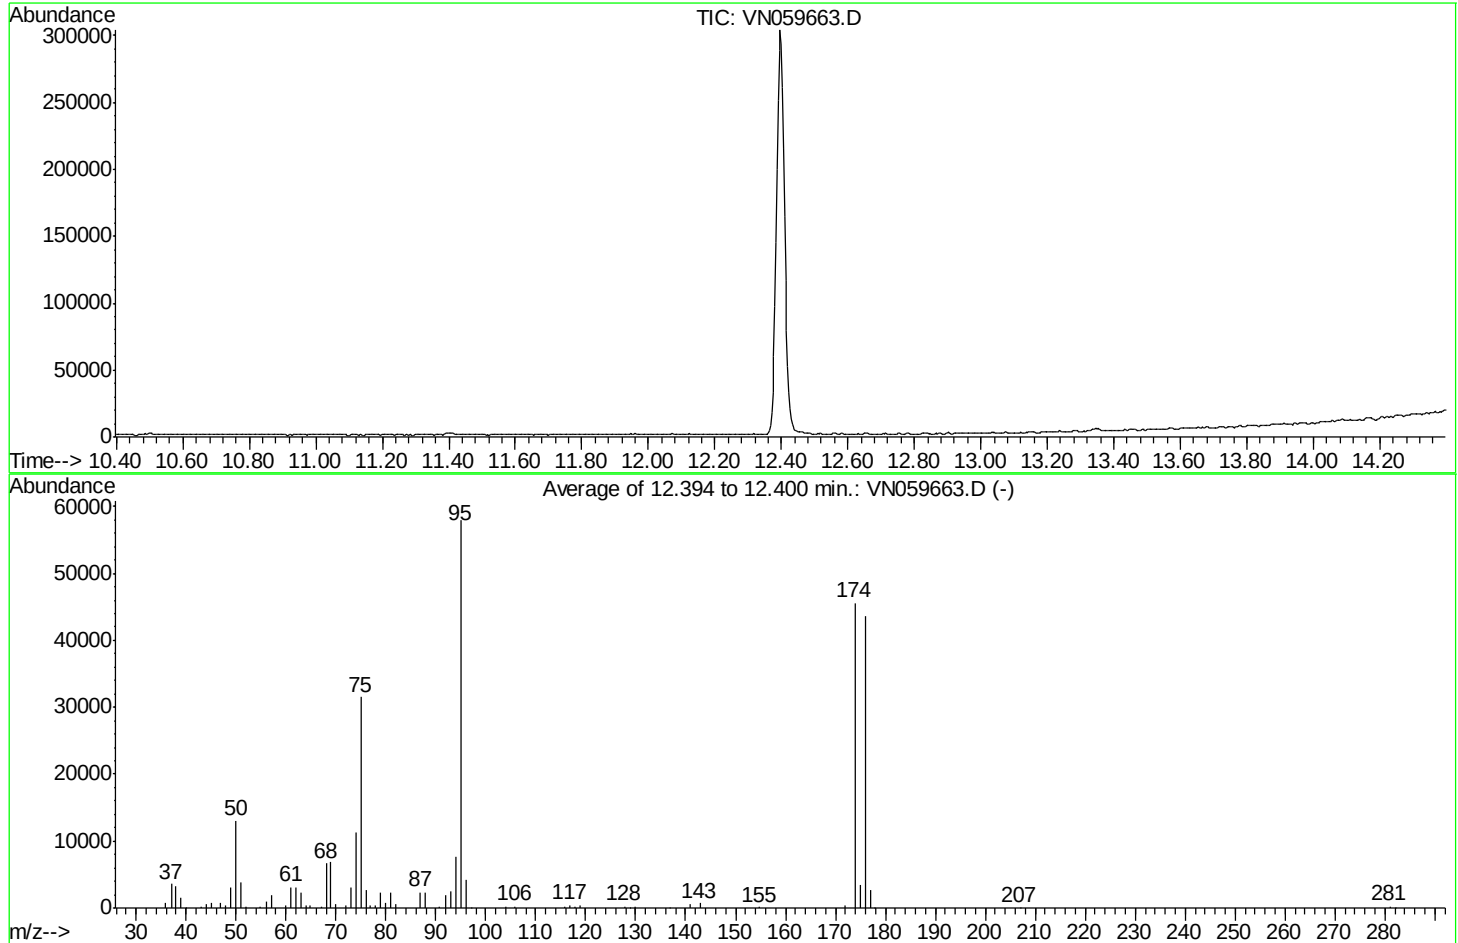

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	13022	PASS
75	95	30	60	54.4	31541	PASS
95	95	100	100	100.0	57941	PASS
96	95	5	9	7.2	4196	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.7	45605	PASS
175	174	5	9	7.6	3446	PASS
176	174	95	101	95.6	43576	PASS
177	176	5	9	6.0	2603	PASS