
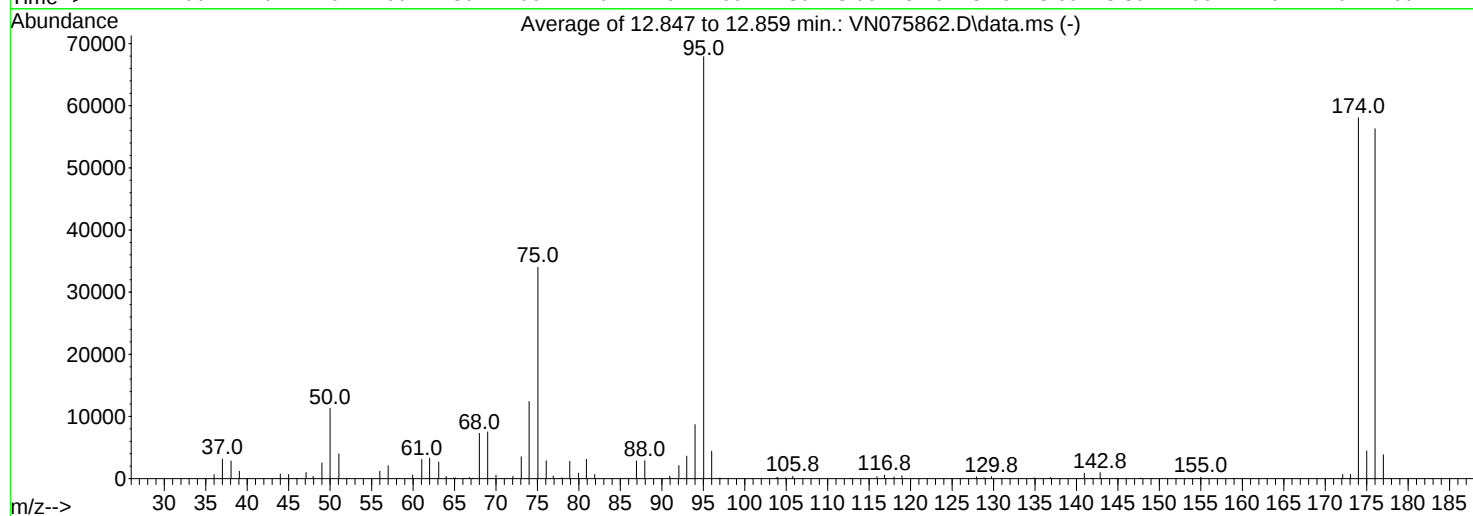


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN121922\  
Data File : VN075862.D  
Acq On : 19 Dec 2022 11:15  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Title : SW846 8260  
Last Update : Wed Dec 14 13:03:41 2022

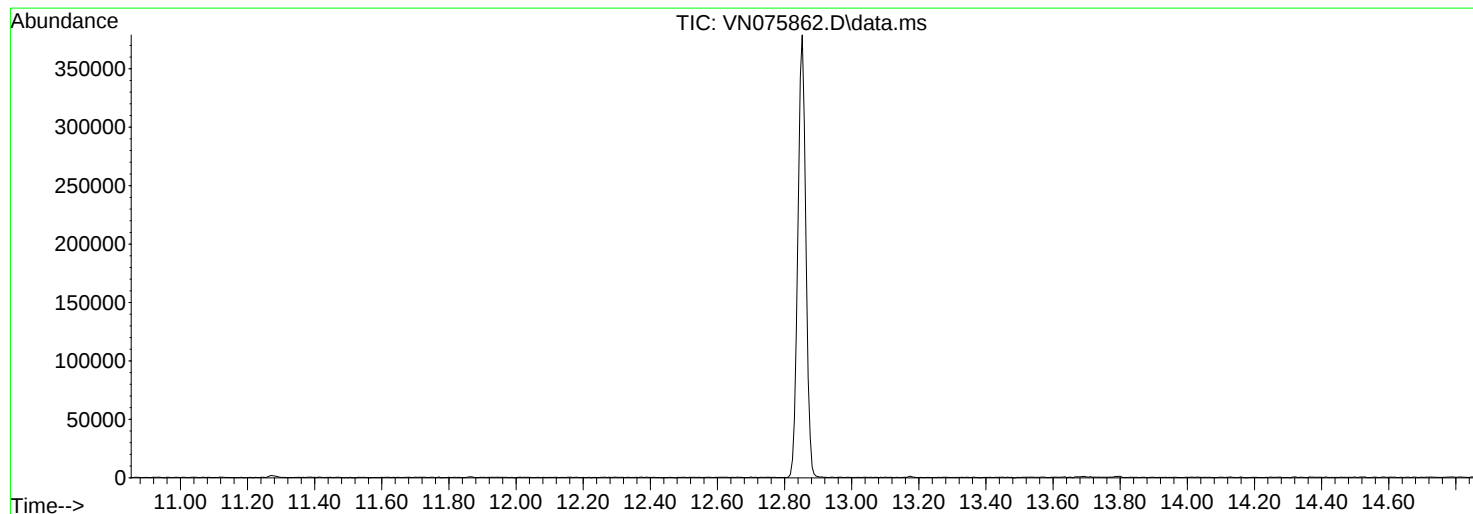

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.7         | 11305      | PASS                |
| 75             | 95              | 30              | 60              | 50.1         | 34000      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 67885      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 4400       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 651        | PASS                |
| 174            | 95              | 50              | 100             | 85.5         | 58051      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 4439       | PASS                |
| 176            | 174             | 95              | 101             | 97.0         | 56304      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 3821       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 637    | 50.00 | 11305  | 64.90 | 127    | 76.05 | 2880   |
| 37.00 | 3128   | 51.05 | 3971   | 65.10 | 122    | 76.90 | 422    |
| 38.05 | 2808   | 52.00 | 78     | 66.80 | 172    | 77.95 | 142    |
| 39.05 | 1181   | 56.00 | 1165   | 67.20 | 65     | 78.90 | 279    |
| 39.90 | 4      | 57.00 | 2081   | 68.00 | 7264   | 79.95 | 852    |
| 44.00 | 747    | 58.00 | 59     | 69.00 | 7519   | 80.90 | 3100   |
| 45.00 | 660    | 59.95 | 589    | 70.00 | 561    | 81.90 | 650    |
| 45.90 | 62     | 61.05 | 3088   | 72.05 | 371    | 86.00 | 73     |
| 47.10 | 958    | 62.00 | 3281   | 73.05 | 3528   | 86.95 | 2857   |
| 47.95 | 340    | 63.10 | 2678   | 74.00 | 12397  | 87.95 | 2883   |
| 49.00 | 2527   | 64.00 | 350    | 75.05 | 34000  | 90.95 | 390    |

Average of 12.847 to 12.859 min.: VN075862.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 92.05  | 2105   | 112.80 | 63     | 140.95 | 854    | 175.00 | 4439   |
| 93.00  | 3622   | 115.95 | 301    | 141.80 | 56     | 176.00 | 56304  |
| 94.00  | 8692   | 116.85 | 550    | 142.85 | 978    | 177.00 | 3821   |
| 95.05  | 67885  | 118.00 | 272    | 144.90 | 69     | 177.90 | 53     |
| 96.00  | 4400   | 118.95 | 447    | 147.70 | 64     |        |        |
| 96.90  | 85     | 127.95 | 273    | 147.90 | 64     |        |        |
| 97.10  | 67     | 128.85 | 135    | 155.00 | 235    |        |        |
| 103.80 | 132    | 129.75 | 327    | 158.90 | 58     |        |        |
| 104.00 | 207    | 130.90 | 60     | 172.10 | 665    |        |        |
| 104.95 | 124    | 134.90 | 130    | 173.05 | 651    |        |        |
| 105.80 | 369    | 136.85 | 180    | 174.00 | 58051  |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB