

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121923\
 Data File : VN080516.D
 Acq On : 19 Dec 2023 13:35
 Operator : JC\MD
 Sample : 05886-09 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 AUD-1302

Quant Time: Dec 20 04:01:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 13 01:57:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	217513	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	406556	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	423540	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	193584	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	159073	57.259	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 114.520%	
35) Dibromofluoromethane	8.165	113	136021	52.768	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.540%	
50) Toluene-d8	10.565	98	483333	50.276	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.560%	
62) 4-Bromofluorobenzene	12.847	95	198706	54.432	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 108.860%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121923\
Data File : VN080516.D
Acq On : 19 Dec 2023 13:35
Operator : JC\MD
Sample : 05886-09 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1302

Quant Time: Dec 20 04:01:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 13 01:57:14 2023
Response via : Initial Calibration




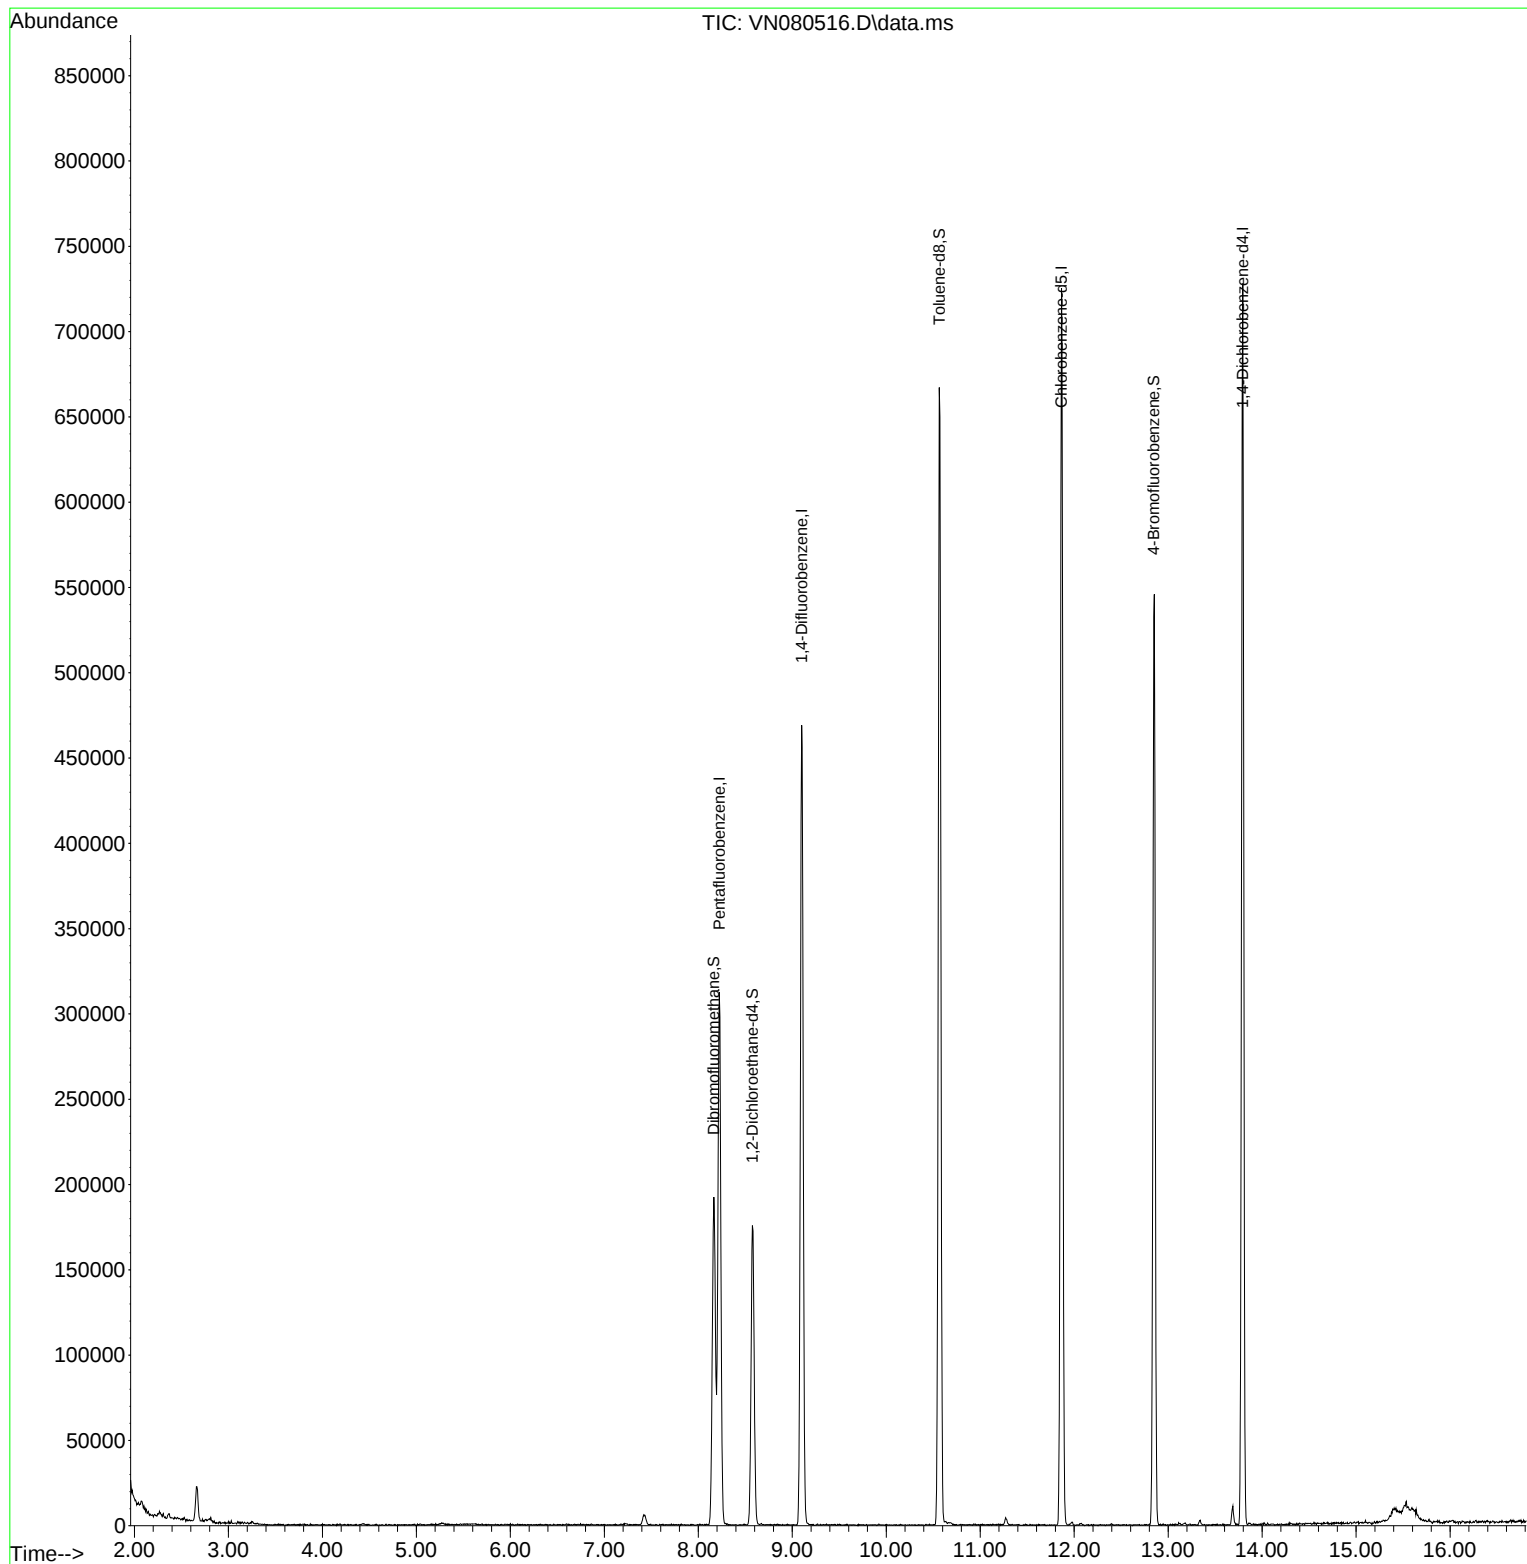


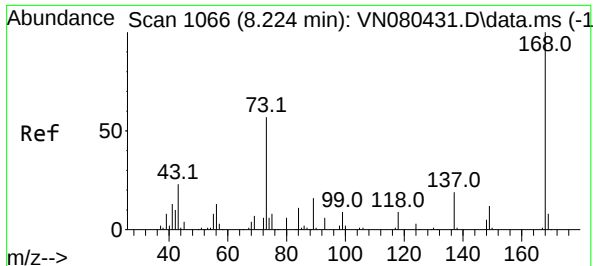

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35




Instrument :
MSVOA_N
ClientSampleId :
AUD-1302


Tgt Ion:168 Resp: 217513
Ion Ratio Lower Upper
168 100
99 63.3 53.0 79.6

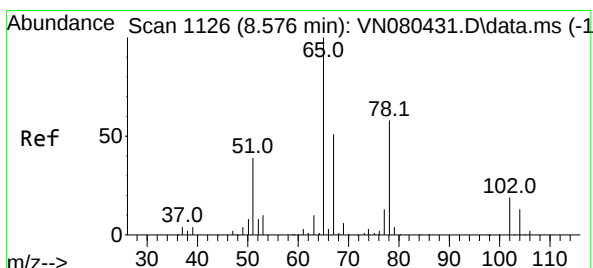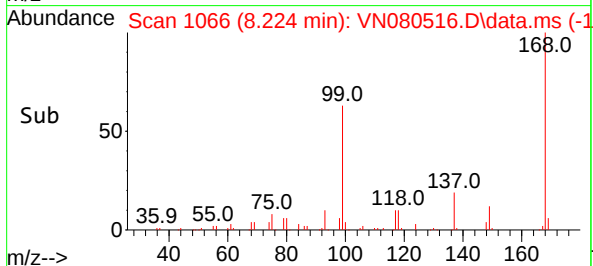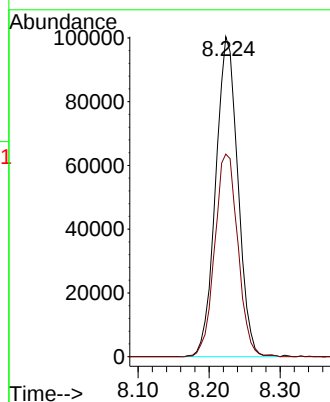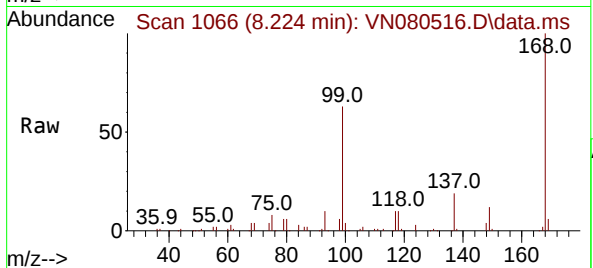

#33
1,2-Dichloroethane-d4
Concen: 57.259 ug/l
RT: 8.576 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35

Tgt Ion: 65 Resp: 159073
Ion Ratio Lower Upper
65 100
67 49.5 0.0 106.6

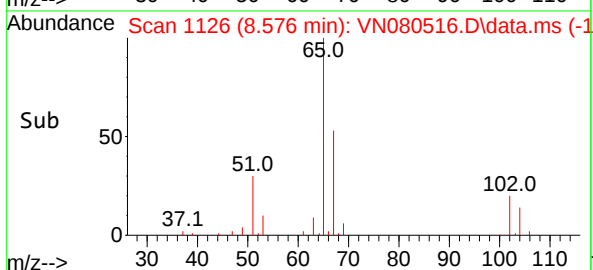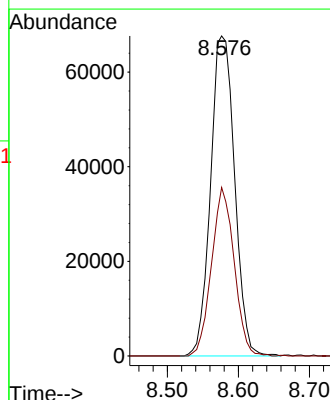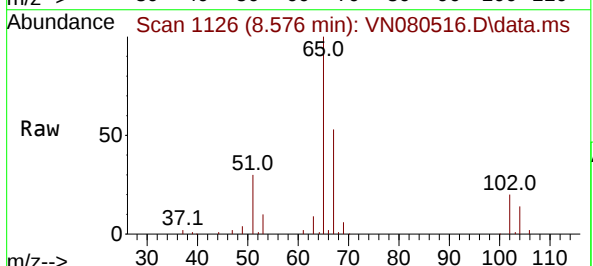

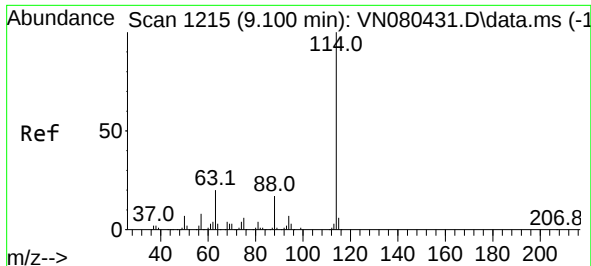

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN080516.D

Acq: 19 Dec 2023 13:35

Instrument :

MSVOA_N

ClientSampleId :

AUD-1302





Tgt Ion:114 Resp: 406556

Ion Ratio Lower Upper

114 100

63 21.1 0.0 36.4

88 18.0 0.0 30.6

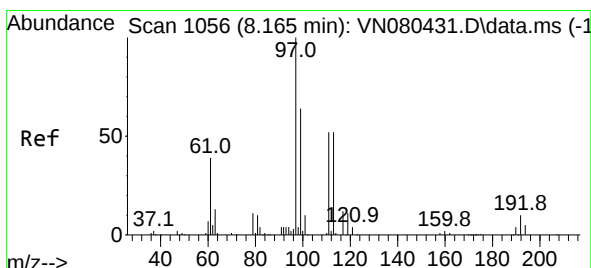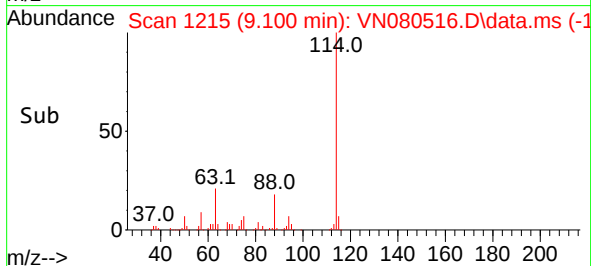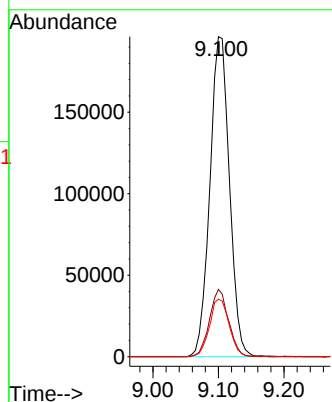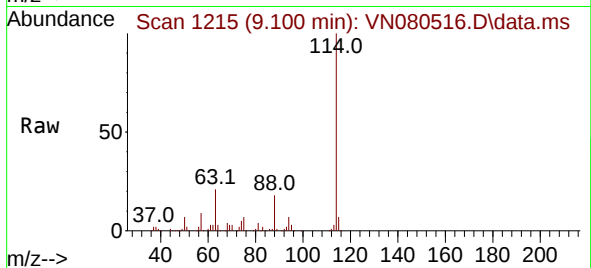

#35

Dibromofluoromethane

Concen: 52.768 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN080516.D

Acq: 19 Dec 2023 13:35




Tgt Ion:113 Resp: 136021


Ion Ratio Lower Upper

113 100

111 102.8 82.6 123.8

192 18.6 12.7 19.1


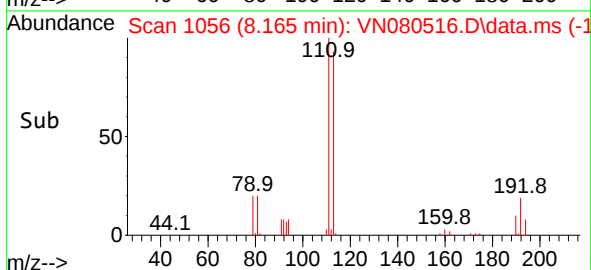
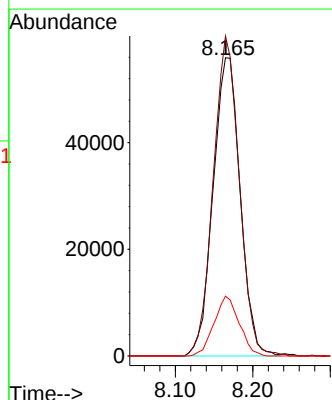
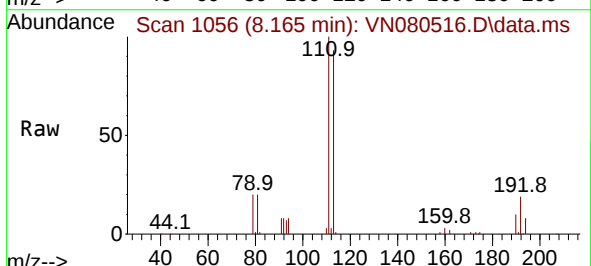


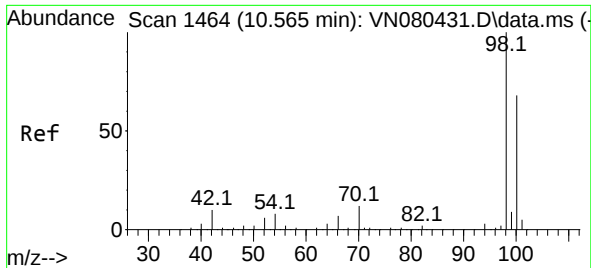

#50
Toluene-d8
Concen: 50.276 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35




Instrument :
MSVOA_N
ClientSampleId :
AUD-1302


Tgt Ion: 98 Resp: 483333
Ion Ratio Lower Upper
98 100
100 65.6 52.0 78.0

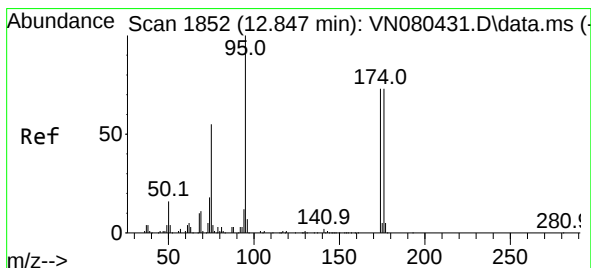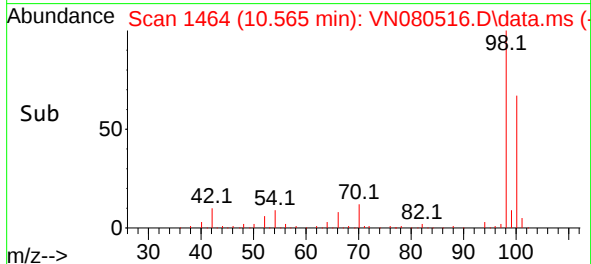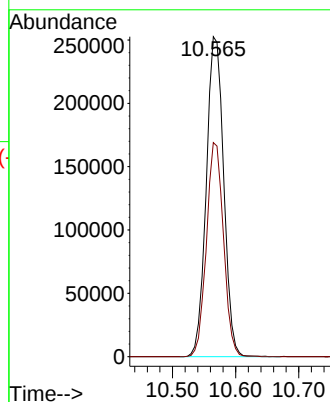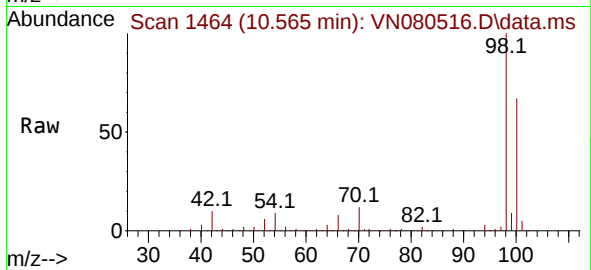

#62
4-Bromofluorobenzene
Concen: 54.432 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35

Tgt Ion: 95 Resp: 198706
Ion Ratio Lower Upper
95 100
174 72.6 0.0 143.8
176 71.7 0.0 135.8


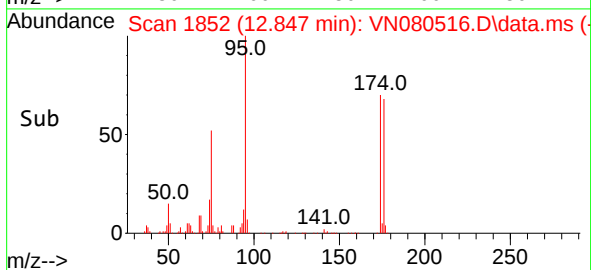
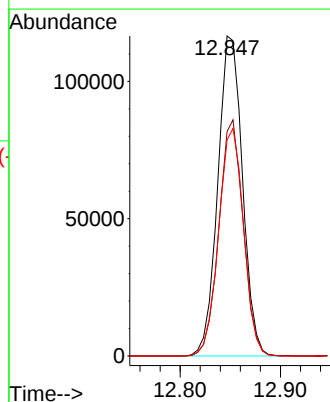
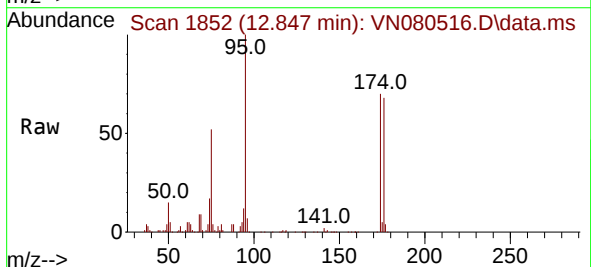


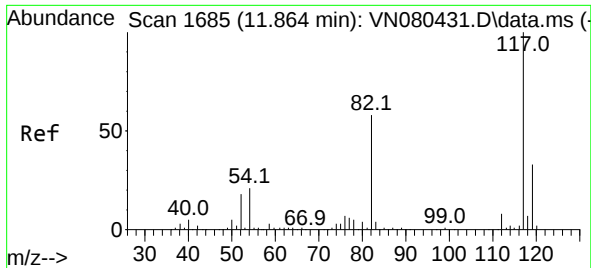

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35

Instrument :
MSVOA_N
ClientSampleId :
AUD-1302

Tgt Ion:117 Resp: 423540
Ion Ratio Lower Upper
117 100
82 61.5 44.0 66.0
119 31.1 25.6 38.4

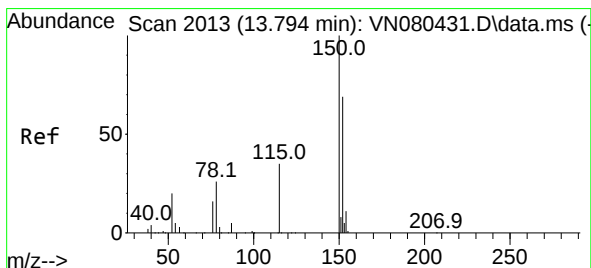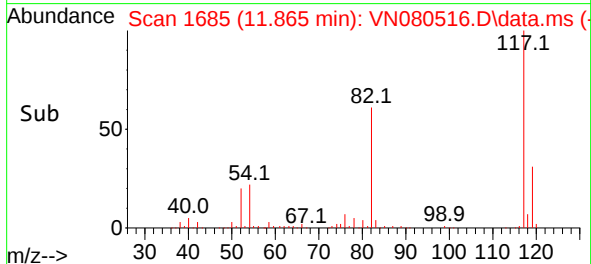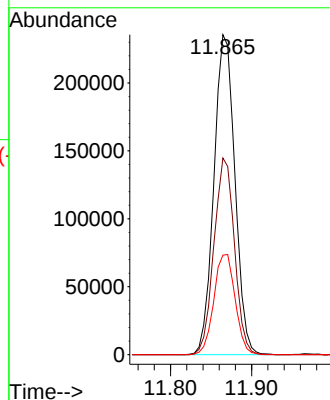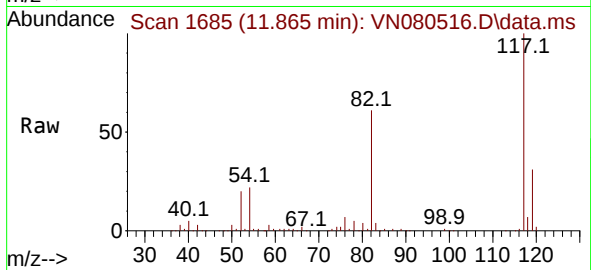

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080516.D
Acq: 19 Dec 2023 13:35

Tgt Ion:152 Resp: 193584
Ion Ratio Lower Upper
152 100
115 65.2 32.3 96.8
150 157.7 0.0 355.8

