
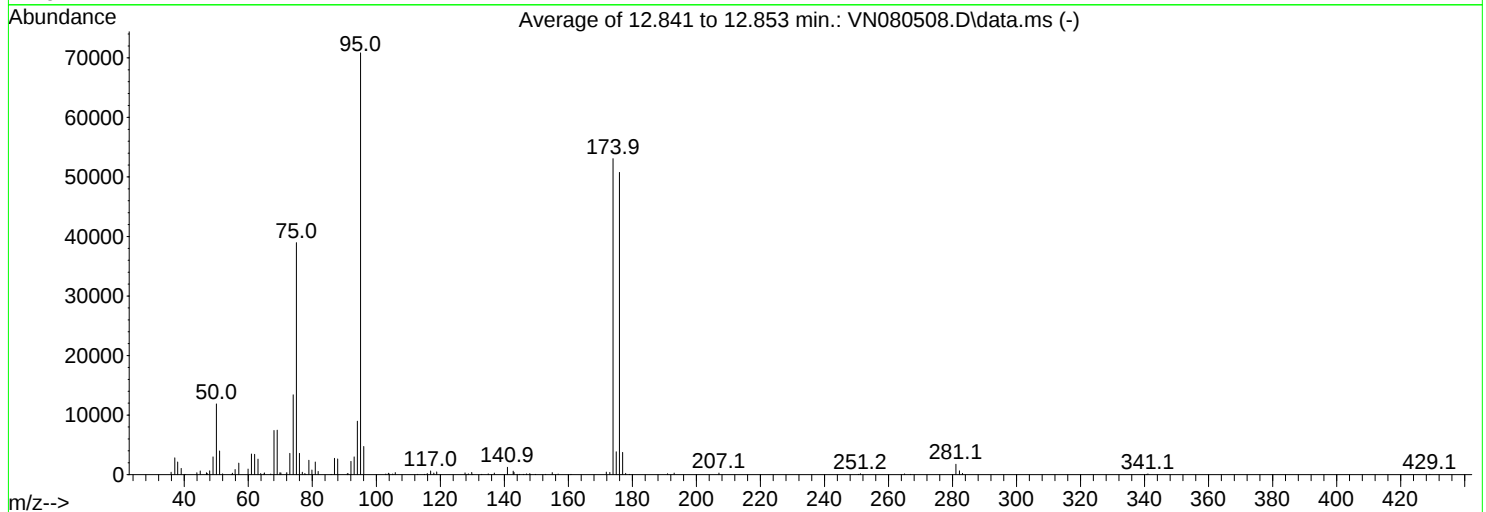


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121923\
Data File : VN080508.D
Acq On : 19 Dec 2023 09:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

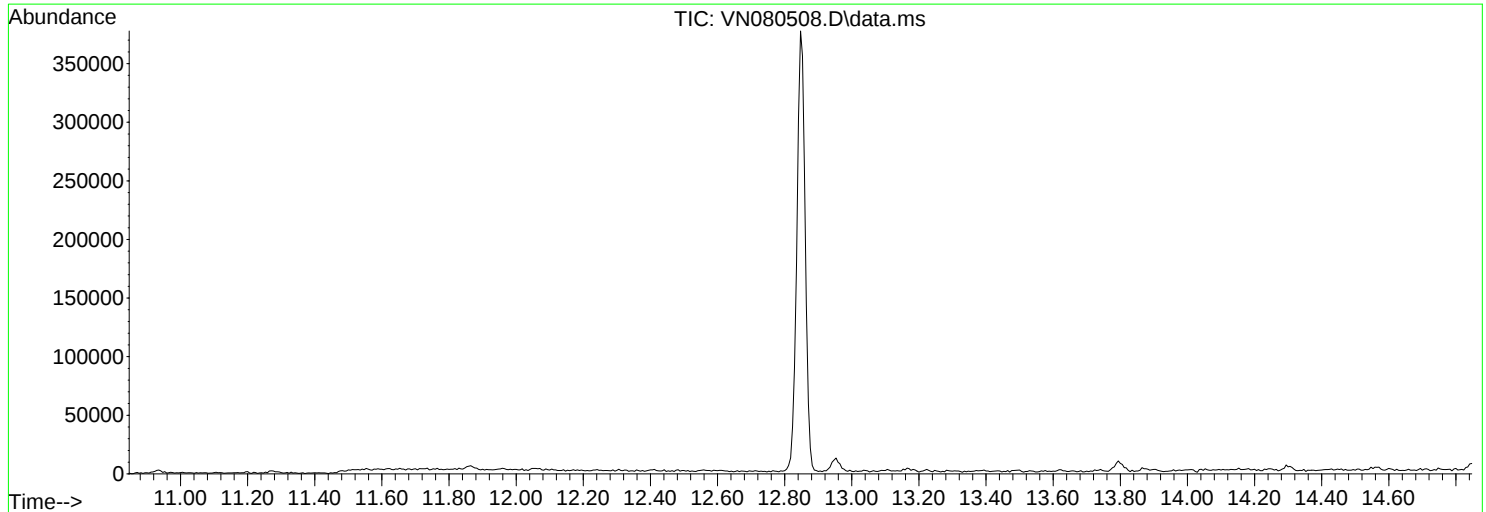

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	11879	PASS
75	95	30	60	55.0	38965	PASS
95	95	100	100	100.0	70845	PASS
96	95	5	9	6.7	4734	PASS
173	174	0.00	2	0.7	379	PASS
174	95	50	100	74.9	53075	PASS
175	174	5	9	7.2	3846	PASS
176	174	95	101	95.6	50765	PASS
177	176	5	9	7.3	3726	PASS

Average of 12.841 to 12.853 min.: VN080508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	396	49.00	2982	63.05	2608	73.00	358
37.05	2832	50.05	11879	63.90	189	74.05	1340
37.95	2132	51.05	3990	64.90	107	75.05	3896
39.05	1043	52.00	131	65.05	293	76.00	357
39.95	5	54.80	54	67.05	118	76.90	394
40.20	66	55.05	238	68.05	7424	77.70	192
43.95	312	55.90	850	69.05	7481	78.00	52
45.00	634	57.05	1926	69.90	312	78.95	2431
46.95	316	59.95	953	70.20	286	79.90	793
47.20	190	61.00	3473	71.90	140	80.95	2138
47.95	638	62.00	3408	72.05	347	81.85	539

Average of 12.841 to 12.853 min.: VN080508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.90	51	103.75	241	128.30	65	144.70	51
86.95	2744	104.10	112	128.75	146	146.00	56
87.95	2640	105.10	117	129.80	367	146.95	130
90.90	136	105.90	354	130.10	70	147.90	163
91.10	215	112.90	56	132.90	61	148.10	84
92.05	2236	115.00	60	134.95	142	149.70	71
93.05	2985	115.90	195	136.85	279	152.90	58
94.05	8969	116.95	621	140.95	1230	154.95	351
95.05	70845	117.95	273	142.75	597	156.80	100
96.05	4734	118.85	470	143.00	383	160.80	52
102.95	113	127.70	299	144.00	56	171.85	422

Average of 12.841 to 12.853 min.: VN080508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.95	379	251.20	160				
173.95	53075	265.00	137				
174.95	3846	266.90	65				
175.95	50765	281.05	1740				
176.95	3726	282.15	640				
177.90	225	283.10	230				
179.10	52	340.70	71				
191.00	165	341.05	146				
193.05	266	429.10	67				
207.05	267						
250.60	62						

Instrument :

MSVOA_N

ClientSampleId :

BFB