

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN122018\
 Data File : VN053071.D
 Acq On : 20 Dec 2018 22:35
 Operator : MD\SY
 Sample : VN1220WBL02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 32 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1220WBL02

Quant Time: Dec 21 02:45:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 18 13:03:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1288313	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1976146	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1783176	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	739876	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	632706	48.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.78%	
35) Dibromofluoromethane	7.59	113	523227	57.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.92%	
50) Toluene-d8	10.09	98	2419239	49.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.84%	
62) 4-Bromofluorobenzene	12.40	95	813928	47.84	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.68%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN122018\
Data File : VN053071.D
Acq On : 20 Dec 2018 22:35
Operator : MD\SY
Sample : VN1220WBL02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 32 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN1220WBL02

Quant Time: Dec 21 02:45:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 18 13:03:37 2018
Response via : Initial Calibration

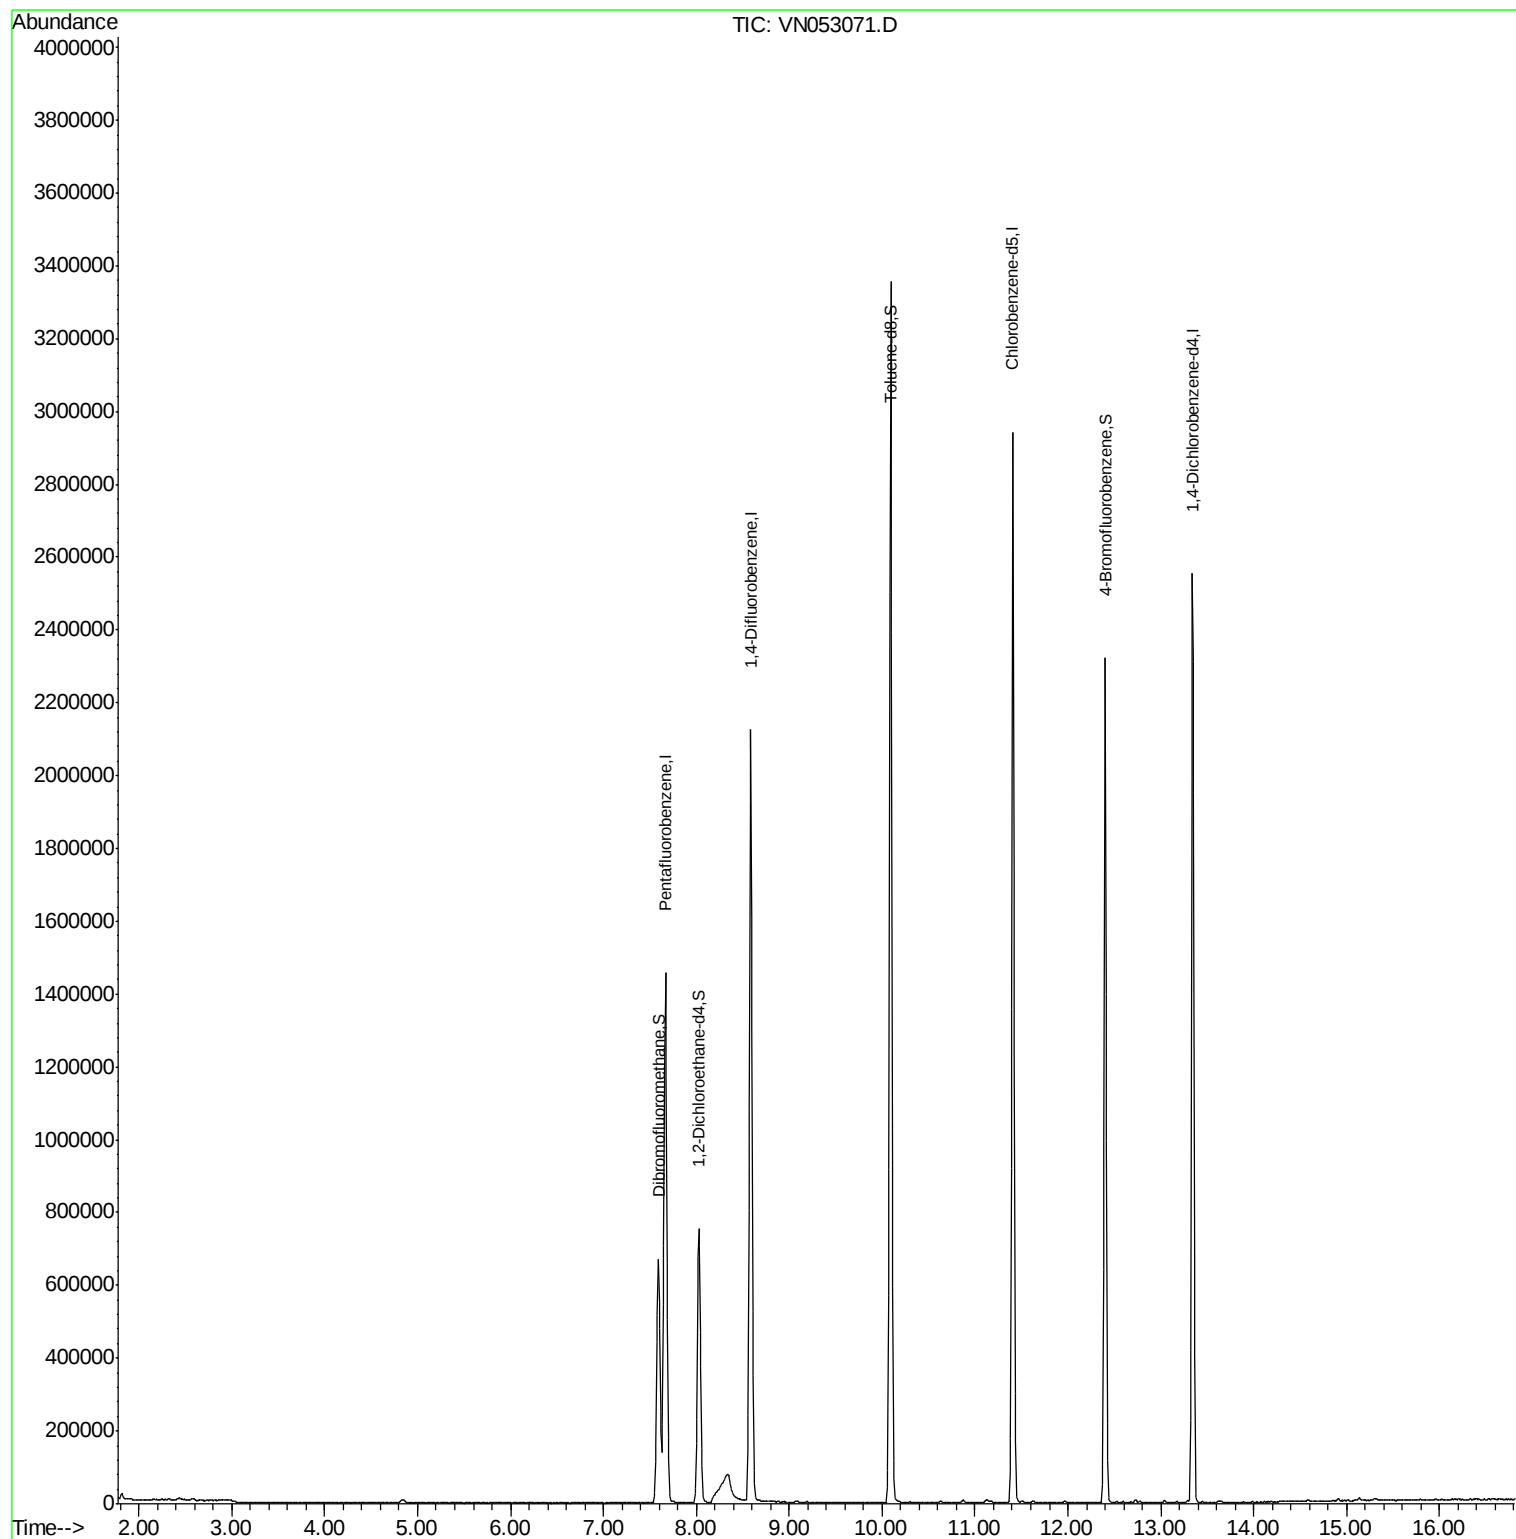

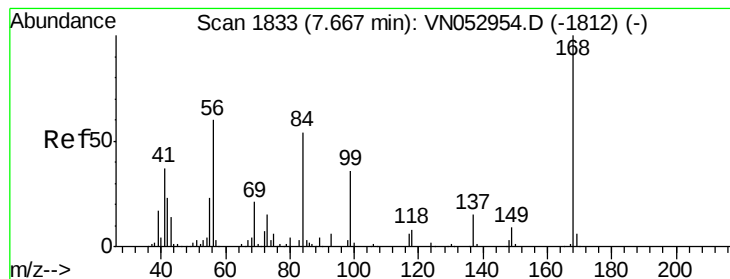

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN053071.D

Acq: 20 Dec 2018 22:35

Instrument :

MSVOA_N

ClientSampleId :


VN1220WBL02

Tot Ion:168 Resp: 1288313

Ion Ratio Lower Upper

168 100

99 49.6 40.2 60.2

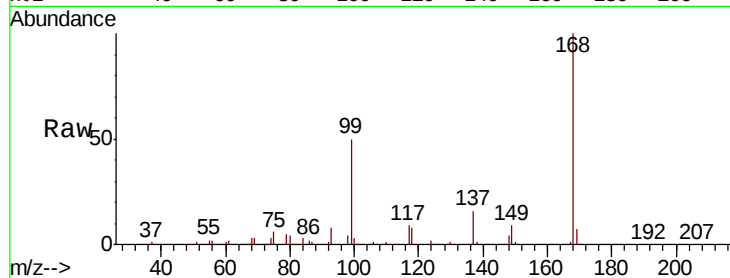

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67

600000

500000

400000



300000

200000

100000

0

Time-->

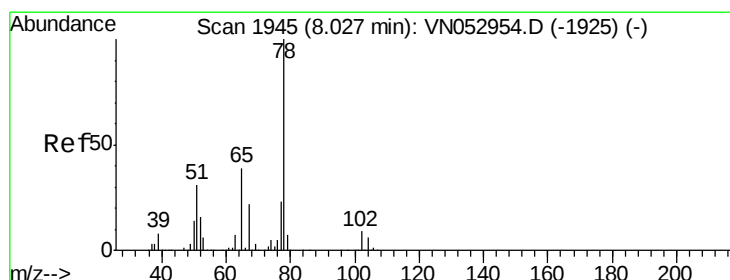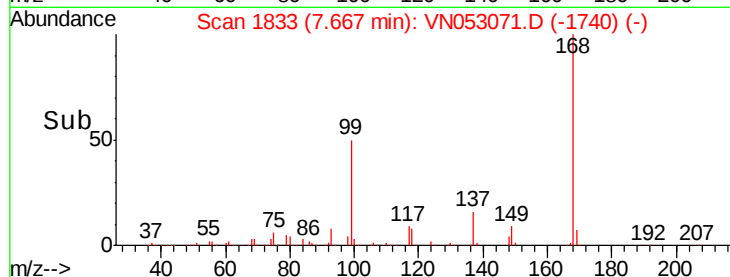

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN053071.D


Acq: 20 Dec 2018 22:35

Tgt Ion: 65 Resp: 632706

Ion Ratio Lower Upper

65 100

67 54.6 0.0 110.4

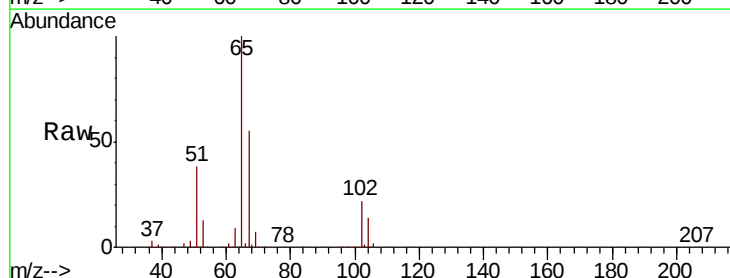

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03

300000

250000

200000


150000


100000

50000

0

Time-->

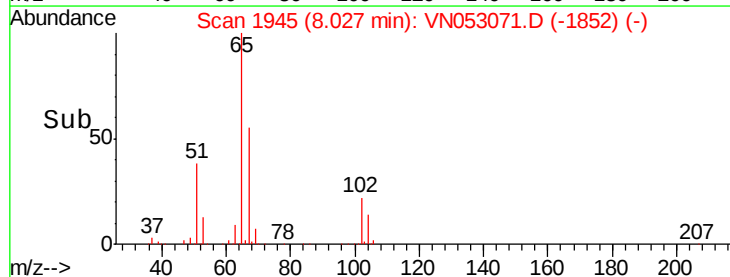


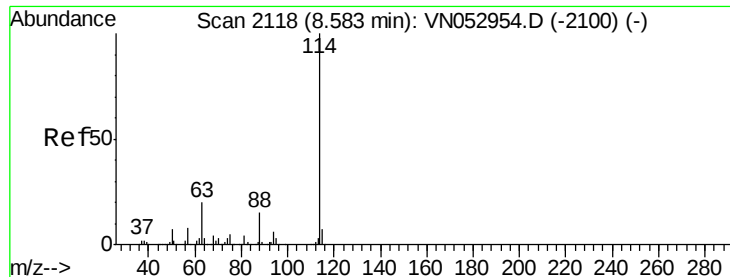




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.59 min Scan# 2119
Delta R.T. 0.00 min
Lab File: VN053071.D
Acq: 20 Dec 2018 22:35

Instrument :
MSVOA_N
ClientSampleId :
VN1220WBL02

Tot Ion:114 Resp: 1976146
Ion Ratio Lower Upper
114 100
63 19.9 0.0 39.8
88 15.6 0.0 31.0

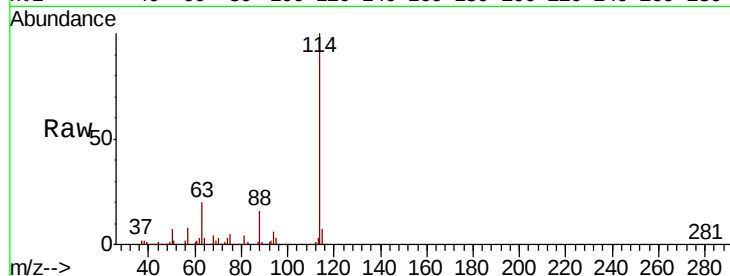


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

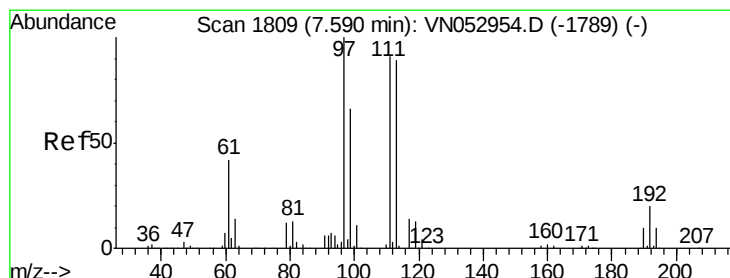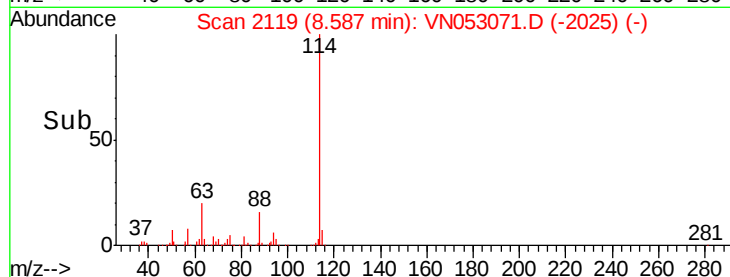
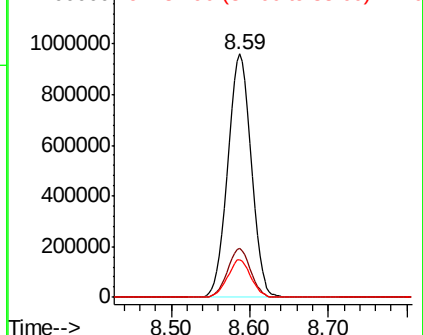



#35
Dibromofluoromethane
Concen: 50.000 ug/l
RT: 7.59 min Scan# 1810
Delta R.T. 0.00 min
Lab File: VN053071.D
Acq: 20 Dec 2018 22:35

Tgt Ion:113 Resp: 523227
Ion Ratio Lower Upper
113 100
111 102.7 83.0 124.4
192 22.7 17.5 26.3

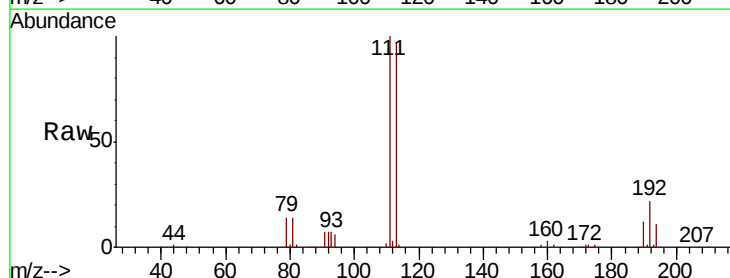

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

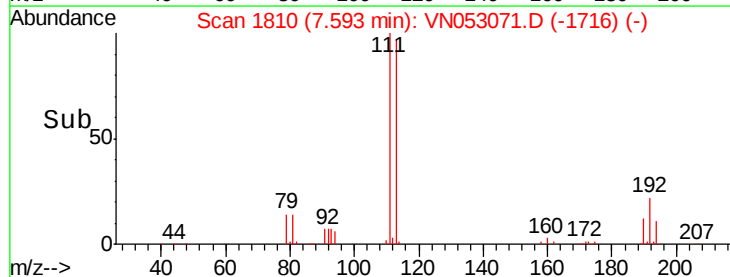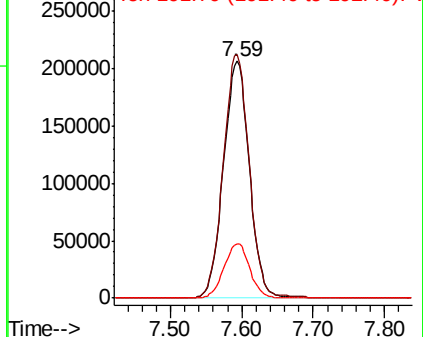

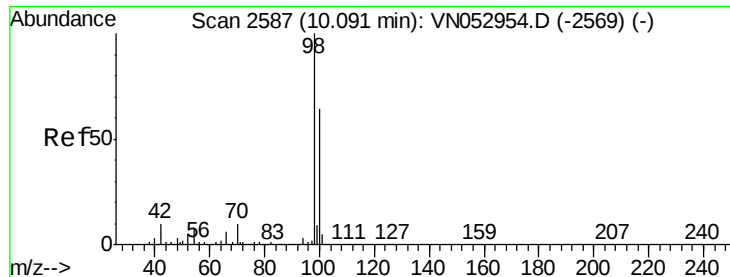

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN053071.D

Acq: 20 Dec 2018 22:35

Instrument :

MSVOA_N

ClientSampleId :





VN1220WBL02

Tot Ion: 98 Resp: 2419239

Ion Ratio Lower Upper

98 100

100 64.0 51.6 77.4

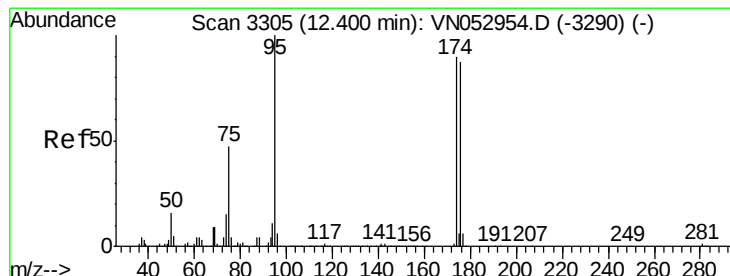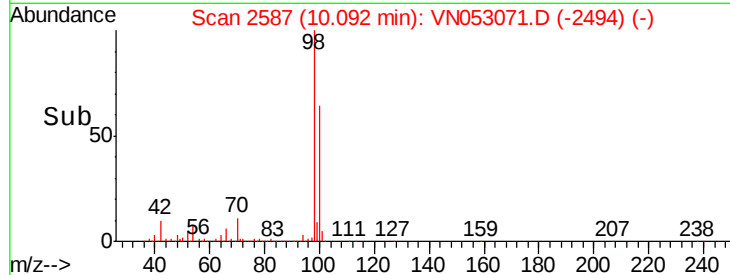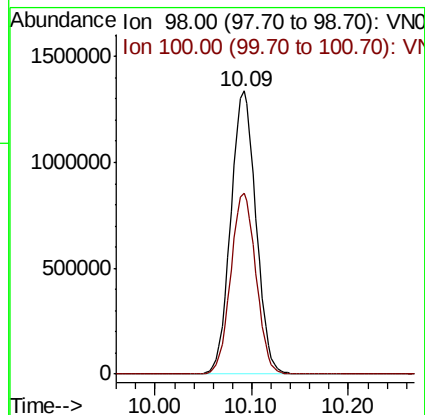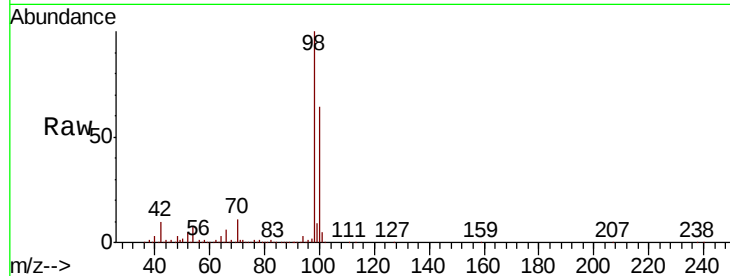

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN053071.D

Acq: 20 Dec 2018 22:35




Tgt Ion: 95 Resp: 813928


Ion Ratio Lower Upper

95 100

174 90.1 0.0 178.8

176 87.0 0.0 173.8

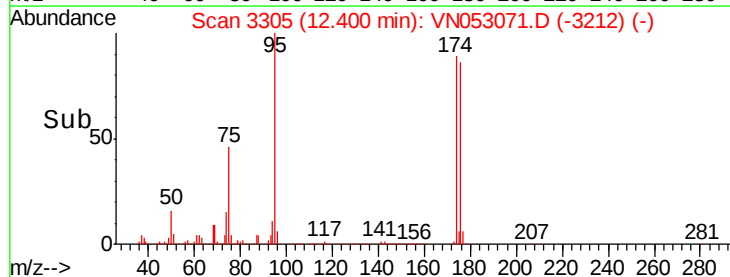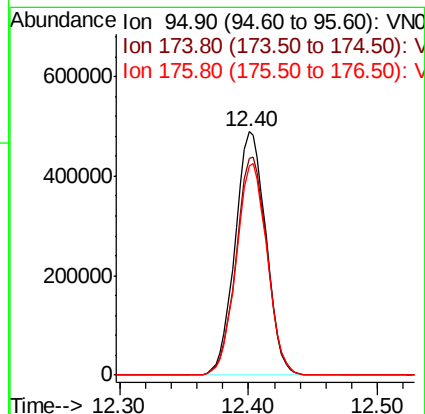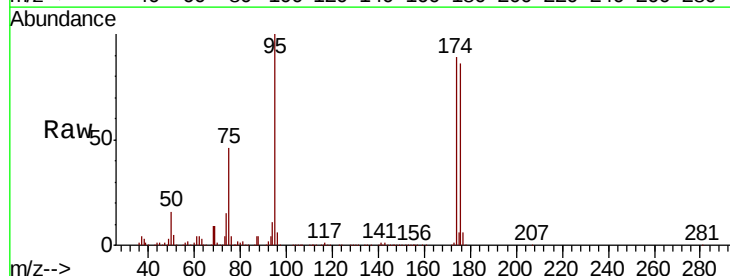


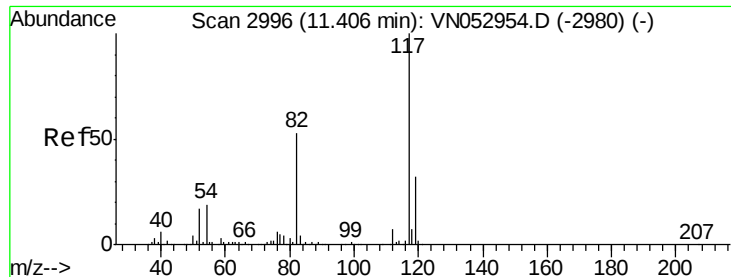




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN053071.D
Acq: 20 Dec 2018 22:35

Instrument :
MSVOA_N
ClientSampled :
VN1220WBL02

Tot Ion:117 Resp: 1783176
Ion Ratio Lower Upper
117 100
82 53.3 42.8 64.2
119 32.0 25.5 38.3

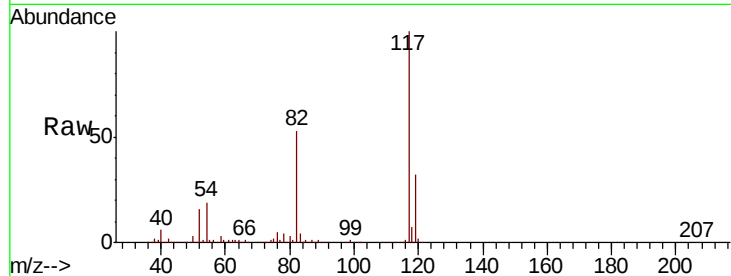


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

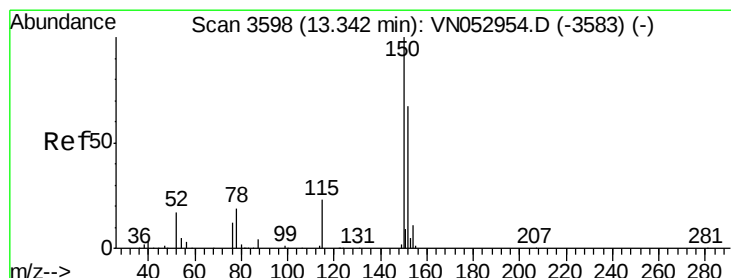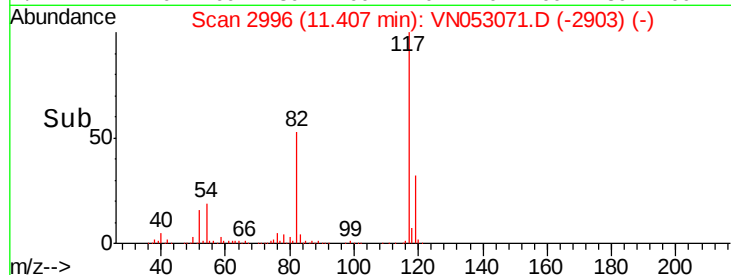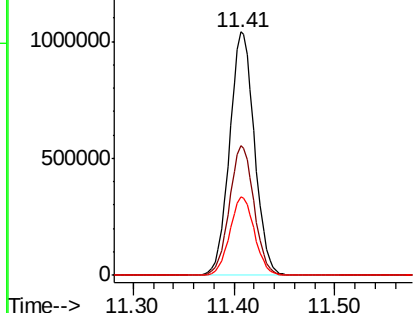

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN053071.D
Acq: 20 Dec 2018 22:35

Tgt Ion:152 Resp: 739876
Ion Ratio Lower Upper
152 100
115 56.1 28.3 85.0
150 156.7 0.0 347.8

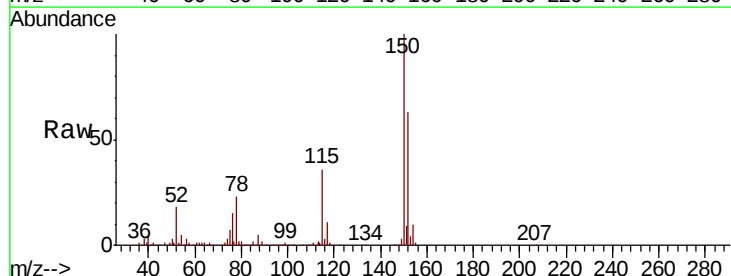

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

