


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122021\
 Data File : VN070229.D
 Acq On : 20 Dec 2021 9:45
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
 Title : SW846 8260
 Last Update : Fri Dec 03 08:46:47 2021

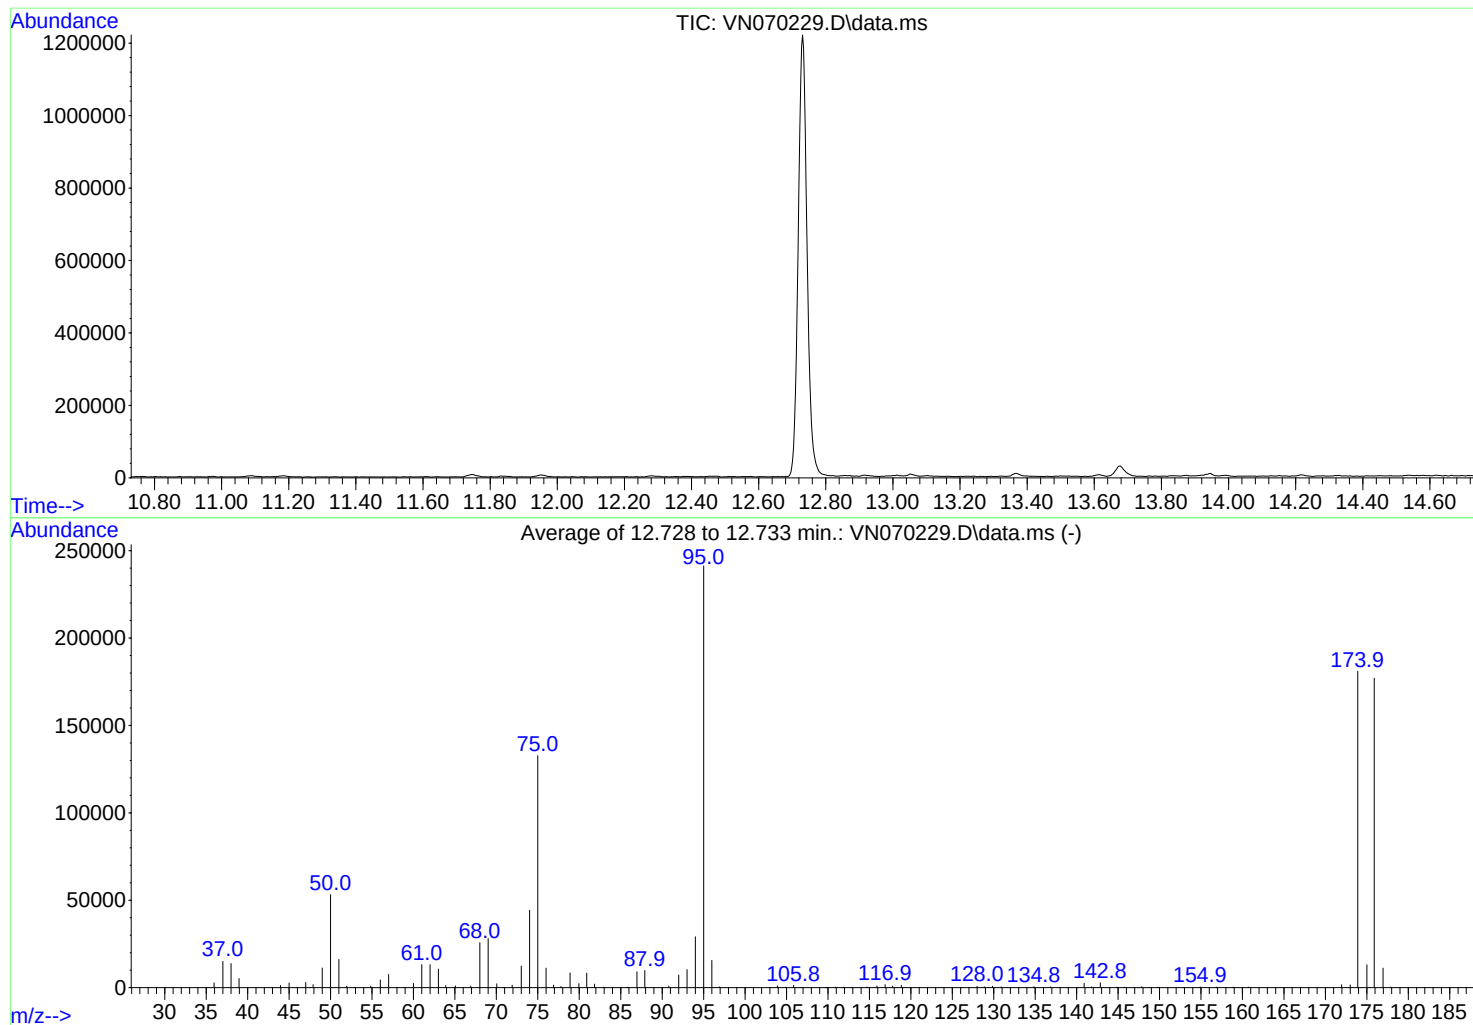

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	53184	PASS
75	95	30	60	55.0	132744	PASS
95	95	100	100	100.0	241301	PASS
96	95	5	9	6.4	15539	PASS
173	174	0.00	2	0.9	1592	PASS
174	95	50	100	75.0	180928	PASS
175	174	5	9	7.2	13093	PASS
176	174	95	101	97.9	177067	PASS
177	176	5	9	6.3	11163	PASS