
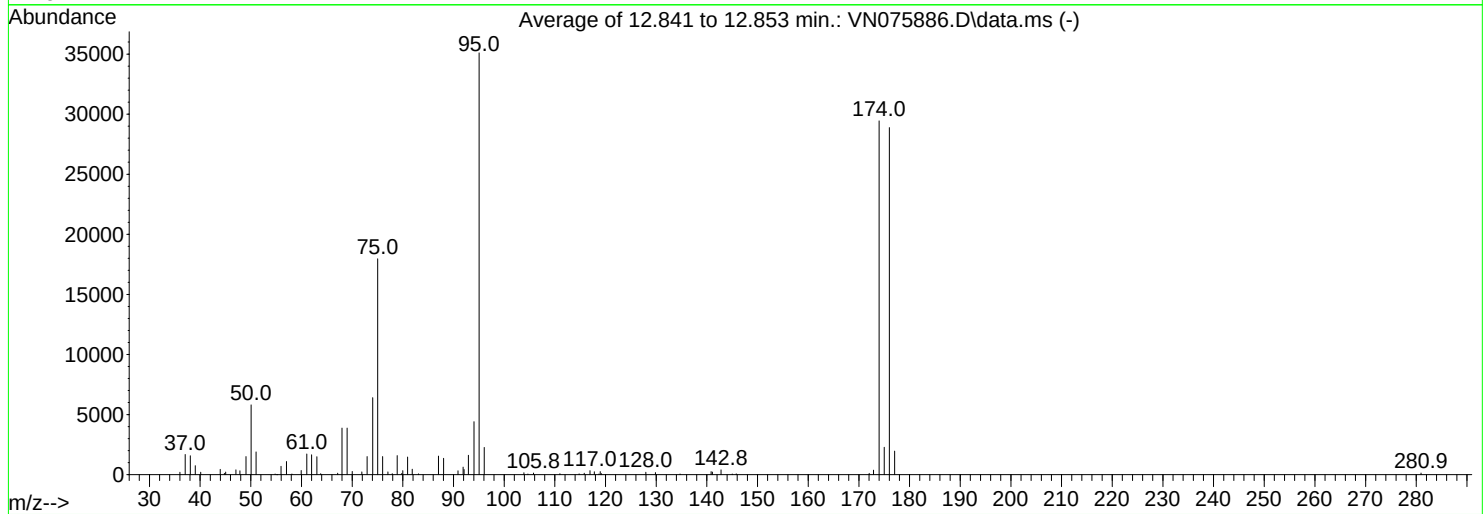


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122022\
 Data File : VN075886.D
 Acq On : 20 Dec 2022 09:41
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

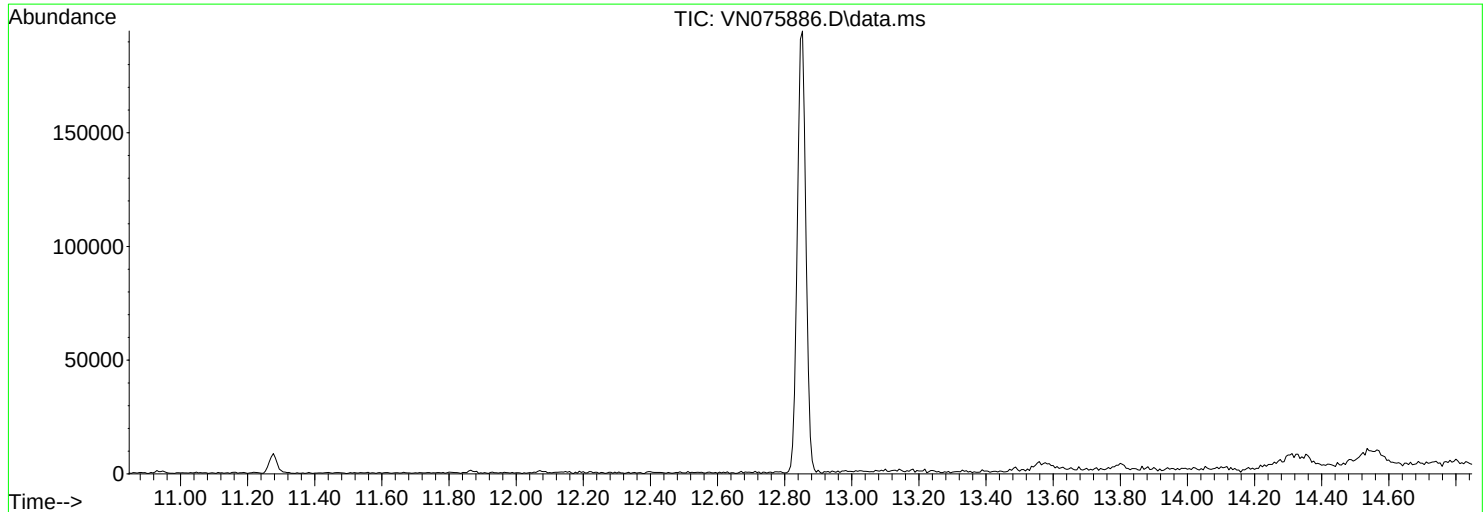

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	5800	PASS
75	95	30	60	51.2	17971	PASS
95	95	100	100	100.0	35104	PASS
96	95	5	9	6.4	2259	PASS
173	174	0.00	2	1.3	373	PASS
174	95	50	100	83.9	29440	PASS
175	174	5	9	7.7	2281	PASS
176	174	95	101	98.1	28888	PASS
177	176	5	9	6.8	1957	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	204	50.05	5800	63.80	87	77.90	7
37.05	1680	51.05	1888	67.15	118	78.90	158
38.05	1566	54.80	56	68.00	3878	79.80	10
39.05	749	55.10	0	69.00	3878	80.00	32
40.10	203	55.95	688	70.00	270	80.95	1461
43.95	438	57.05	1093	71.90	227	81.85	449
44.80	111	58.10	53	72.95	1505	83.10	72
45.05	215	59.95	346	74.05	6410	87.05	1549
47.05	395	61.05	1712	75.05	17971	88.05	1360
47.85	319	62.00	1654	76.00	1501	90.90	315
49.05	1507	63.05	1490	77.05	233	91.90	633

Average of 12.841 to 12.853 min.: VN075886.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.10	425	116.95	332	145.00	54		
92.95	1609	117.80	239	145.80	62		
94.05	4404	118.70	54	172.05	111		
95.05	35104	118.95	254	172.90	373		
96.05	2259	119.20	79	174.00	29440		
103.90	162	127.95	201	175.00	2281		
104.70	51	129.85	178	176.00	28888		
105.80	129	134.70	55	177.05	1957		
111.00	74	140.85	253	280.95	129		
114.80	62	141.10	211				
115.80	118	142.80	406				

Instrument :

MSVOA_N

ClientSampleId :

BFB