

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122023\
 Data File : VN080561.D
 Acq On : 20 Dec 2023 20:51
 Operator : JC\MD
 Sample : 05863-02 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NWB-1987

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Title : SW846 8260

Signal : TIC: VN080561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.083	17	22	30	rVB2	25417	43850	2.77%	0.435%
2	2.507	90	94	101	rVB2	9471	16718	1.06%	0.166%
3	2.665	114	121	128	rVB	87888	156979	9.92%	1.558%
4	4.283	387	396	411	rVB2	7918	21040	1.33%	0.209%
5	4.430	411	421	430	rBV2	8467	23315	1.47%	0.231%
6	4.700	456	467	484	rBV	190002	622781	39.37%	6.182%
7	8.165	1045	1056	1061	rBV	207090	501834	31.72%	4.982%
8	8.224	1061	1066	1078	rVB	372932	823929	52.08%	8.179%
9	8.577	1112	1126	1137	rBV	212427	479969	30.34%	4.765%
10	9.100	1205	1215	1229	rBV	618982	1246271	78.78%	12.371%
11	10.565	1456	1464	1471	rBV	764194	1435568	90.75%	14.250%
12	10.630	1471	1475	1484	rVB	36283	68834	4.35%	0.683%
13	11.865	1677	1685	1697	rVB	882936	1572570	99.41%	15.610%
14	12.071	1712	1720	1728	rBV2	16033	35427	2.24%	0.352%
15	12.847	1845	1852	1861	rBV	645902	1126172	71.19%	11.179%
16	13.341	1931	1936	1941	rBV9	7305	16009	1.01%	0.159%
17	13.794	2006	2013	2022	rBV	935443	1581909	100.00%	15.703%
18	13.870	2022	2026	2032	rVB	62602	100995	6.38%	1.003%
19	15.029	2219	2223	2231	rBV9	8502	22660	1.43%	0.225%
20	15.500	2299	2303	2308	rVB8	11392	19008	1.20%	0.189%
21	15.647	2321	2328	2335	rVV2	20382	50313	3.18%	0.499%
22	15.841	2355	2361	2366	rBV8	12276	25329	1.60%	0.251%
23	16.164	2411	2416	2420	rBV8	10829	17792	1.12%	0.177%
24	16.711	2502	2509	2515	rBV8	12831	33088	2.09%	0.328%
25	16.782	2515	2521	2522	rBV5	19526	31474	1.99%	0.312%




Sum of corrected areas: 10073834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122023\
Data File : VN080561.D
Acq On : 20 Dec 2023 20:51
Operator : JC\MD
Sample : 05863-02 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1987

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

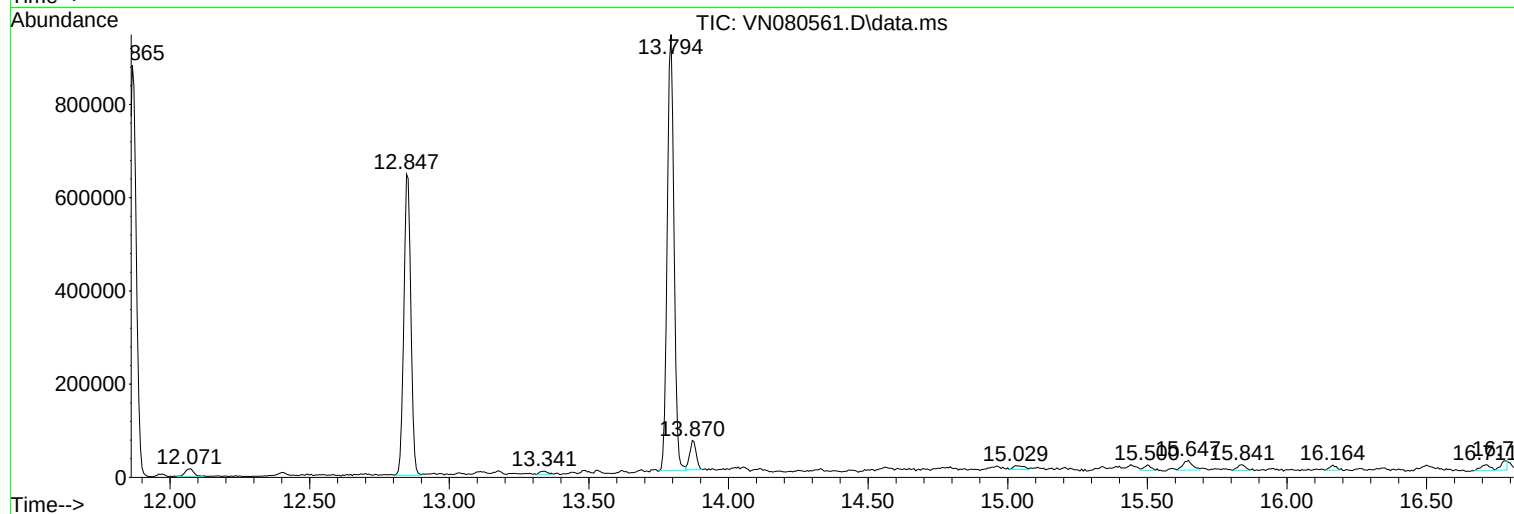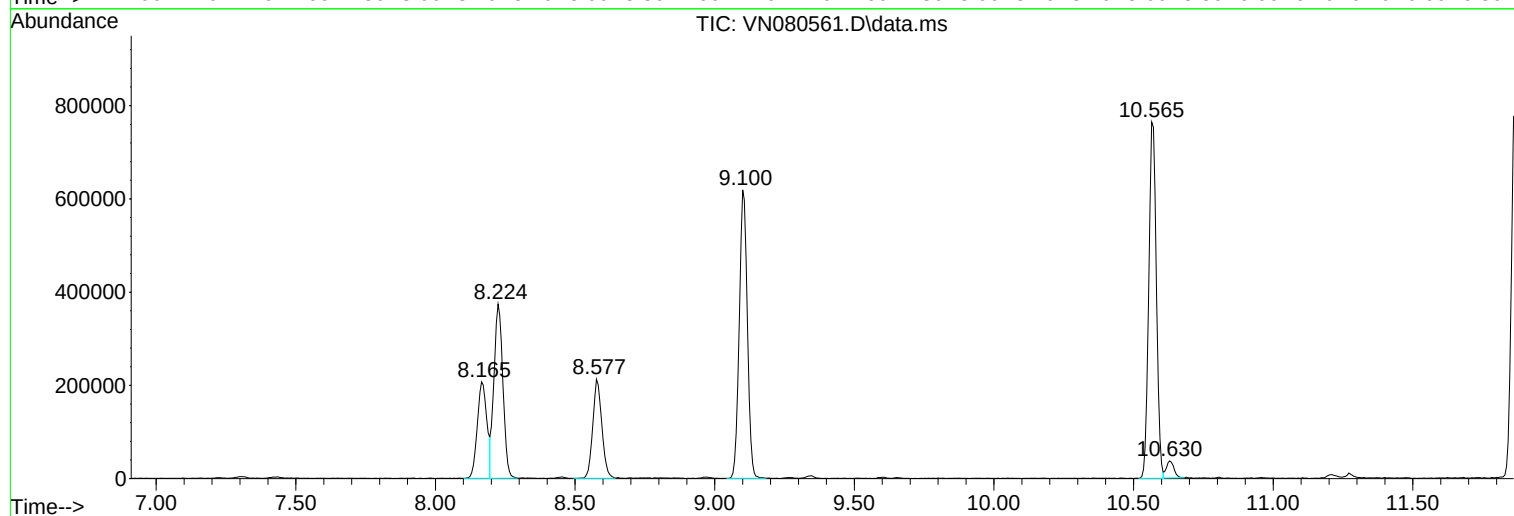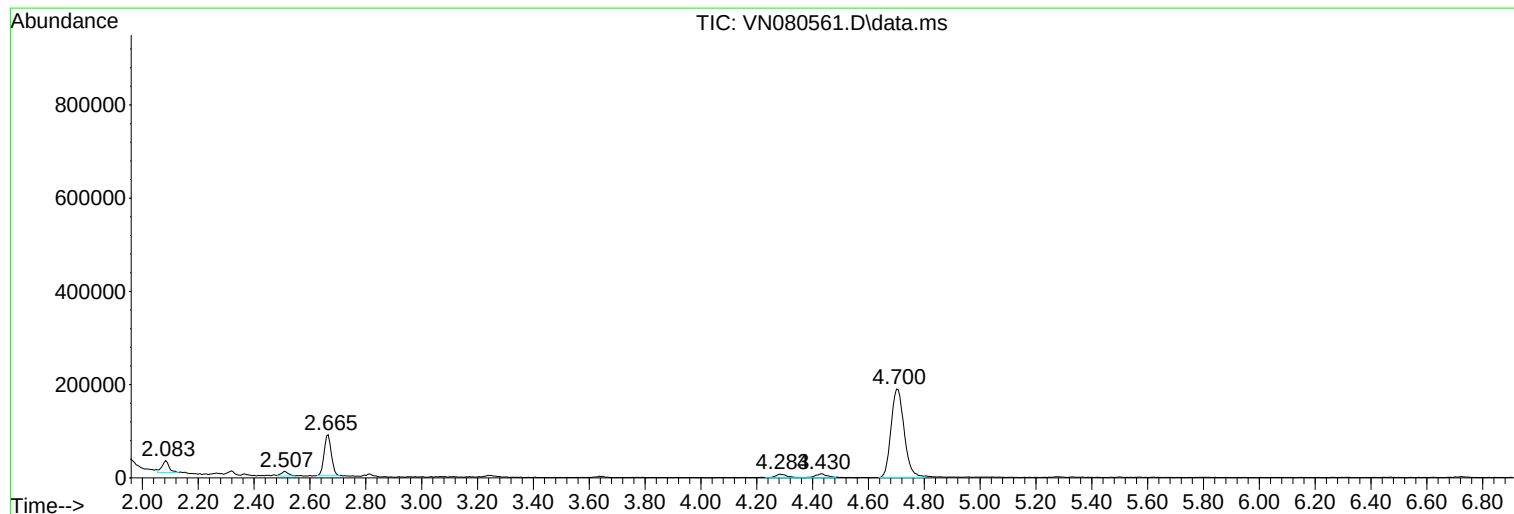

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122023\
Data File : VN080561.D
Acq On : 20 Dec 2023 20:51
Operator : JC\MD
Sample : 05863-02 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1987










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.700	37.79 ug/l	622781	Pentafluorobenzene	8.224

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	64
3			Formic acid, 1-methylethyl ester	88	C4H8O2	000625-55-8	39
4			R-(-)-1,2-propanediol	76	C3H8O2	004254-14-2	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

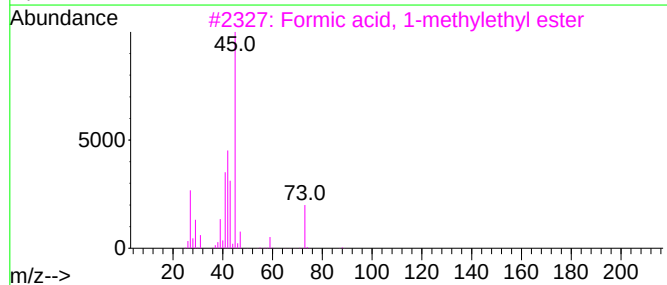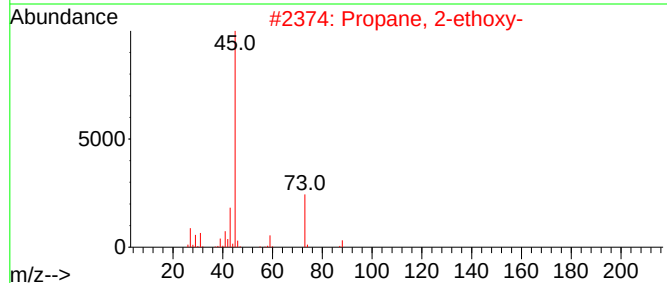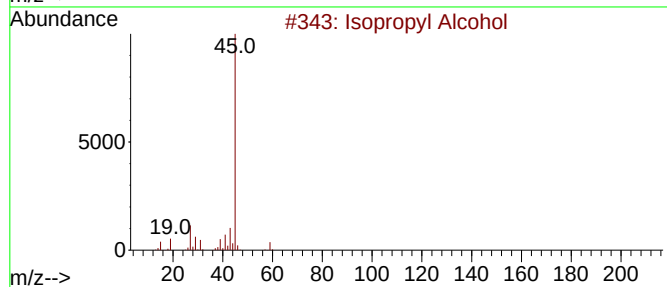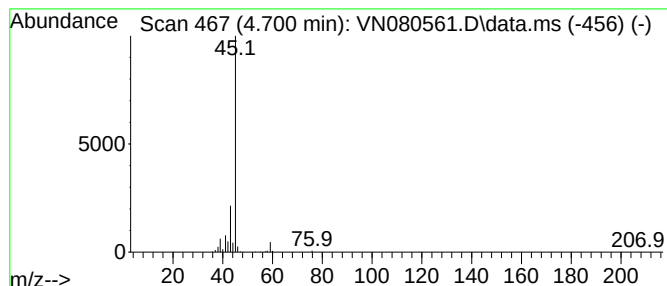

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122023\
Data File : VN080561.D
Acq On : 20 Dec 2023 20:51
Operator : JC\MD
Sample : 05863-02 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1987

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	4.700	37.8	ug/l	622781	1	8.224	823929	50.0