
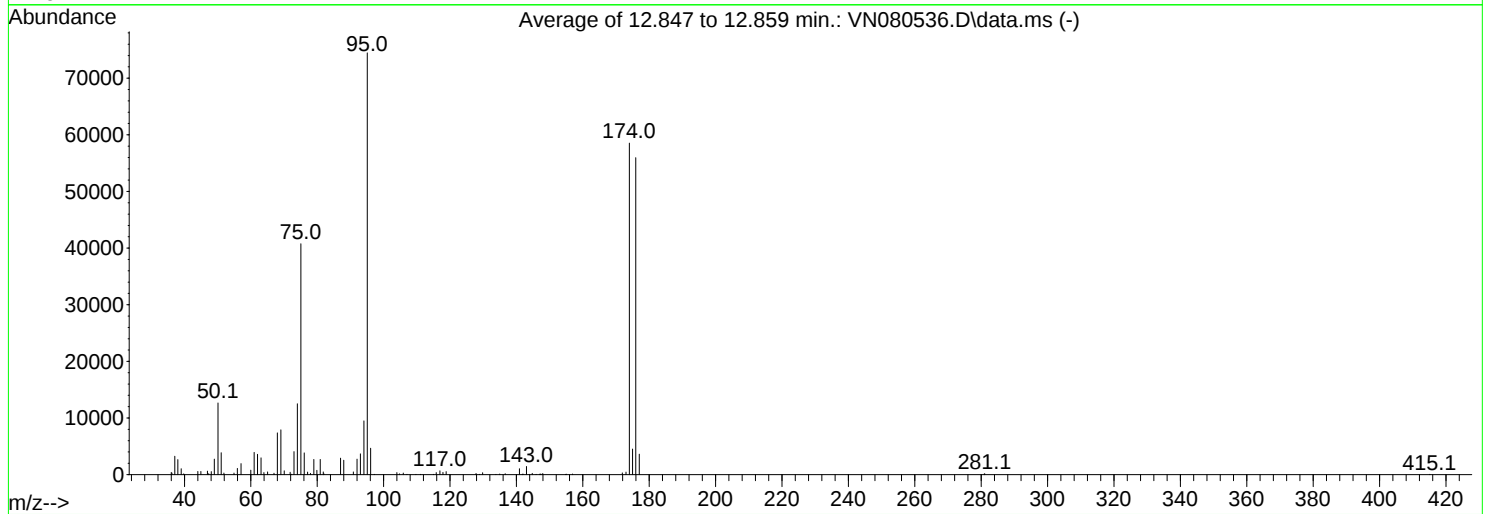


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122023\
Data File : VN080536.D
Acq On : 20 Dec 2023 10:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

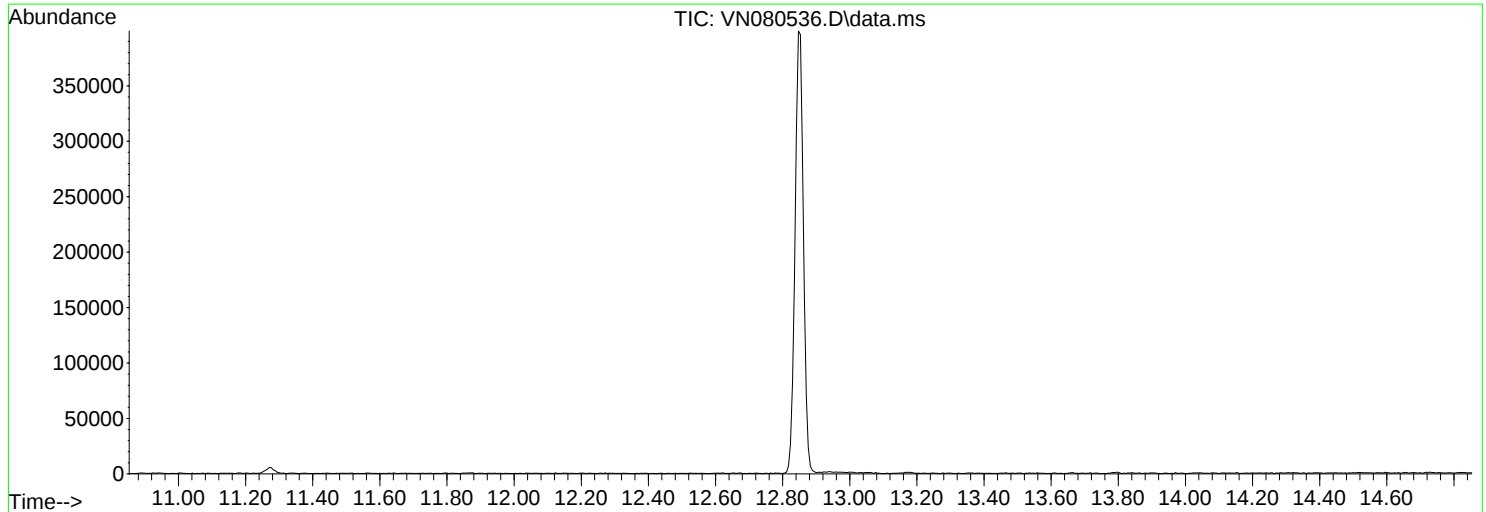

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	12652	PASS
75	95	30	60	54.7	40771	PASS
95	95	100	100	100.0	74477	PASS
96	95	5	9	6.3	4677	PASS
173	174	0.00	2	0.8	453	PASS
174	95	50	100	78.6	58531	PASS
175	174	5	9	7.7	4522	PASS
176	174	95	101	95.6	55981	PASS
177	176	5	9	6.5	3623	PASS

Average of 12.847 to 12.859 min.: VN080536.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	411	49.00	2752	63.95	383	76.05	383
36.20	287	50.10	12652	65.05	468	77.10	441
37.10	3240	51.05	3867	66.95	244	77.95	23
38.00	2669	51.90	285	68.00	7370	78.95	267
39.00	1059	54.90	290	69.05	7901	79.90	768
39.80	158	55.95	1095	70.05	686	80.90	2681
44.00	580	57.05	1941	71.85	424	81.80	479
44.95	575	60.00	791	72.10	75	82.00	148
46.90	636	61.00	3925	73.00	4057	87.00	2926
47.30	166	62.00	3601	74.00	12522	88.00	2538
48.05	551	63.05	2972	75.05	40771	90.85	471

Average of 12.847 to 12.859 min.: VN080536.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	2755	111.10	55	134.95	112	147.70	99
93.00	3686	115.00	53	136.60	165	147.95	209
94.05	9481	115.85	378	140.90	1047	154.80	68
95.05	74477	116.95	681	141.70	56	155.00	75
96.05	4677	117.85	406	141.95	117	156.90	120
97.20	59	118.80	545	143.00	1430	171.90	303
104.00	362	127.80	166	143.90	55	173.00	453
104.75	139	128.00	109	144.75	224	174.00	58531
105.90	287	128.90	54	145.90	63	174.95	4522
107.00	60	129.80	334	147.00	81	175.95	55981
109.70	53	133.80	63	147.20	114	177.00	3623

Average of 12.847 to 12.859 min.: VN080536.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
280.90	105						
281.05	173						
415.10	52						

Instrument :

MSVOA_N

ClientSampleId :

BFB