
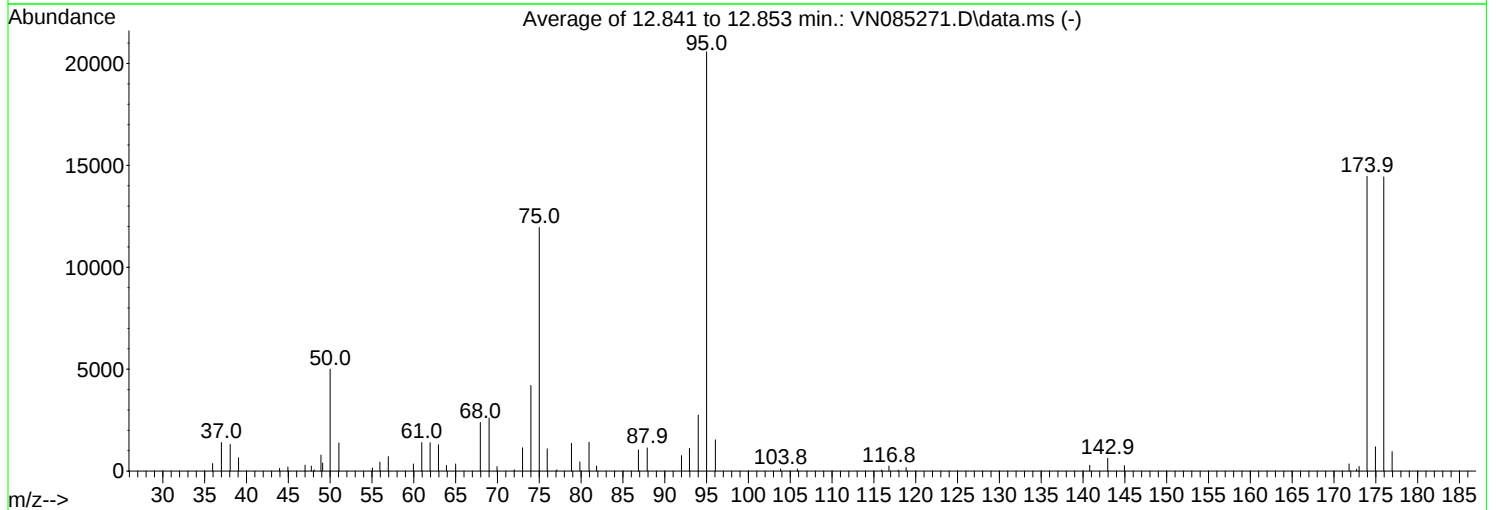


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122024\
Data File : VN085271.D
Acq On : 20 Dec 2024 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Dec 21 02:03:07 2024

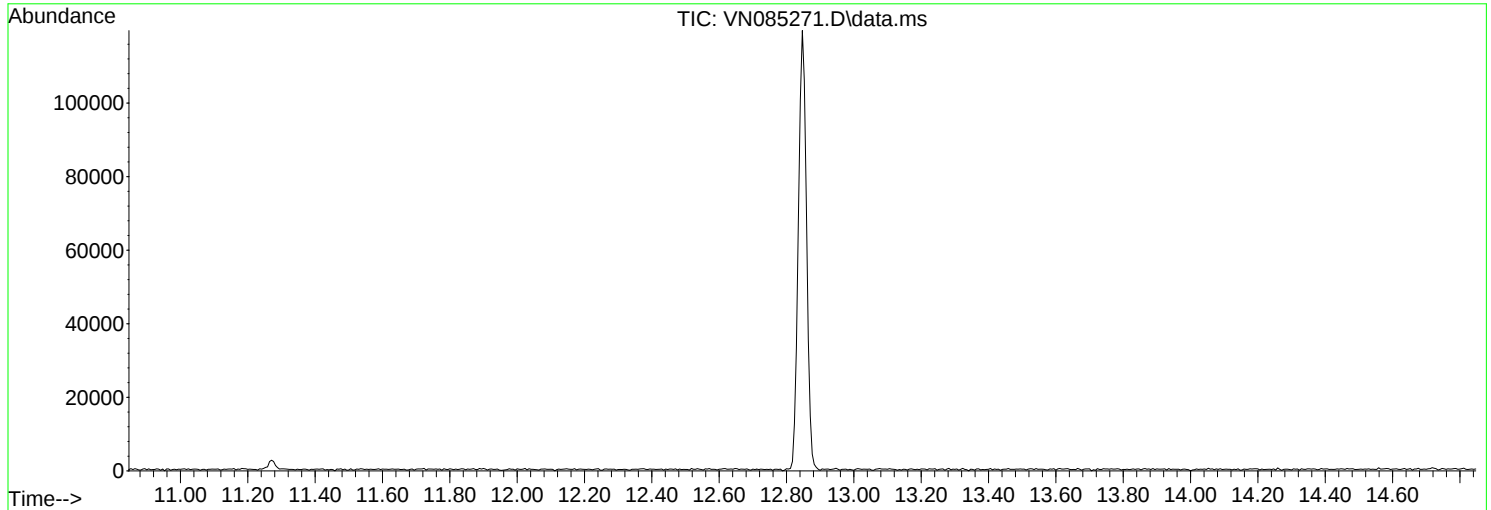

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	5003	PASS
75	95	30	60	58.1	11958	PASS
95	95	100	100	100.0	20576	PASS
96	95	5	9	7.5	1534	PASS
173	174	0.00	2	1.6	229	PASS
174	95	50	100	70.3	14462	PASS
175	174	5	9	8.2	1190	PASS
176	174	95	101	99.8	14434	PASS
177	176	5	9	6.6	957	PASS