


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122118\
 Data File : VN053091.D
 Acq On : 21 Dec 2018 8:34
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N112618W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Nov 27 00:48:33 2018

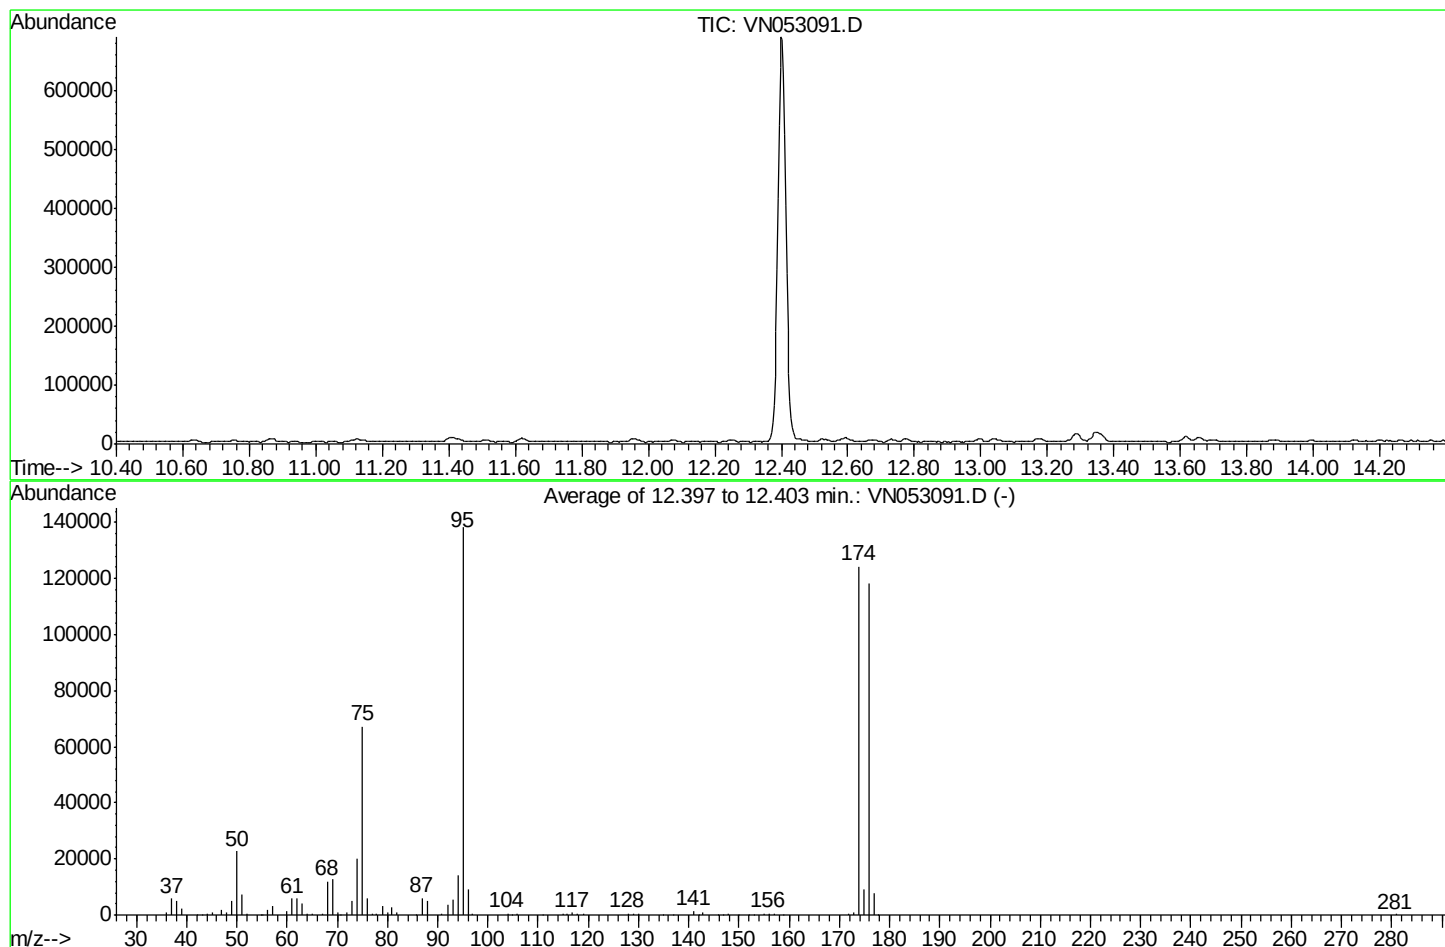

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	22728	PASS
75	95	30	60	48.6	67221	PASS
95	95	100	100	100.0	138304	PASS
96	95	5	9	6.6	9161	PASS
173	174	0.00	2	0.8	1031	PASS
174	95	50	100	89.8	124234	PASS
175	174	5	9	7.5	9263	PASS
176	174	95	101	95.2	118264	PASS
177	176	5	9	6.6	7830	PASS