


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN122118\
 Data File : VN053098.D
 Acq On : 21 Dec 2018 12:50
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Title : SW846 8260
 Last Update : Tue Dec 18 13:03:37 2018

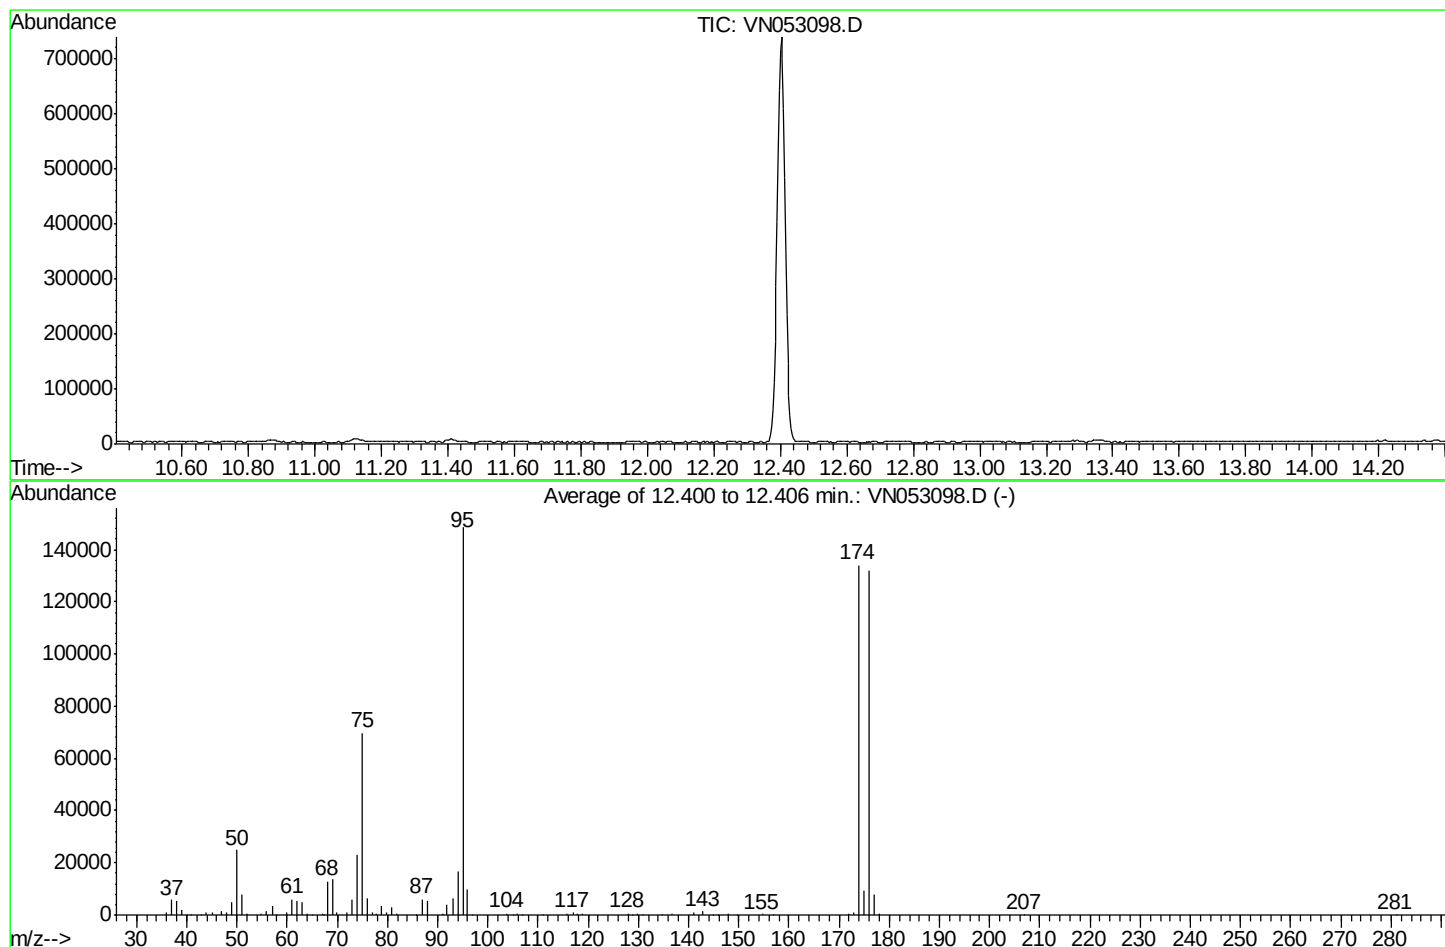

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	24842	PASS
75	95	30	60	46.9	69666	PASS
95	95	100	100	100.0	148544	PASS
96	95	5	9	6.6	9841	PASS
173	174	0.00	2	0.9	1182	PASS
174	95	50	100	90.1	133909	PASS
175	174	5	9	7.2	9580	PASS
176	174	95	101	98.5	131848	PASS
177	176	5	9	6.0	7882	PASS