
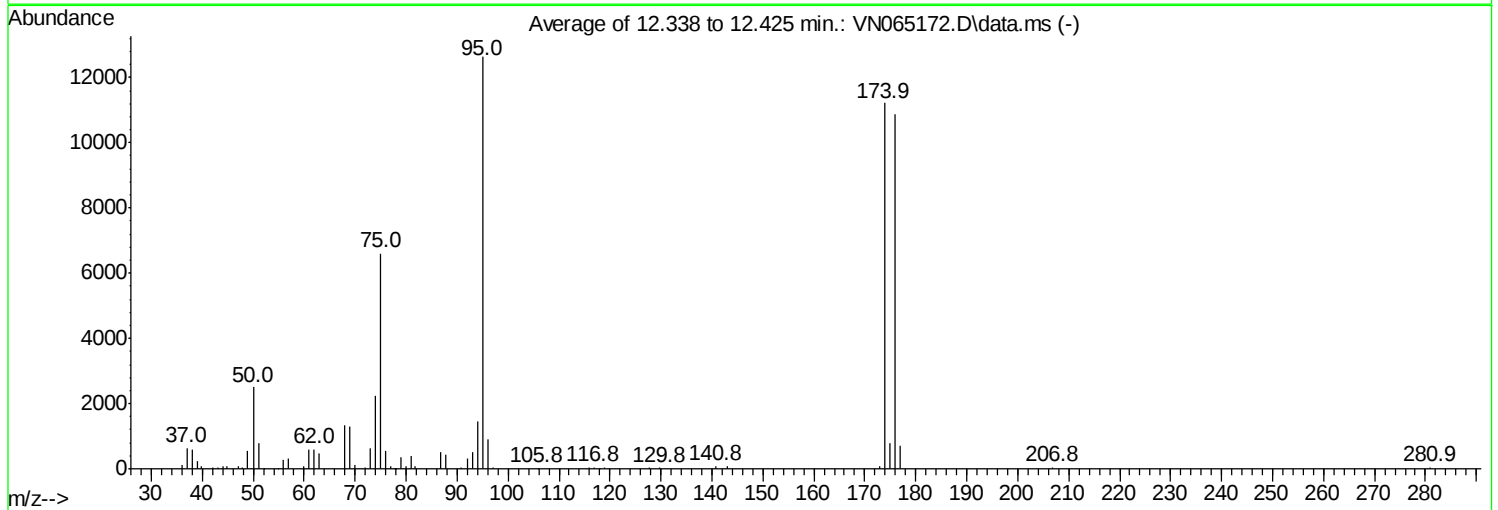


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122120\
 Data File : VN065172.D
 Acq On : 21 Dec 2020 10:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122120w.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Dec 21 13:17:58 2020

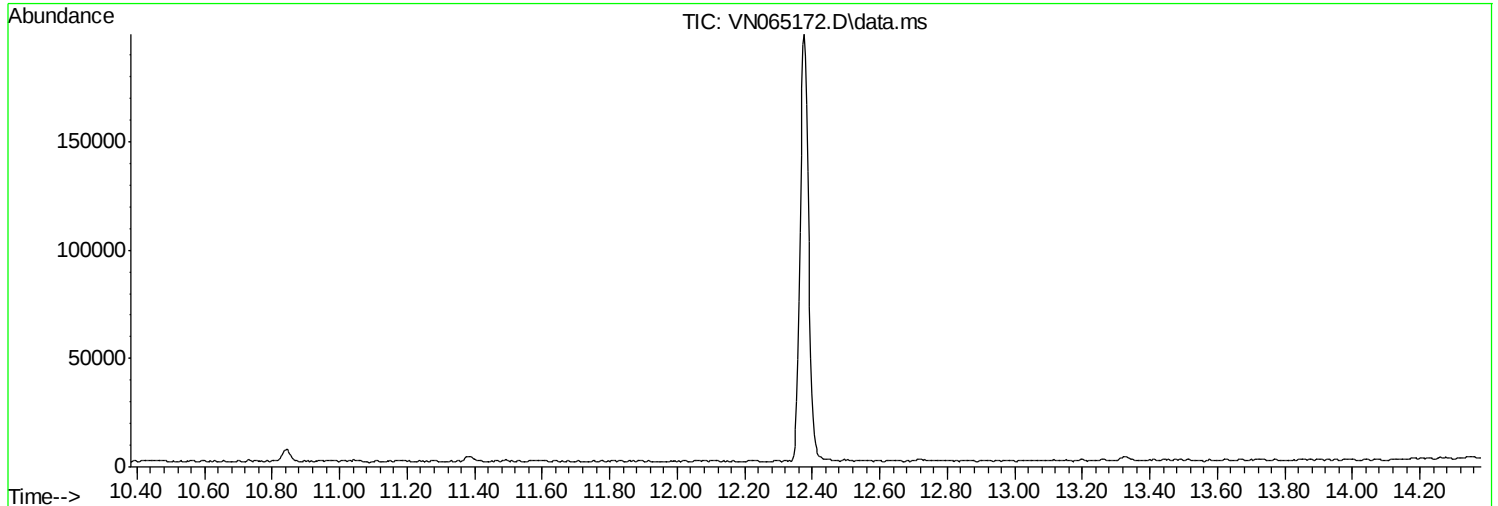

AutoFind: Averaged scan 3296 to 3323; Bkg corrected with scan 3295

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	2507	PASS
75	95	30	60	52.3	6613	PASS
95	95	100	100	100.0	12635	PASS
96	95	5	9	7.0	890	PASS
173	174	0.00	2	0.7	76	PASS
174	95	50	100	88.8	11221	PASS
175	174	5	9	7.2	803	PASS
176	174	95	101	96.9	10869	PASS
177	176	5	9	6.6	715	PASS