

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122122\
Data File : VN075926.D
Acq On : 21 Dec 2022 17:53
Operator : JC\MD
Sample : N6168-06 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M

Title : SW846 8260

Signal : TIC: VN075926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.836	125	133	140	rVB4	10627	30736	1.88%	0.355%
2	3.806	290	298	308	rBV3	8723	23948	1.46%	0.277%
3	4.306	372	383	395	rBV	13121	36813	2.25%	0.425%
4	8.177	1030	1041	1045	rBV	228836	554283	33.90%	6.406%
5	8.230	1045	1050	1063	rVB	451685	997712	61.02%	11.531%
6	8.583	1101	1110	1122	rBV	225319	510565	31.23%	5.901%
7	9.106	1190	1199	1211	rBV	608212	1221225	74.69%	14.114%
8	10.571	1437	1448	1460	rBV	880008	1635049	100.00%	18.897%
9	11.871	1661	1669	1683	rVB	777048	1405048	85.93%	16.239%
10	12.853	1827	1836	1847	rVB	598982	1014471	62.05%	11.725%
11	13.794	1988	1996	2006	rBV	727915	1222525	74.77%	14.129%




Sum of corrected areas: 8652375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122122\
Data File : VN075926.D
Acq On : 21 Dec 2022 17:53
Operator : JC\MD
Sample : N6168-06 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

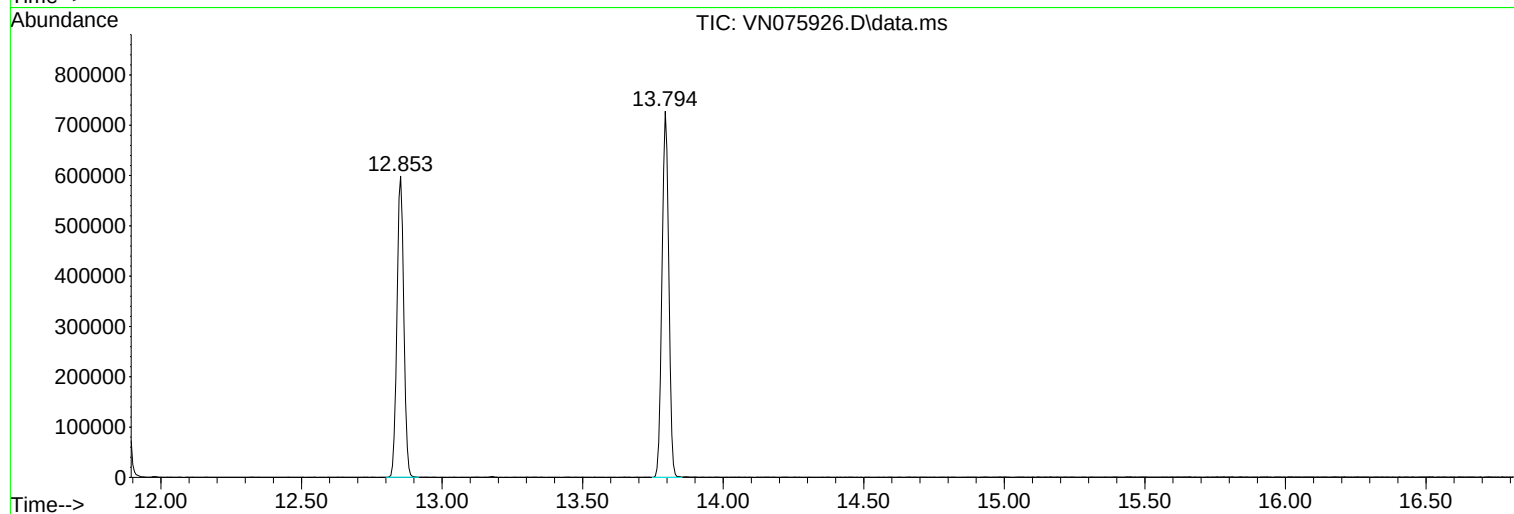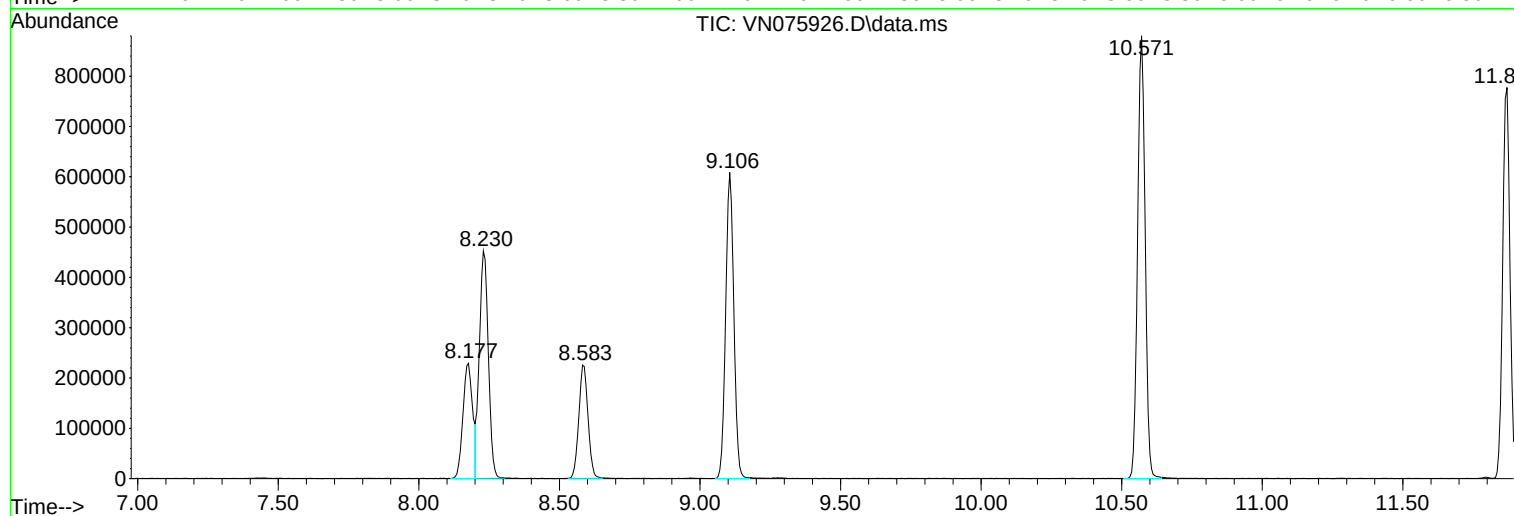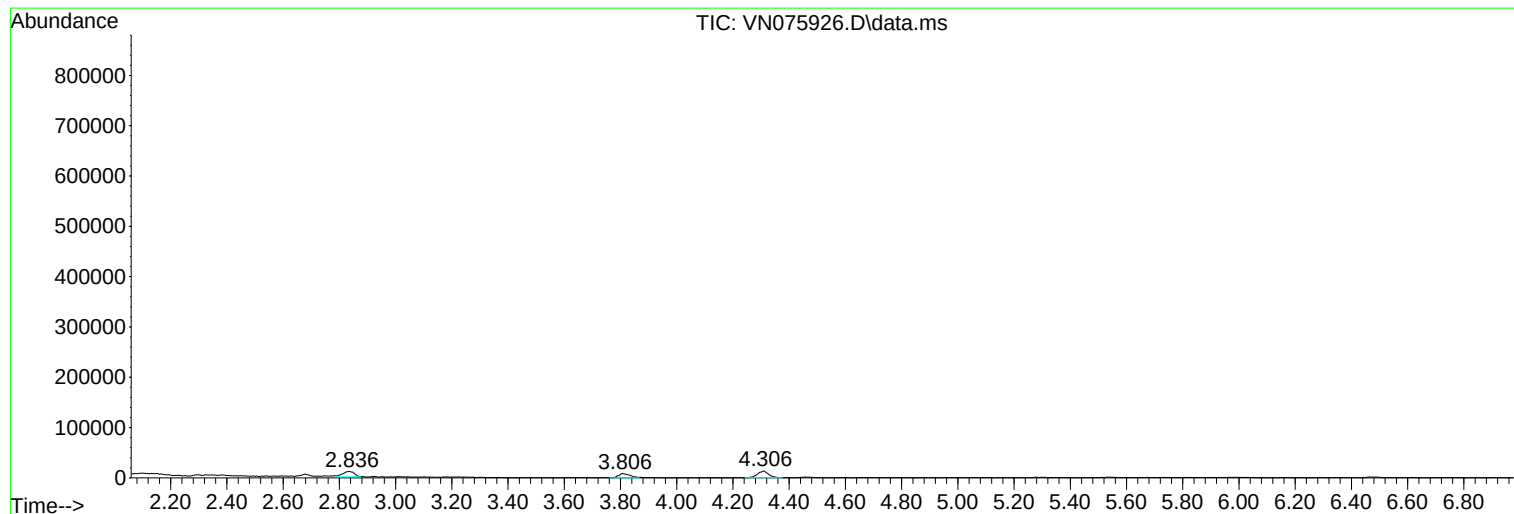

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122122\
Data File : VN075926.D
Acq On : 21 Dec 2022 17:53
Operator : JC\MD
Sample : N6168-06 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122122\
Data File : VN075926.D
Acq On : 21 Dec 2022 17:53
Operator : JC\MD
Sample : N6168-06 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc