


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN122122\  
 Data File : VN075907.D  
 Acq On : 21 Dec 2022 09:49  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
 Title : SW846 8260  
 Last Update : Wed Dec 14 13:03:41 2022

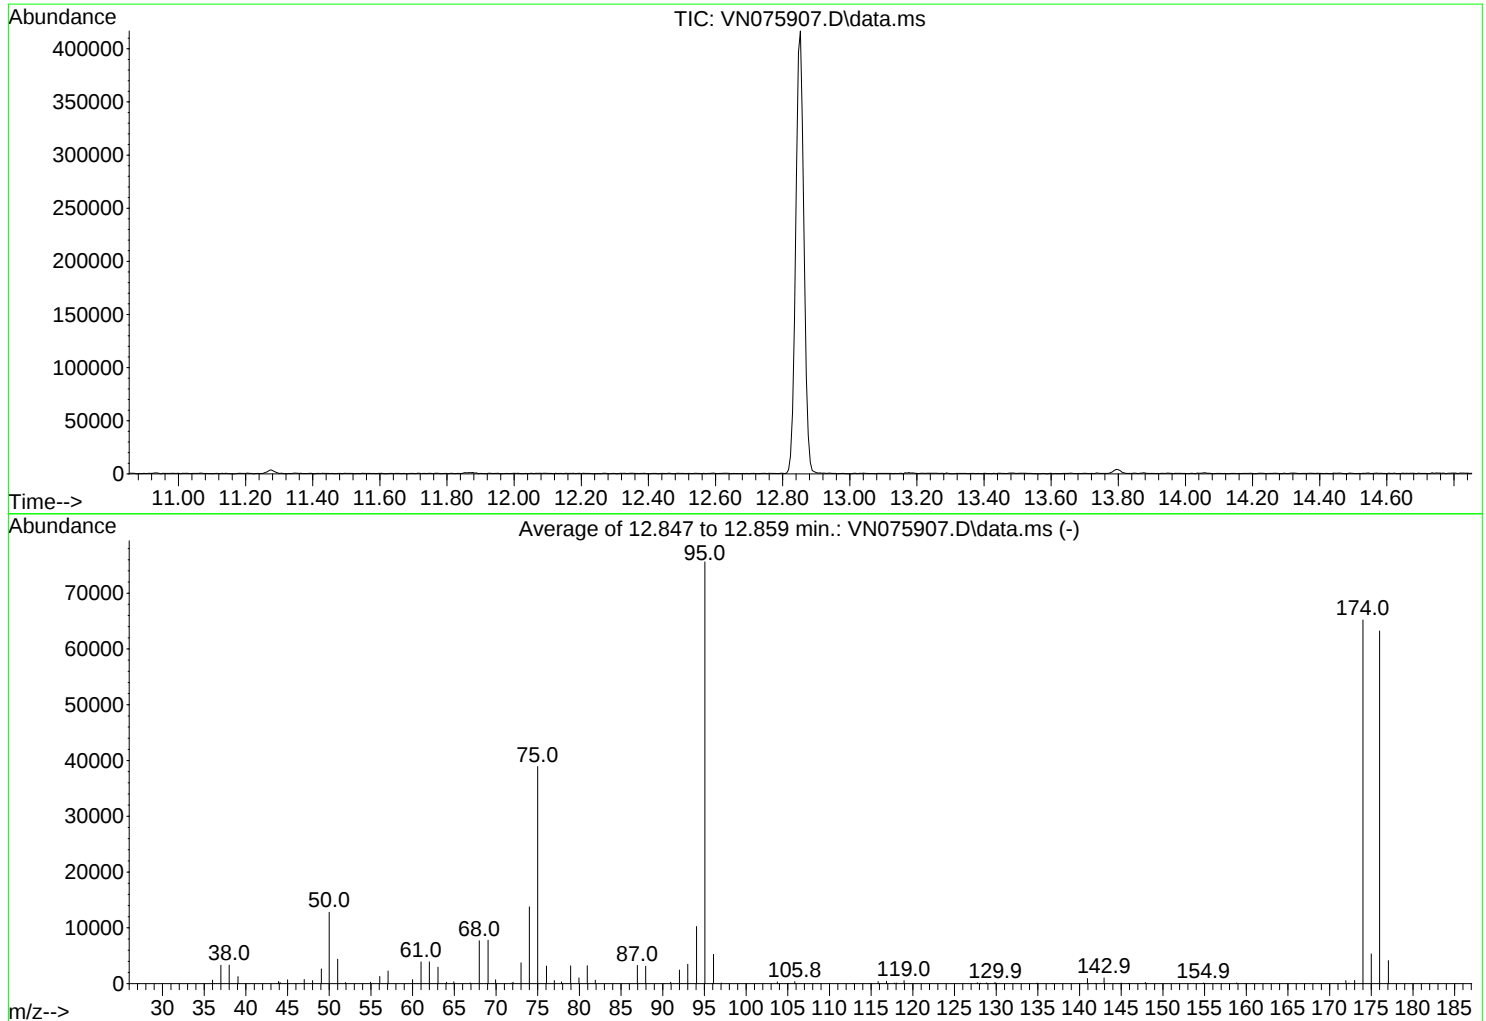

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.9         | 12803      | PASS                |
| 75             | 95              | 30              | 60              | 51.5         | 38936      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 75619      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 5247       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 565        | PASS                |
| 174            | 95              | 50              | 100             | 86.2         | 65189      | PASS                |
| 175            | 174             | 5               | 9               | 8.2          | 5325       | PASS                |
| 176            | 174             | 95              | 101             | 97.0         | 63219      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 4135       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 631    | 51.00 | 4390   | 66.90 | 145    | 77.85 | 30     |
| 37.00 | 3311   | 51.95 | 213    | 68.00 | 7692   | 78.95 | 318    |
| 38.00 | 3321   | 54.95 | 261    | 69.05 | 7786   | 79.95 | 103    |
| 39.05 | 1266   | 56.05 | 1285   | 69.95 | 690    | 80.95 | 322    |
| 43.90 | 361    | 57.05 | 2264   | 71.90 | 115    | 81.90 | 631    |
| 44.10 | 233    | 60.00 | 713    | 72.05 | 275    | 86.95 | 3261   |
| 45.00 | 686    | 61.00 | 3892   | 73.00 | 3729   | 87.95 | 3100   |
| 47.00 | 754    | 62.00 | 3901   | 74.00 | 13773  | 90.95 | 265    |
| 48.00 | 535    | 63.05 | 2962   | 75.00 | 38936  | 92.00 | 2441   |
| 49.05 | 2631   | 64.05 | 271    | 76.05 | 3162   | 93.00 | 3482   |
| 50.00 | 12803  | 64.95 | 353    | 77.00 | 560    | 94.05 | 10242  |

Average of 12.847 to 12.859 min.: VN075907.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 95.05  | 75619  | 118.05 | 122    | 142.95 | 1024   | 174.00 | 65189  |
| 96.10  | 5247   | 118.95 | 551    | 145.00 | 112    | 175.00 | 5325   |
| 97.05  | 118    | 127.75 | 169    | 145.90 | 70     | 176.00 | 63219  |
| 103.75 | 330    | 128.10 | 83     | 147.90 | 228    | 177.05 | 4135   |
| 105.10 | 53     | 128.85 | 149    | 148.10 | 55     |        |        |
| 105.85 | 375    | 129.80 | 139    | 154.90 | 157    |        |        |
| 112.90 | 57     | 129.95 | 180    | 158.85 | 143    |        |        |
| 114.90 | 57     | 134.90 | 128    | 160.80 | 51     |        |        |
| 115.85 | 372    | 136.80 | 57     | 171.95 | 561    |        |        |
| 116.85 | 444    | 140.95 | 932    | 172.30 | 109    |        |        |
| 117.80 | 126    | 141.90 | 52     | 173.00 | 565    |        |        |