

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
 Data File : VN080565.D
 Acq On : 21 Dec 2023 11:43
 Operator : JC\MD
 Sample : VN1221MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1221MBL01

Quant Time: Dec 22 03:56:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 13 01:57:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	232475	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	436219	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	452706	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	194995	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	160065	53.908	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 107.820%	
35) Dibromofluoromethane	8.165	113	140637	50.849	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.700%	
50) Toluene-d8	10.565	98	507037	49.155	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.320%	
62) 4-Bromofluorobenzene	12.847	95	196418	50.147	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.300%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
Data File : VN080565.D
Acq On : 21 Dec 2023 11:43
Operator : JC\MD
Sample : VN1221MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1221MBL01

Quant Time: Dec 22 03:56:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 13 01:57:14 2023
Response via : Initial Calibration




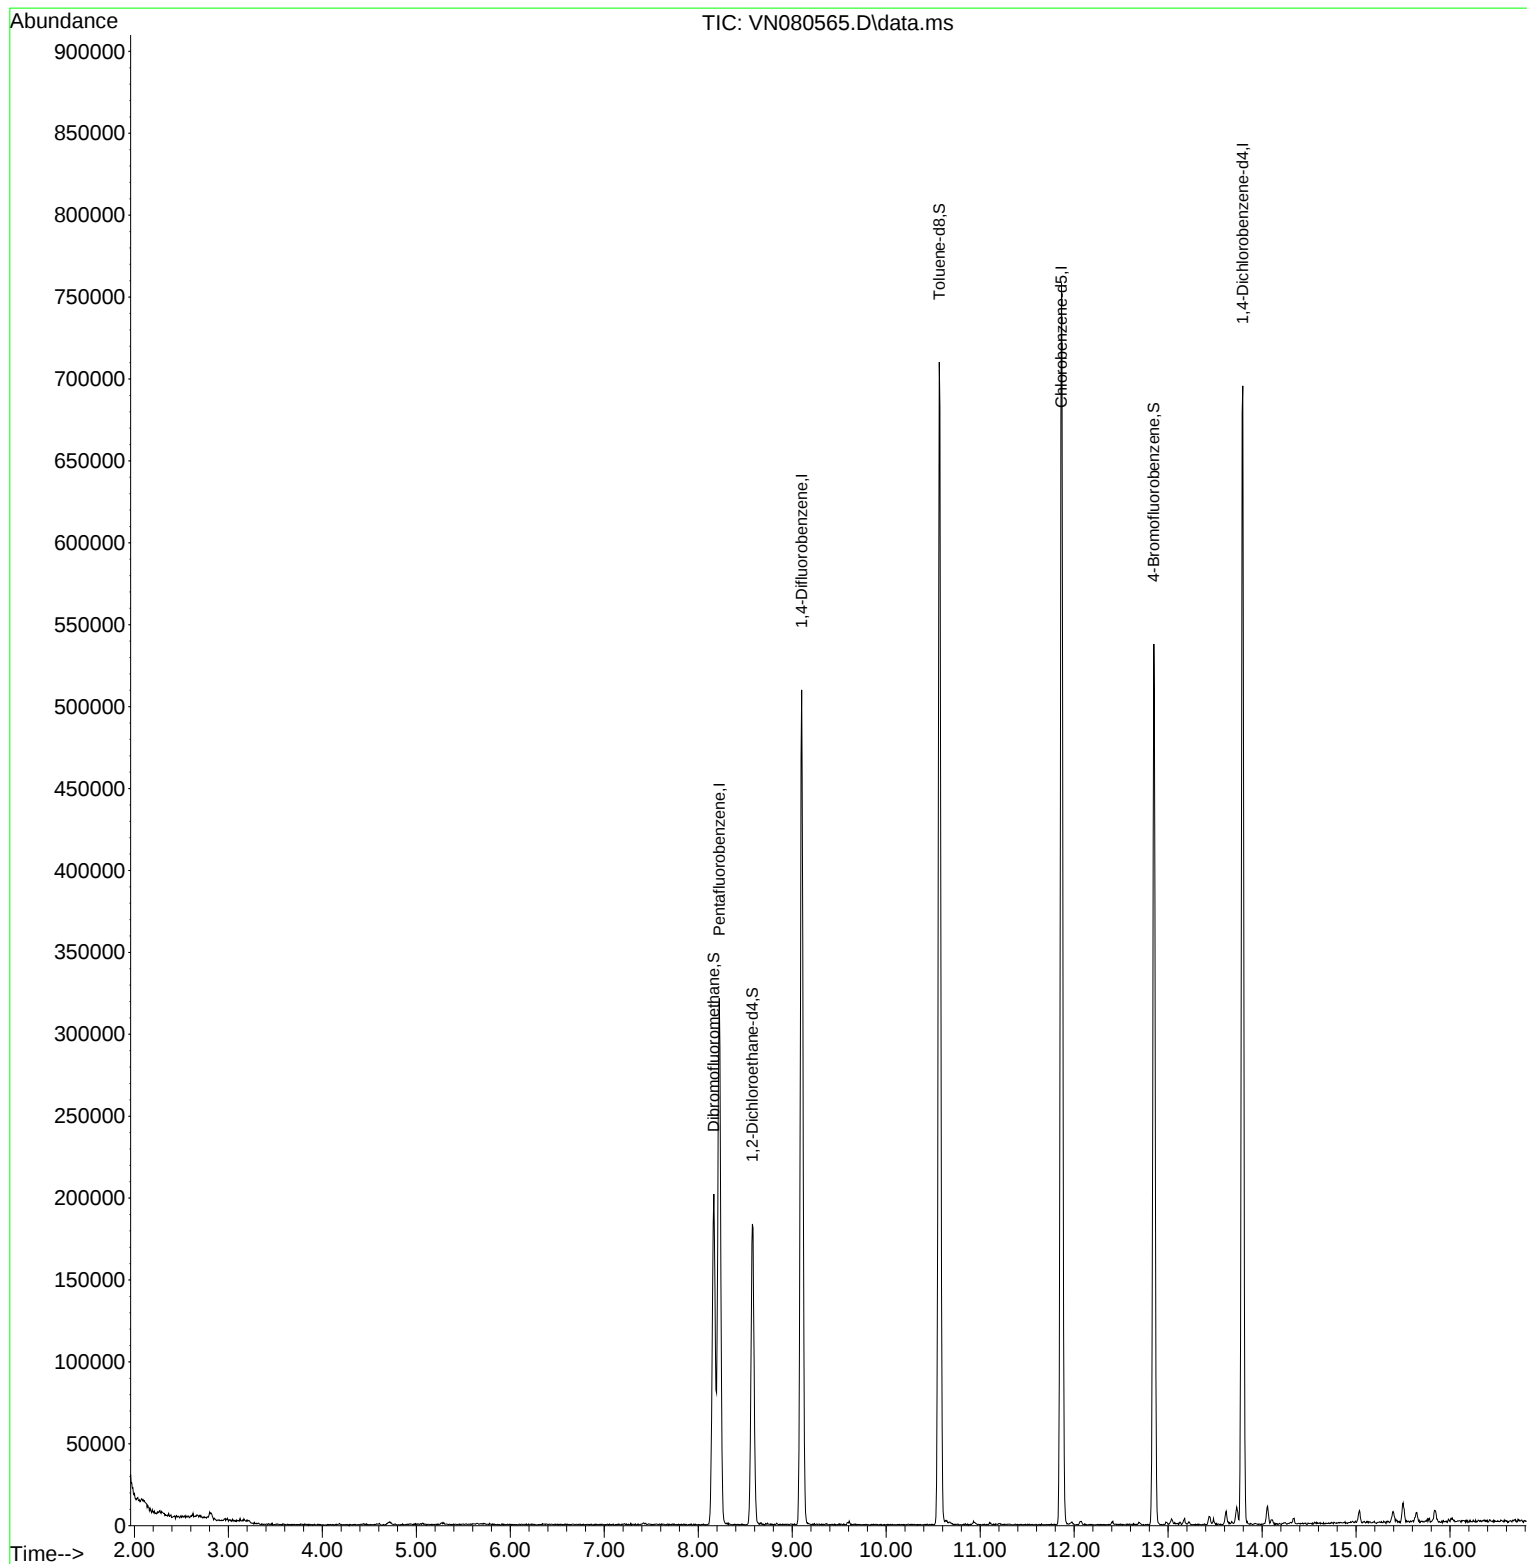


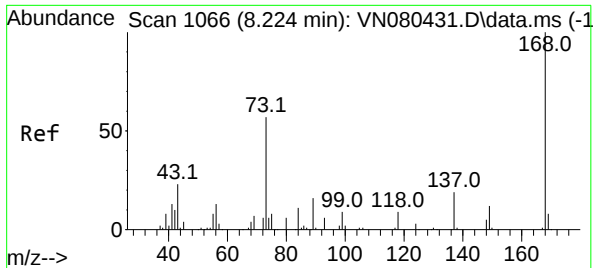

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43




Instrument :
MSVOA_N
ClientSampleId :
VN1221MBL01


Tgt Ion:168 Resp: 232475
Ion Ratio Lower Upper
168 100
99 63.2 53.0 79.6

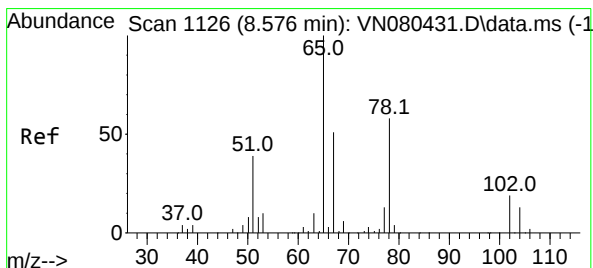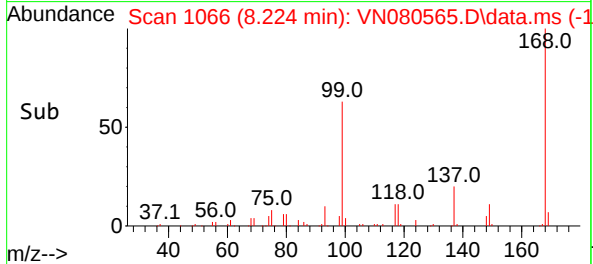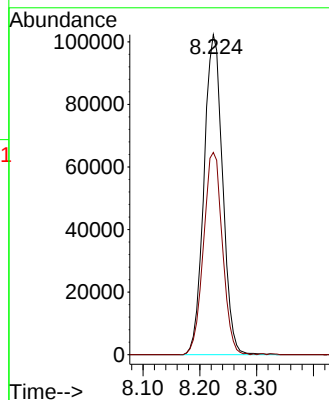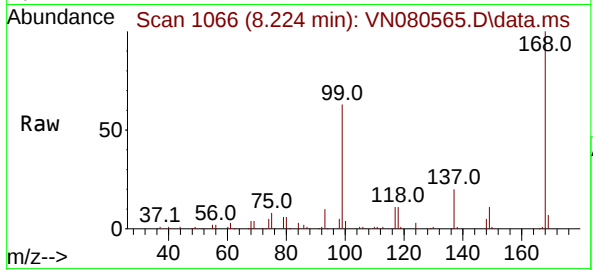

#33
1,2-Dichloroethane-d4
Concen: 53.908 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43

Tgt Ion: 65 Resp: 160065
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.6

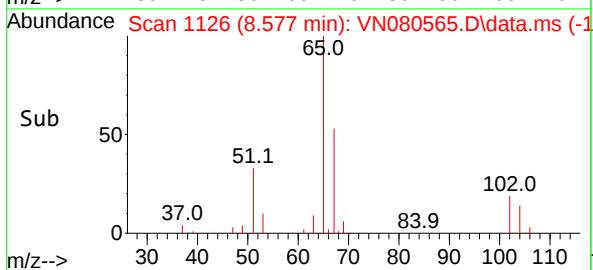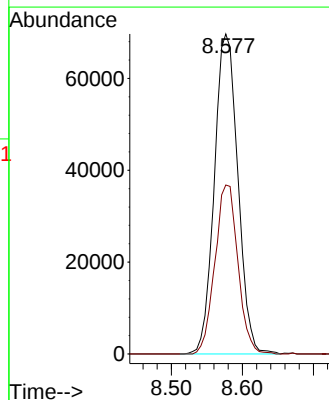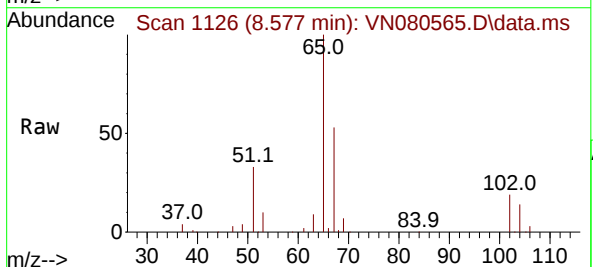

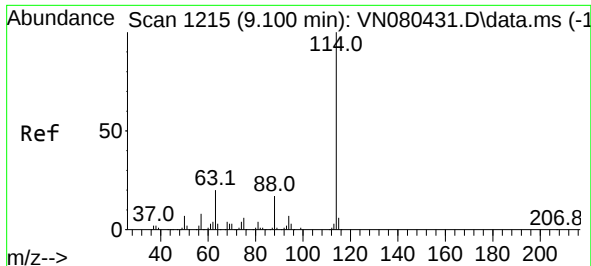

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN080565.D

Acq: 21 Dec 2023 11:43

Instrument :

MSVOA_N

ClientSampleId :

VN1221MBL01





Tgt Ion:114 Resp: 436219

Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.4

88 17.1 0.0 30.6

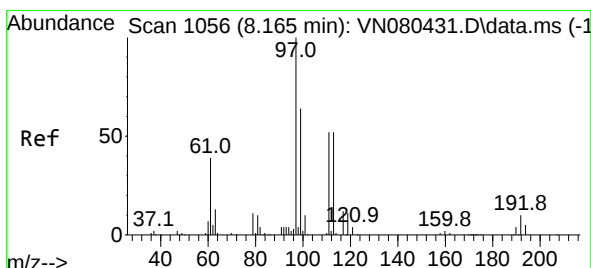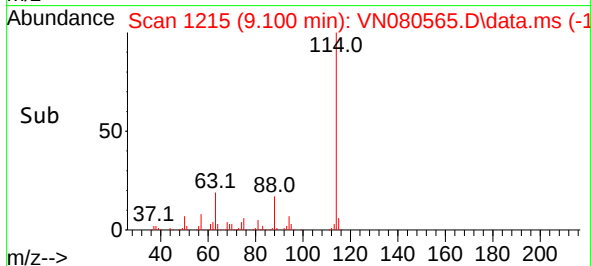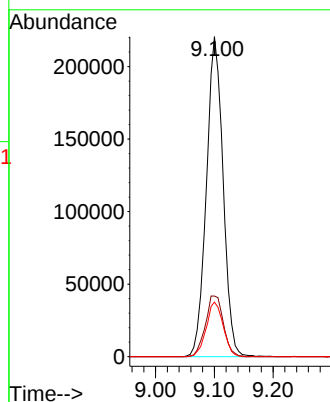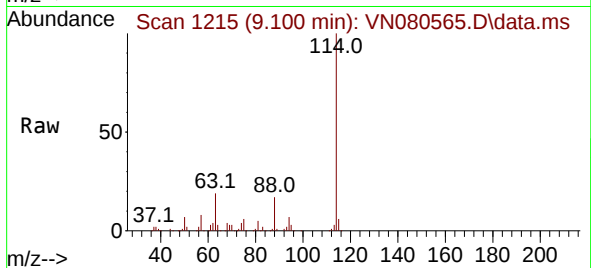

#35

Dibromofluoromethane

Concen: 50.849 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN080565.D

Acq: 21 Dec 2023 11:43




Tgt Ion:113 Resp: 140637


Ion Ratio Lower Upper

113 100

111 103.3 82.6 123.8

192 18.7 12.7 19.1


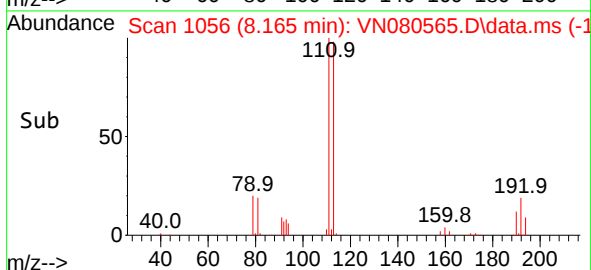
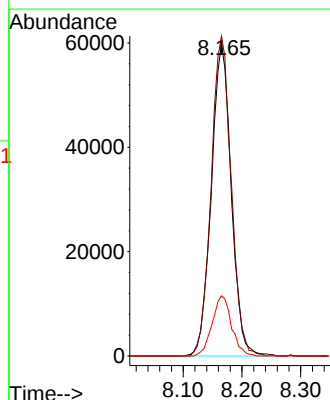
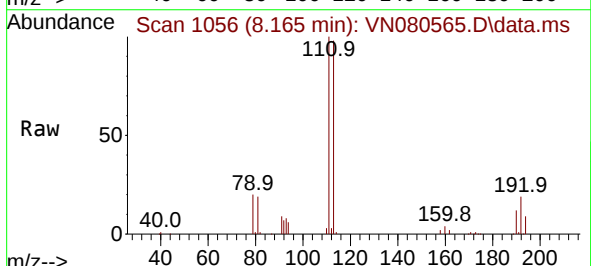


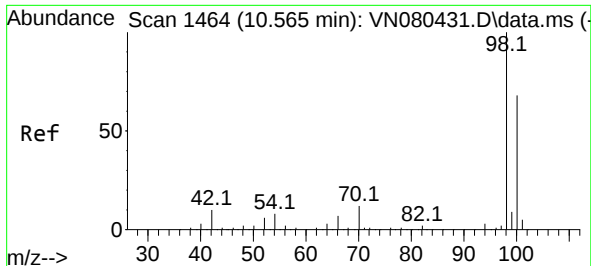

#50
Toluene-d8
Concen: 49.155 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43




Instrument :
MSVOA_N
ClientSampleId :
VN1221MBL01


Tgt Ion: 98 Resp: 507037
Ion Ratio Lower Upper
98 100
100 65.7 52.0 78.0

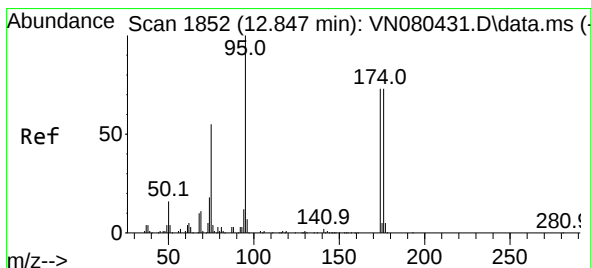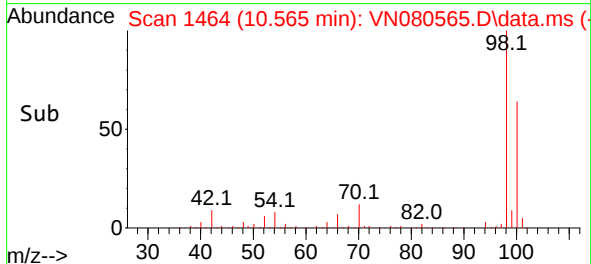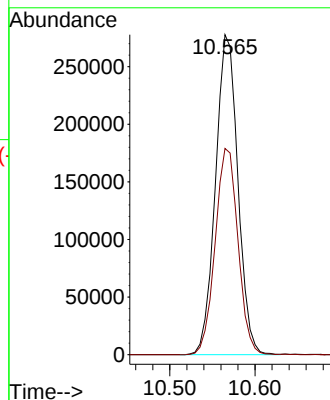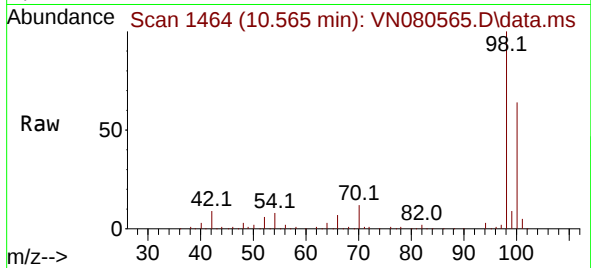

#62
4-Bromofluorobenzene
Concen: 50.147 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43

Tgt Ion: 95 Resp: 196418
Ion Ratio Lower Upper
95 100
174 74.1 0.0 143.8
176 71.0 0.0 135.8


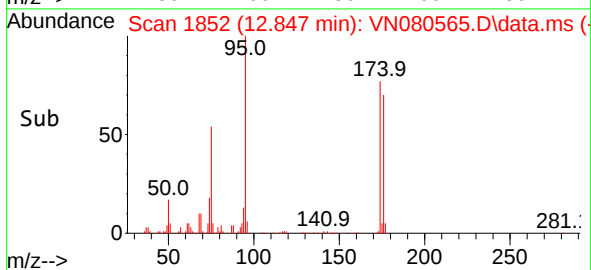
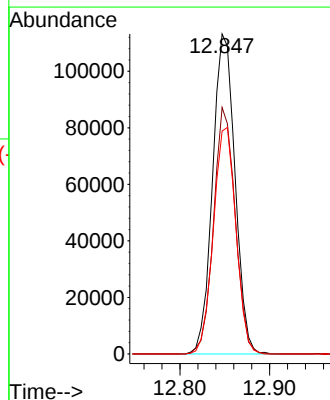
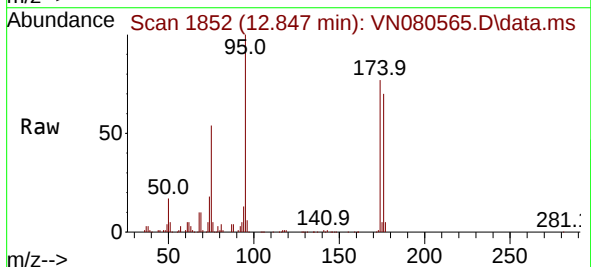


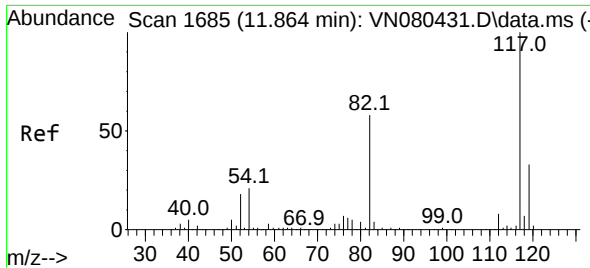

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43

Instrument :
MSVOA_N
ClientSampleId :
VN1221MBL01

Tgt Ion:117 Resp: 452706
Ion Ratio Lower Upper
117 100
82 59.2 44.0 66.0
119 32.8 25.6 38.4

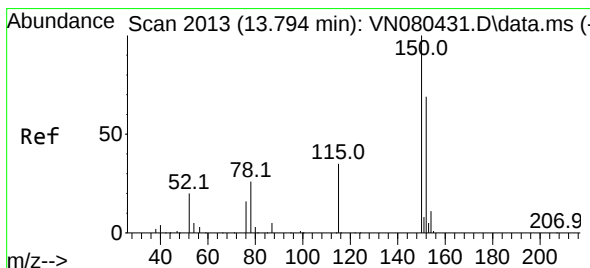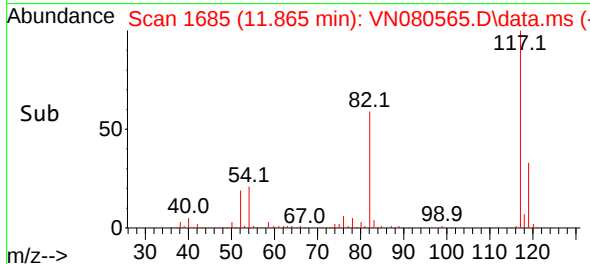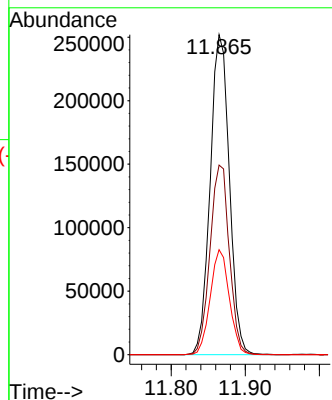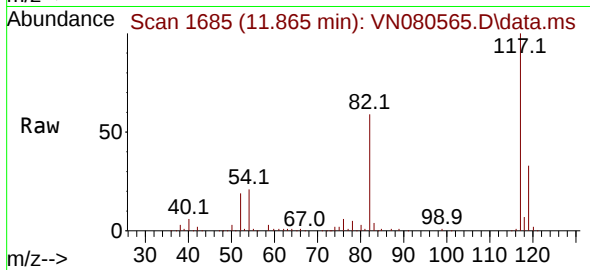

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080565.D
Acq: 21 Dec 2023 11:43

Tgt Ion:152 Resp: 194995
Ion Ratio Lower Upper
152 100
115 64.0 32.3 96.8
150 156.3 0.0 355.8

