

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
 Data File : VN080583.D
 Acq On : 21 Dec 2023 19:01
 Operator : JC\MD
 Sample : 05975-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FB01-122023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M

Title : SW846 8260

Signal : TIC: VN080583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.430	920	931	944	rVB	24322	65902	2.97%	0.454%
2	8.171	1044	1057	1061	rBV2	325939	782434	35.22%	5.390%
3	8.224	1061	1066	1081	rVB	507311	1093525	49.23%	7.533%
4	8.577	1117	1126	1136	rBV	320216	683040	30.75%	4.705%
5	9.100	1204	1215	1227	rBV	862730	1748531	78.71%	12.045%
6	10.571	1454	1465	1475	rBV	1206084	2221471	100.00%	15.303%
7	11.865	1677	1685	1698	rBV	1231986	2153926	96.96%	14.838%
8	12.853	1844	1853	1862	rBV	883594	1512345	68.08%	10.418%
9	13.794	2005	2013	2023	rBV	1296479	2132655	96.00%	14.691%
10	14.100	2055	2065	2074	rBV7	9288	30263	1.36%	0.208%
11	15.235	2243	2258	2282	rBV2	571644	2092389	94.19%	14.414%




Sum of corrected areas: 14516481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
Data File : VN080583.D
Acq On : 21 Dec 2023 19:01
Operator : JC\MD
Sample : 05975-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB01-122023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

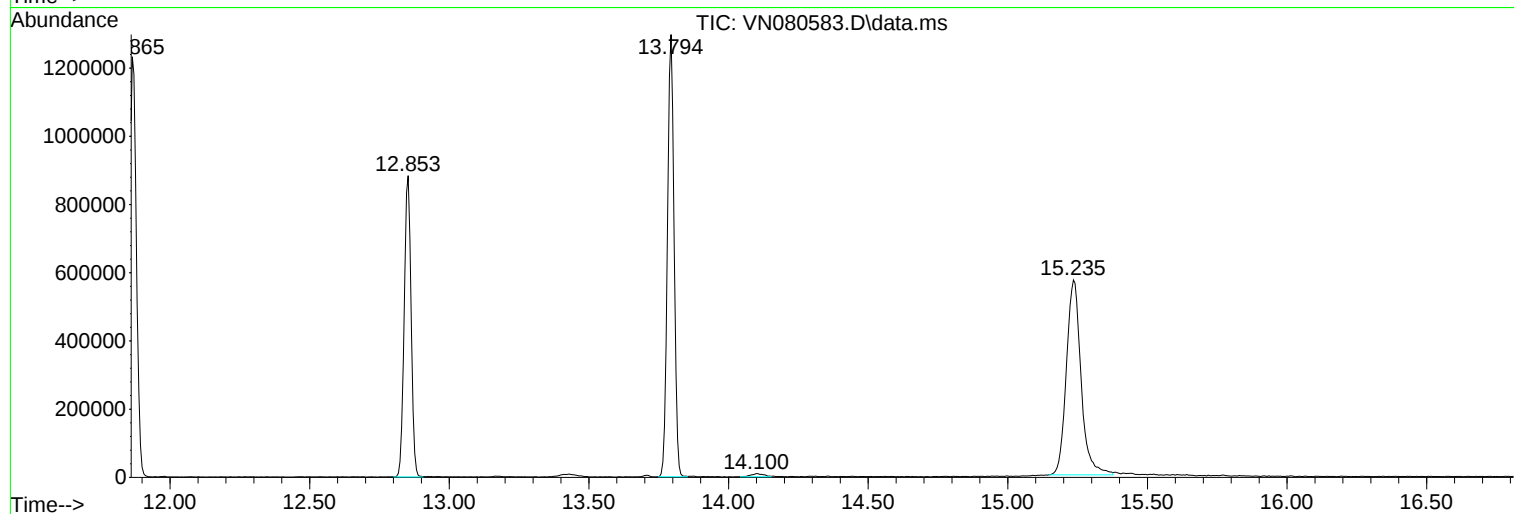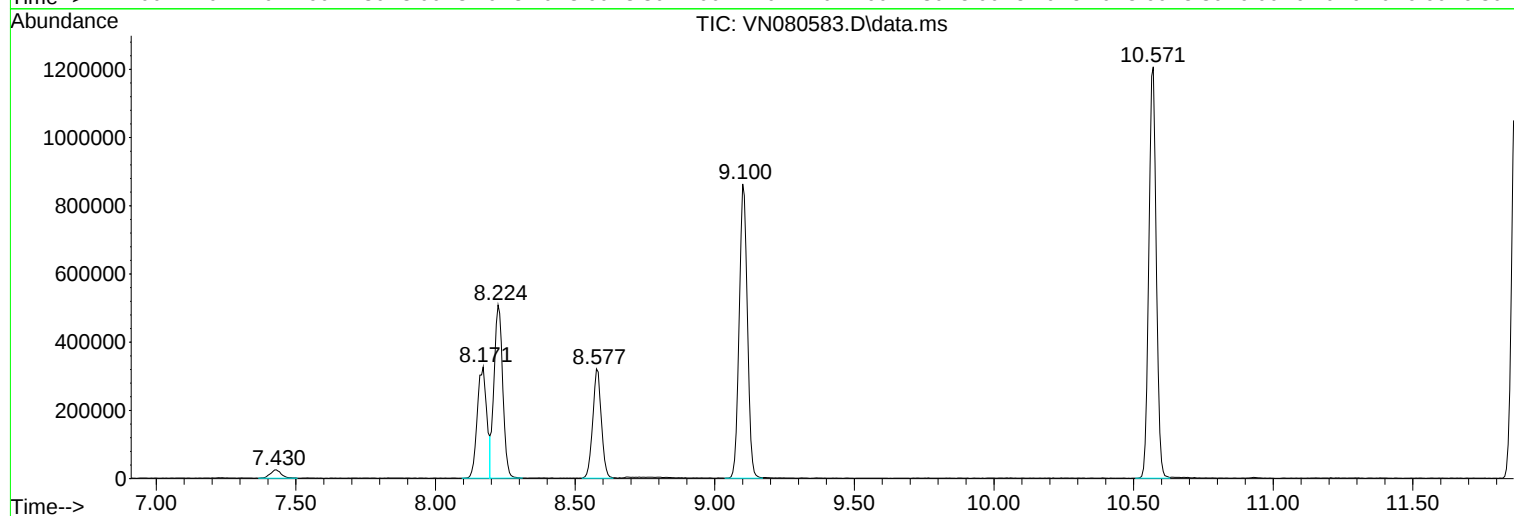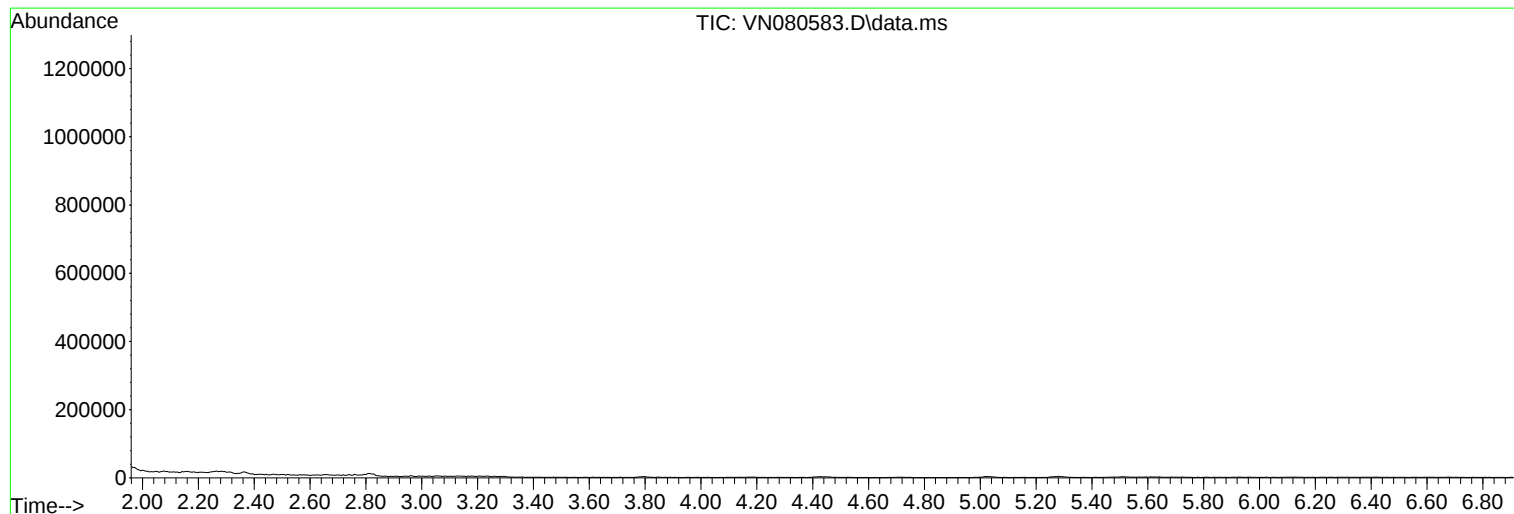

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
Data File : VN080583.D
Acq On : 21 Dec 2023 19:01
Operator : JC\MD
Sample : 05975-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB01-122023










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 trans-.beta.-Ionone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.235	49.06 ug/l	2092390	1,4-Dichlorobenzene-d4	13.794

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			trans-.beta.-Ionone	192	C13H20O	000079-77-6	98
2			3-Buten-2-one, 4-(2,6,6-trimethy...	192	C13H20O	014901-07-6	98
3			5-Aminomethylene-6-hydroxy-4-met...	177	C8H7N3O2	1000223-27-4	50
4			2,6-Diisopropylanisole	192	C13H20O	002944-52-7	50
5			2-(1,1-Dimethylethyl)-6-(1-methy...	192	C13H20O	022791-95-3	50

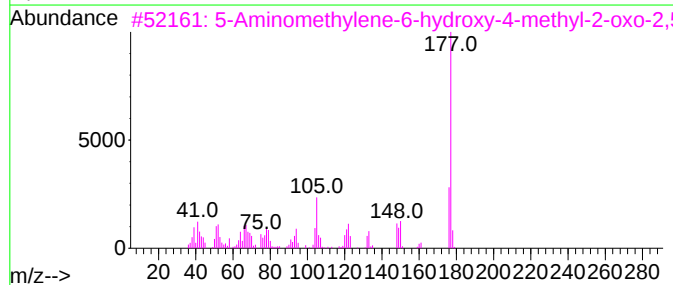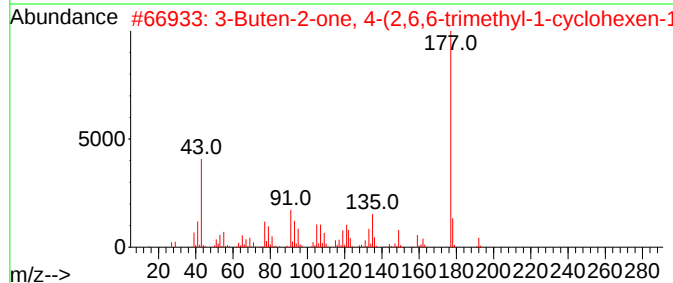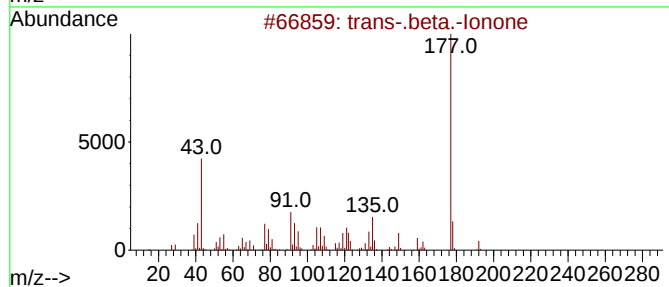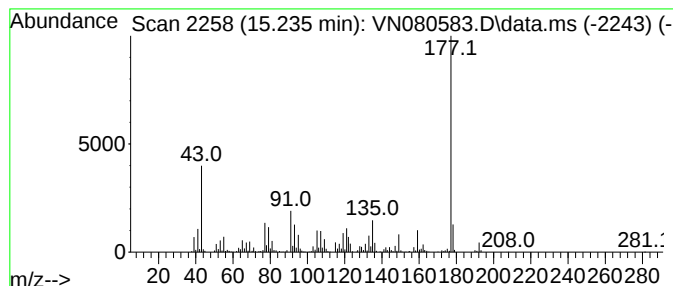

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
Data File : VN080583.D
Acq On : 21 Dec 2023 19:01
Operator : JC\MD
Sample : 05975-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB01-122023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
trans-.beta.-Io...	15.235	49.1	ug/l	2092390	4	13.794	2132660	50.0