
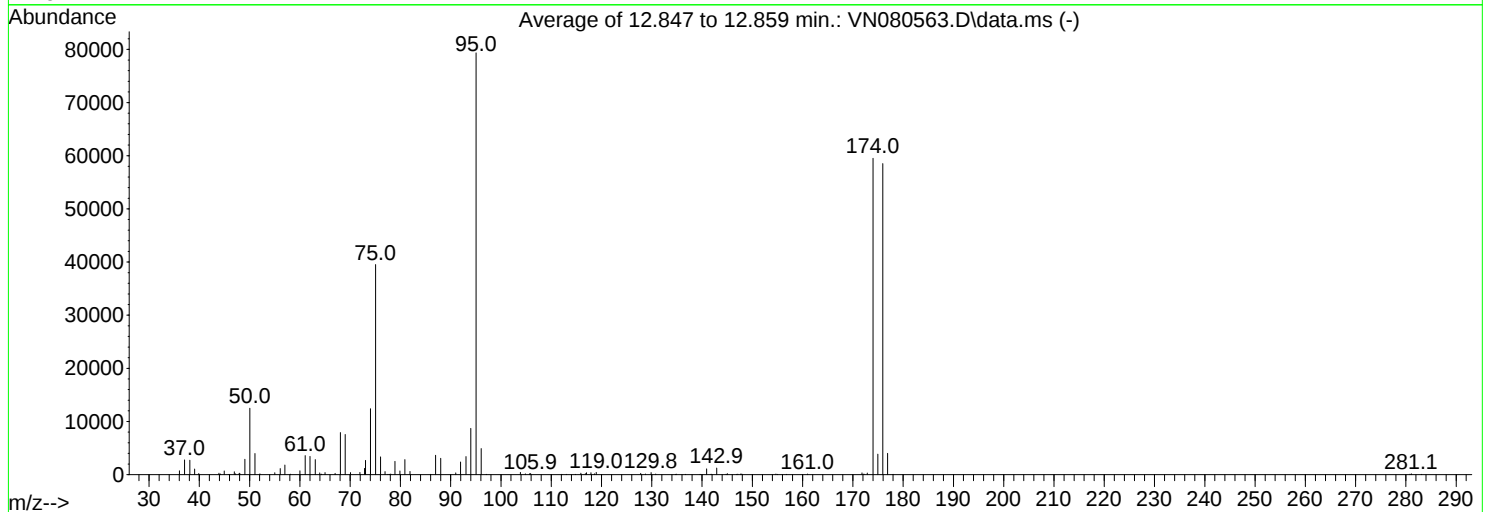


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122123\
Data File : VN080563.D
Acq On : 21 Dec 2023 10:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121223W.M
Title : SW846 8260
Last Update : Wed Dec 13 01:57:14 2023

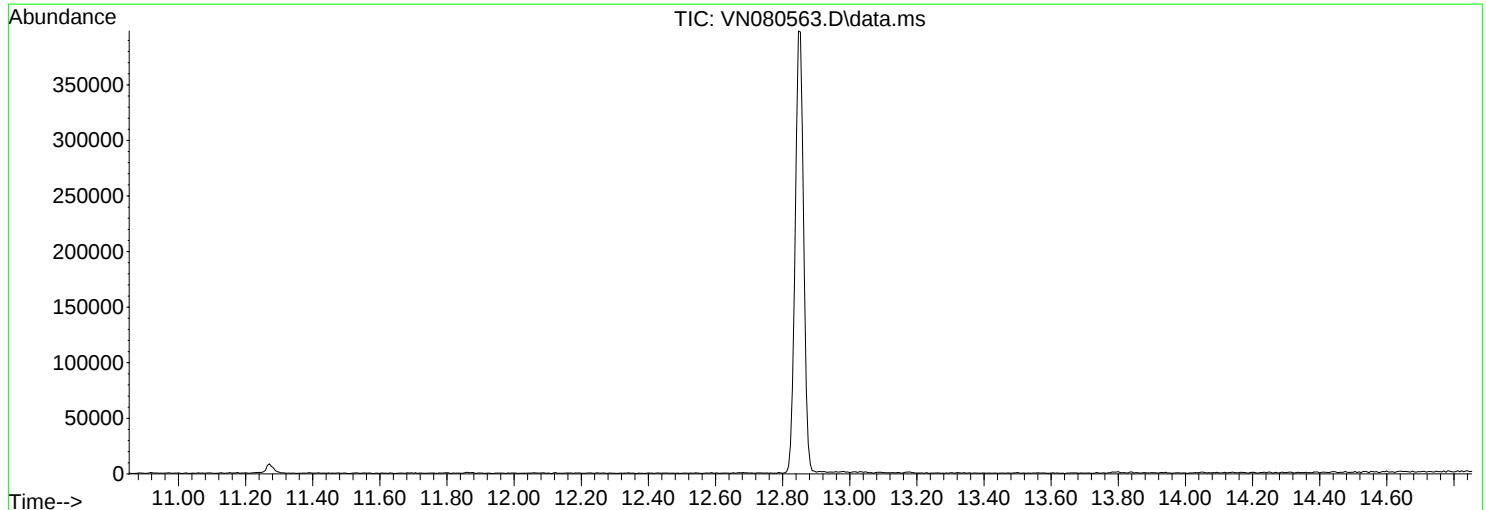

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	12495	PASS
75	95	30	60	49.8	39515	PASS
95	95	100	100	100.0	79352	PASS
96	95	5	9	6.2	4913	PASS
173	174	0.00	2	0.5	288	PASS
174	95	50	100	75.0	59512	PASS
175	174	5	9	6.5	3845	PASS
176	174	95	101	98.4	58531	PASS
177	176	5	9	6.8	3998	PASS

Average of 12.847 to 12.859 min.: VN080563.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	729	47.90	224	61.05	3575	72.85	118
37.05	2775	48.05	286	62.00	3431	73.05	268
38.10	2696	49.05	2897	63.05	2830	74.05	1240
39.05	1044	50.05	12495	63.95	335	75.05	3951
39.90	222	51.05	3979	64.30	89	76.05	3347
43.90	272	52.05	151	65.00	393	76.95	566
44.20	128	55.00	366	67.00	240	77.50	68
44.95	700	56.10	1151	68.05	7935	77.80	76
45.90	53	57.00	1818	69.00	7570	78.10	119
46.95	546	58.10	85	70.05	402	78.90	2492
47.20	154	60.00	717	71.95	425	79.90	683

Average of 12.847 to 12.859 min.: VN080563.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	2820	97.10	59	117.90	355	140.90	1091
81.90	593	103.85	428	118.60	154	141.80	99
86.00	54	104.85	142	118.95	421	142.90	1227
87.00	3657	105.70	179	127.80	257	144.80	93
88.00	3070	105.90	211	128.75	126	145.05	178
91.00	337	112.10	52	129.85	380	146.90	75
91.95	2382	113.00	54	130.80	124	147.10	85
93.05	3399	114.80	62	134.70	54	147.70	128
94.00	8714	115.90	262	134.90	104	147.90	110
95.05	79352	116.80	172	136.70	50	154.70	134
96.05	4913	117.00	353	139.60	50	155.00	63

Average of 12.847 to 12.859 min.: VN080563.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.80	52	281.10	160				
161.00	137	283.10	57				
171.80	346						
172.20	119						
172.85	288						
174.00	59512						
174.95	3845						
175.95	58531						
176.90	3998						
178.00	57						
280.80	80						

Instrument :

MSVOA_N

ClientSampleId :

BFB