


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122218\
 Data File : VN053147.D
 Acq On : 22 Dec 2018 22:05
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N121818W.M
 Title : SW846 8260
 Last Update : Tue Dec 18 13:03:37 2018

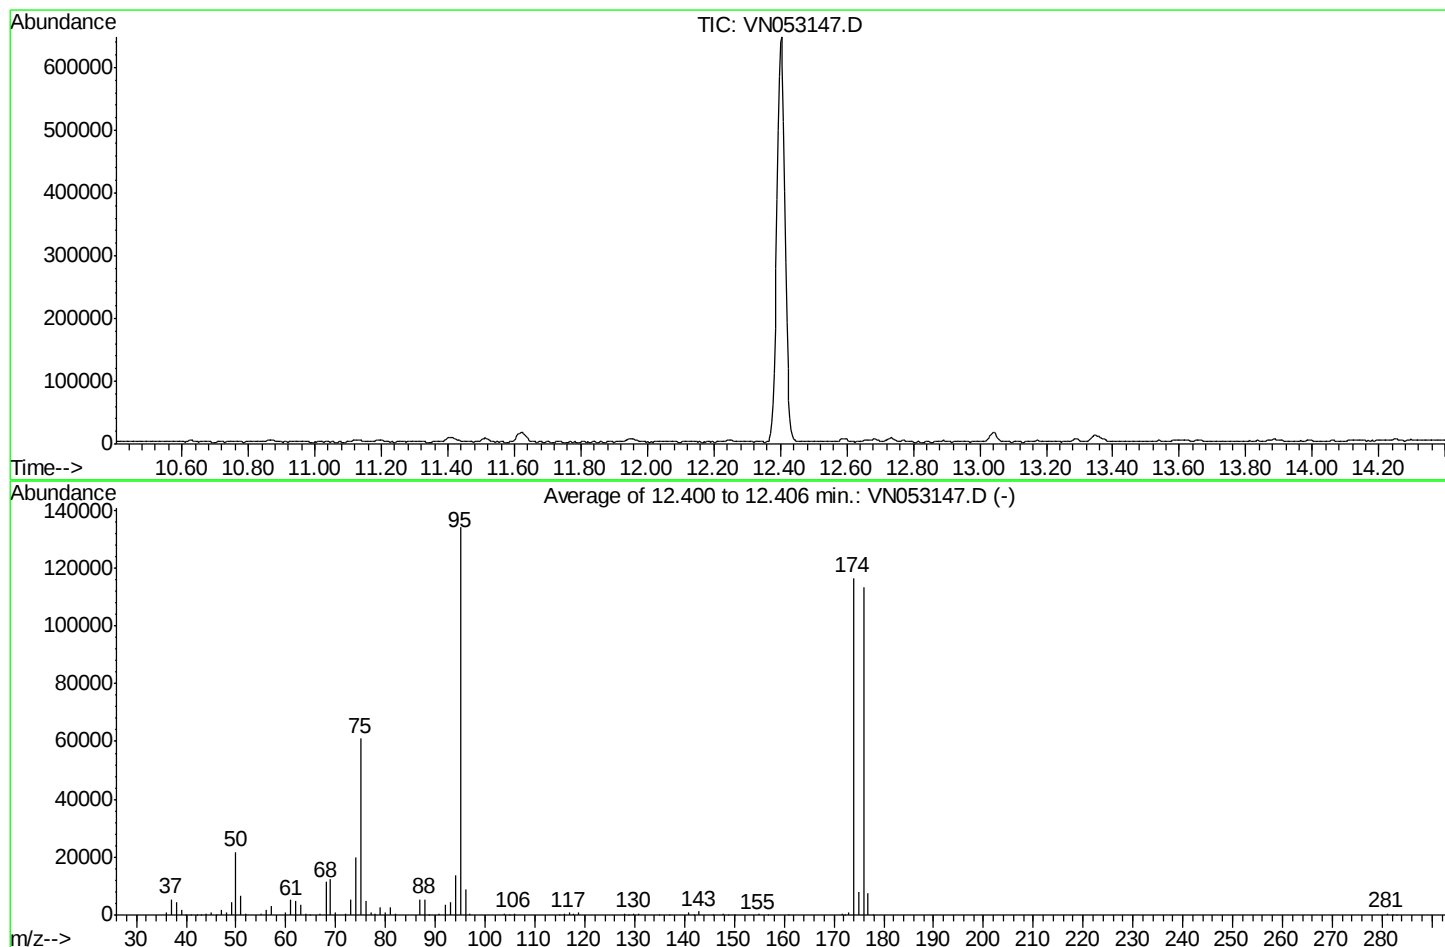

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	21848	PASS
75	95	30	60	45.5	60984	PASS
95	95	100	100	100.0	134053	PASS
96	95	5	9	6.6	8831	PASS
173	174	0.00	2	0.9	1000	PASS
174	95	50	100	86.9	116429	PASS
175	174	5	9	6.8	7962	PASS
176	174	95	101	97.5	113538	PASS
177	176	5	9	6.5	7333	PASS