

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122220\
 Data File : VN065216.D
 Acq On : 22 Dec 2020 23:28
 Operator : JC/MD
 Sample : L5159-22 50X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CGP-11

Quant Time: Dec 23 03:46:42 2020
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 22 15:42:18 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.627	168	235675	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	390389	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.379	117	407155	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.318	152	193619	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.990	65	140015	52.63	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 105.26%			
35) Dibromofluoromethane	7.553	113	121608	51.63	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 103.26%			
50) Toluene-d8	10.058	98	483903	54.82	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 109.64%			
62) 4-Bromofluorobenzene	12.376	95	200438	56.66	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 113.32%			
Target Compounds						Qvalue
11) Tert butyl alcohol	4.772	59	18985	43.61	ug/l #	93
13) Acrolein	3.569	56	171	2.99	ug/l #	50
16) Acetone	3.785	43	39990	26.19	ug/l	97
18) Methyl Acetate	4.296	43	6530	2.73	ug/l #	83
20) Methylene Chloride	4.511	84	1238	0.48	ug/l #	91
22) Diisopropyl ether	5.897	45	8788	1.16	ug/l #	1
25) 2-Butanone	6.804	43	18557	12.42	ug/l	100
29) Tetrahydrofuran	7.174	42	562	0.58	ug/l #	32
31) Cyclohexane	7.624	56	5316	1.35	ug/l #	20
36) 1,1-Dichloropropene	7.627	75	15688	4.42	ug/l #	49
37) Ethyl Acetate	6.804	43	18557	5.27	ug/l #	66
38) Carbon Tetrachloride	7.627	117	20020	5.37	ug/l #	16
40) Benzene	8.003	78	54325	5.14	ug/l	96
43) Isopropyl Acetate	7.984	43	48652	8.02	ug/l #	67
48) Methyl methacrylate	9.135	41	9817	3.33	ug/l #	40
49) 1,4-Dioxane	9.170	88	1980	41.50	ug/l #	26
51) 4-Methyl-2-Pentanone	9.955	43	8283	2.43	ug/l	100
52) Toluene	10.125	92	66074	9.93	ug/l	99
53) t-1,3-Dichloropropene	10.212	75	9854	2.22	ug/l #	42
56) Ethyl methacrylate	10.334	69	1394	0.34	ug/l #	74
59) 2-Hexanone	10.736	43	5864	2.34	ug/l #	56
67) Ethyl Benzene	11.486	91	17936	1.20	ug/l	99
68) m/p-Xylenes	11.588	106	34118	6.06	ug/l	97
69) o-Xylene	11.920	106	17368	3.18	ug/l	93
71) Bromoform	12.376	173	1084	0.39	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.505	83	8072	2.03	ug/l #	24
76) 1,2,3-Trichloropropane	12.376	75	102910	26.05	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.707	105	2620	0.21	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.376	75	102910	65.69	ug/l #	17
84) 1,2,4-Trimethylbenzene	13.013	105	9485	0.77	ug/l	93
95) Naphthalene	15.100	128	6997	4.02	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122220\
Data File : VN065216.D
Acq On : 22 Dec 2020 23:28
Operator : JC/MD
Sample : L5159-22 50X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CGP-11

Quant Time: Dec 23 03:46:42 2020
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 22 15:42:18 2020
Response via : Initial Calibration




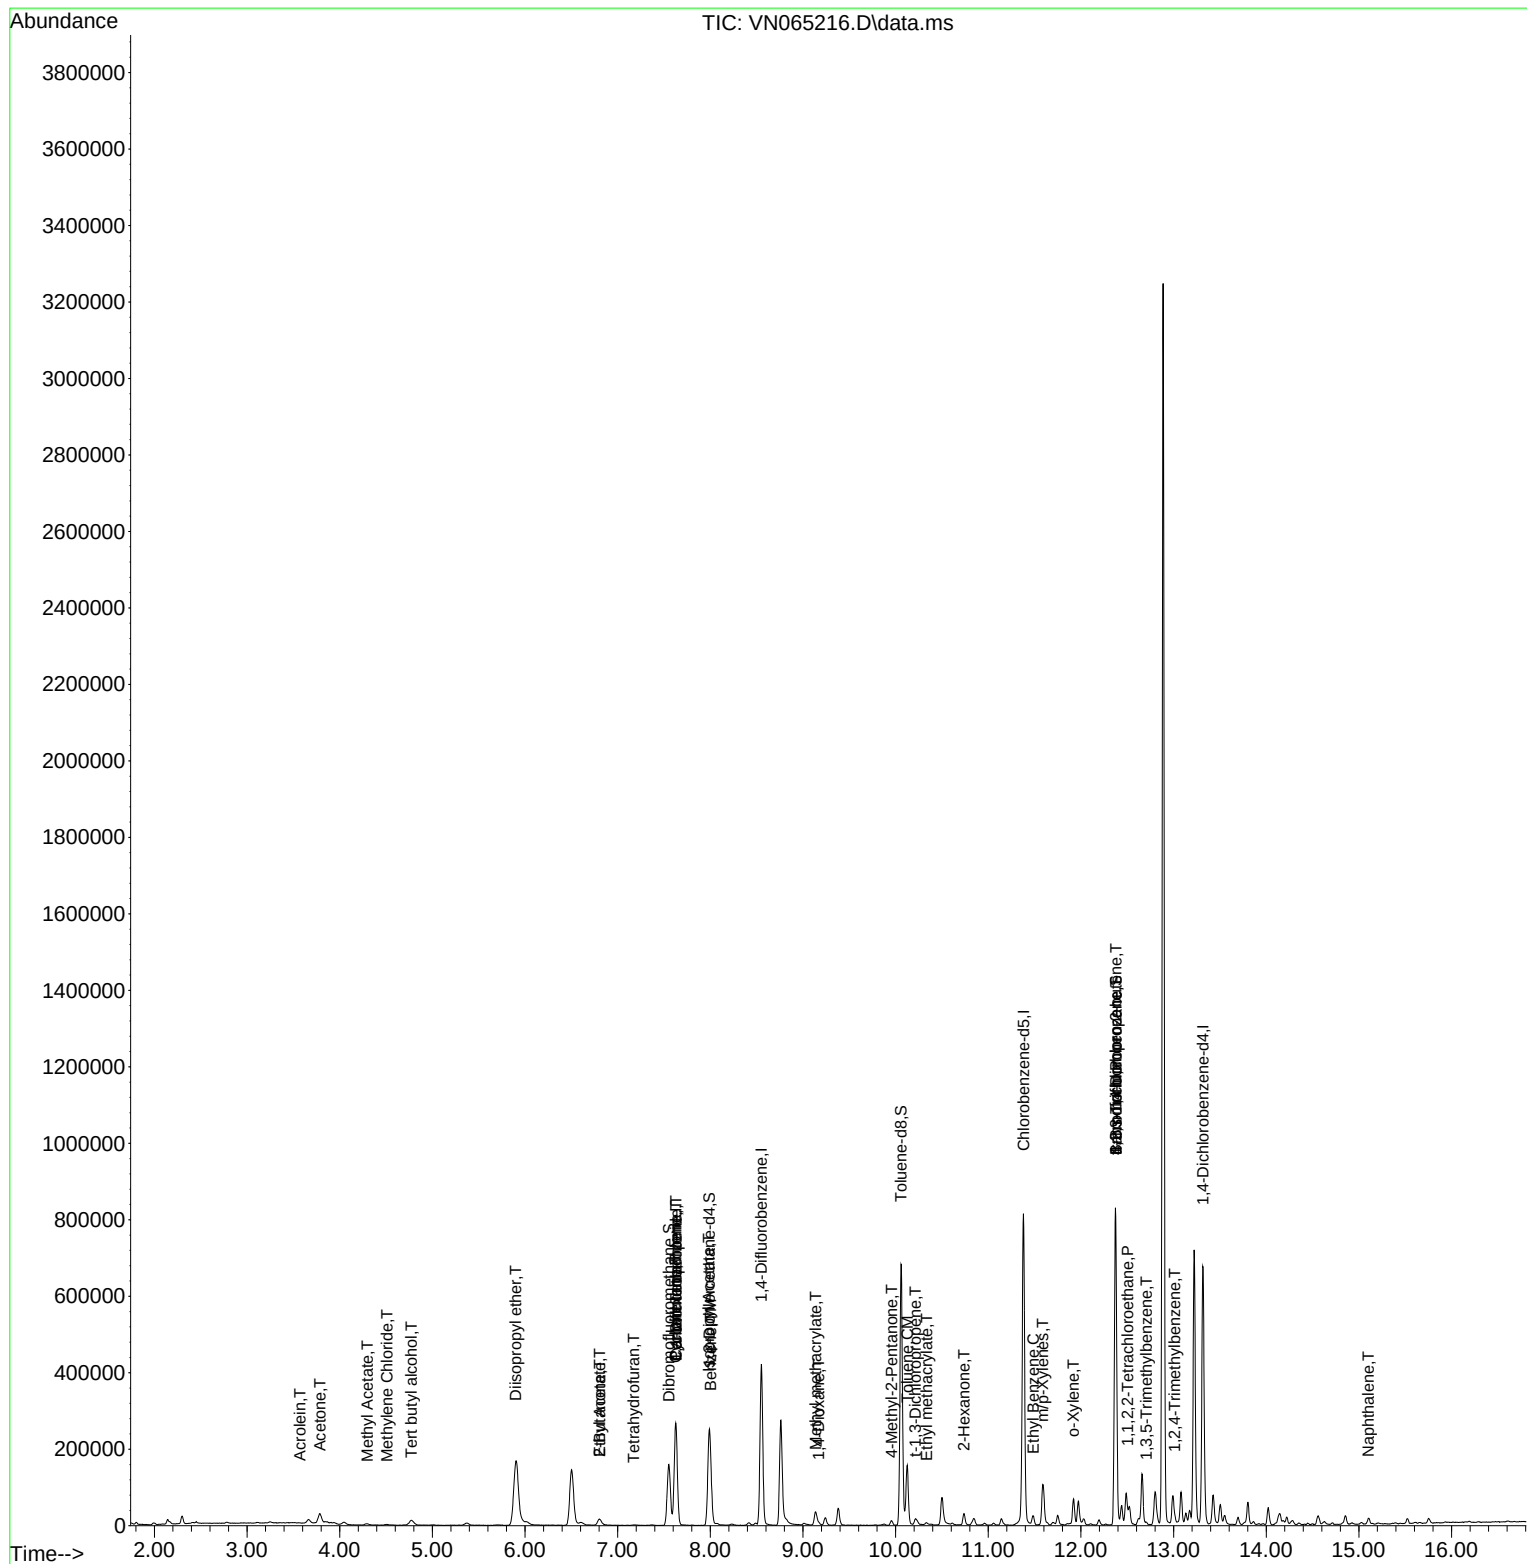


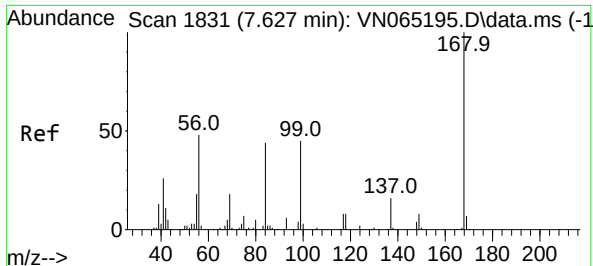

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion:168 Resp: 235675
Ion Ratio Lower Upper
168 100
99 52.2 43.0 64.4

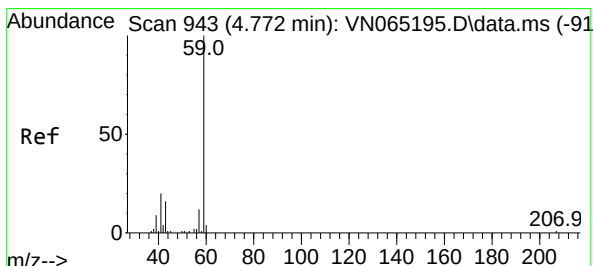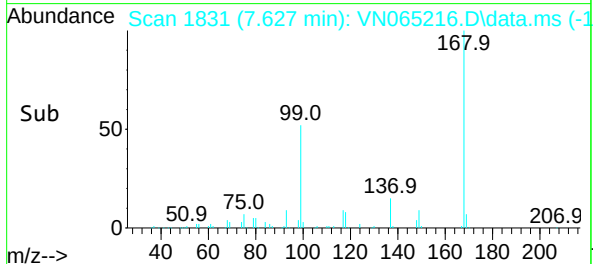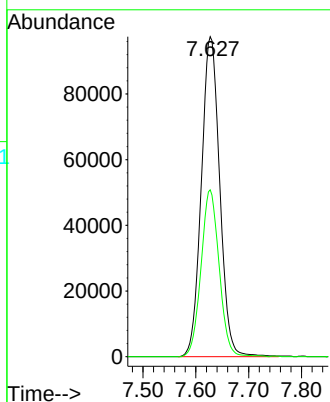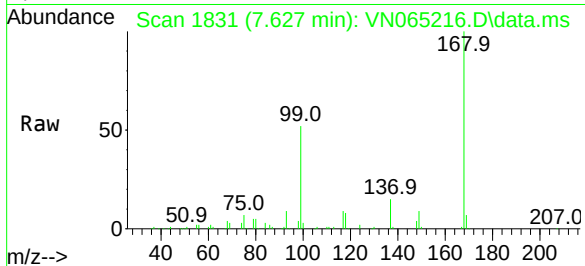

#11
Tert butyl alcohol
Concen: 43.61 ug/l
RT: 4.772 min Scan# 943
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 59 Resp: 18985
Ion Ratio Lower Upper
59 100
57 12.5 7.9 11.9#


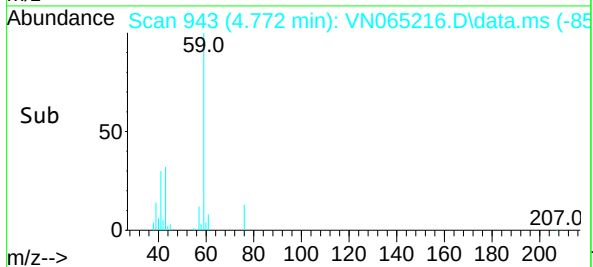
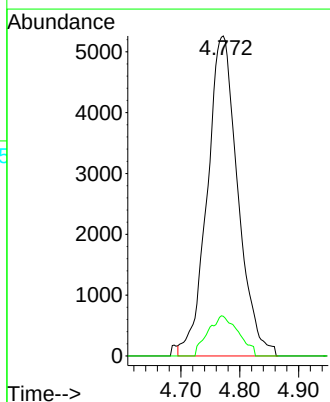
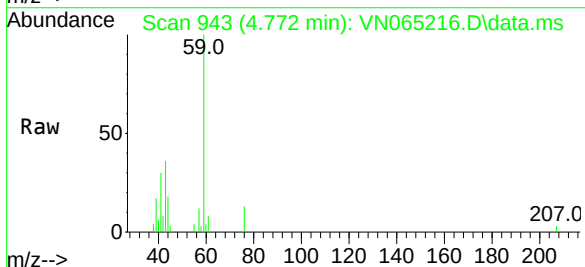


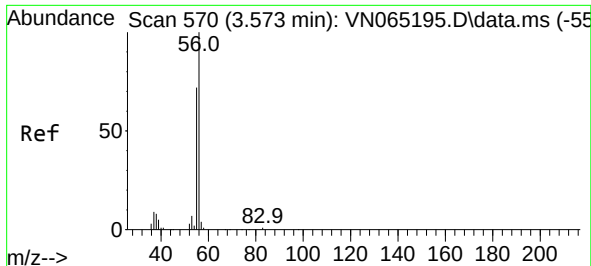

#13
Acrolein
Concen: 2.99 ug/l
RT: 3.569 min Scan# 569
Delta R.T. -0.004 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 56 Resp: 171
Ion Ratio Lower Upper
56 100
55 29.2 56.5 84.7#

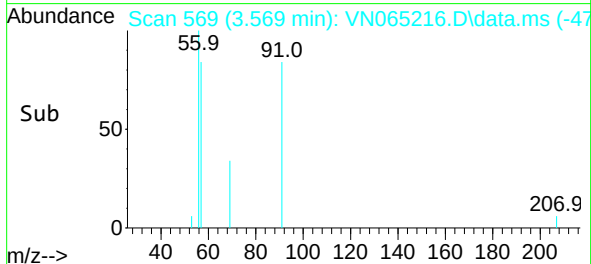

#16
Acetone
Concen: 26.19 ug/l
RT: 3.785 min Scan# 636
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28


Tgt Ion: 43 Resp: 39990
Ion Ratio Lower Upper
43 100
58 30.6 25.7 38.5

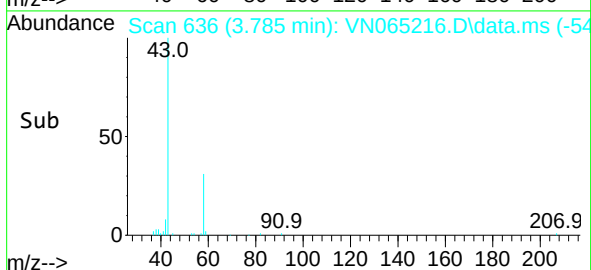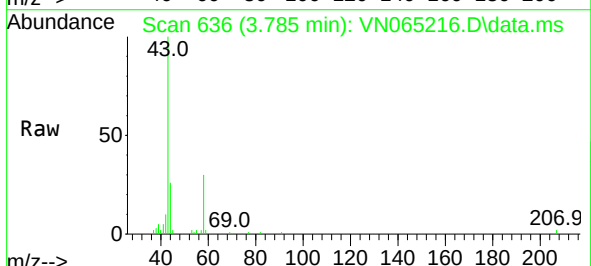



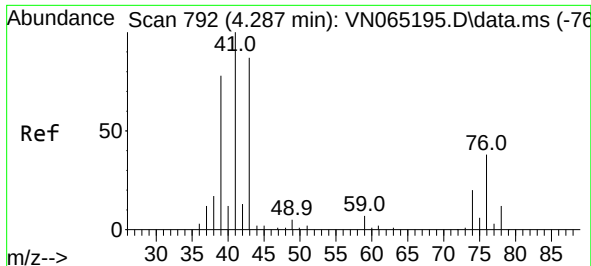


#18
Methyl Acetate
Concen: 2.73 ug/l
RT: 4.296 min Scan# 795
Delta R.T. 0.009 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Instrument :
MSVOA_N
ClientSampled :
CGP-11







Tgt Ion: 43 Resp: 6530
Ion Ratio Lower Upper
43 100
74 16.7 20.2 30.2#

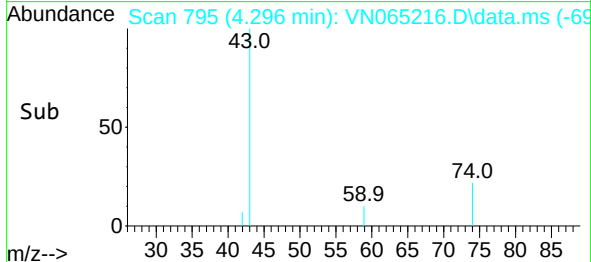

#20
Methylene Chloride
Concen: 0.48 ug/l
RT: 4.511 min Scan# 862
Delta R.T. 0.010 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28


Tgt Ion: 84 Resp: 1238
Ion Ratio Lower Upper
84 100
49 111.1 93.4 140.0
51 50.4 28.2 42.4#
86 58.2 51.7 77.5

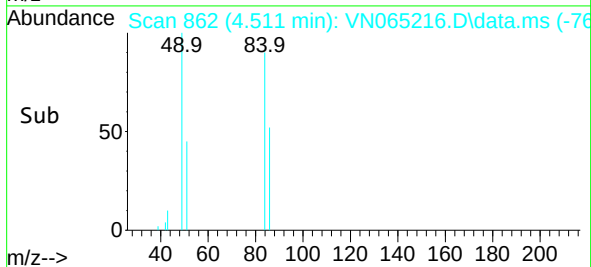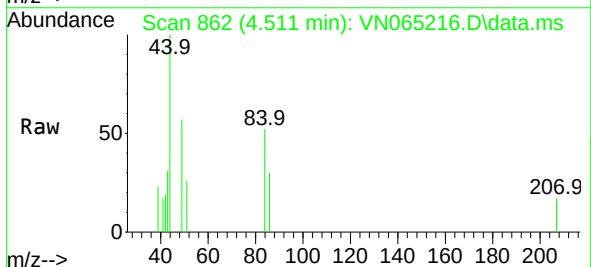



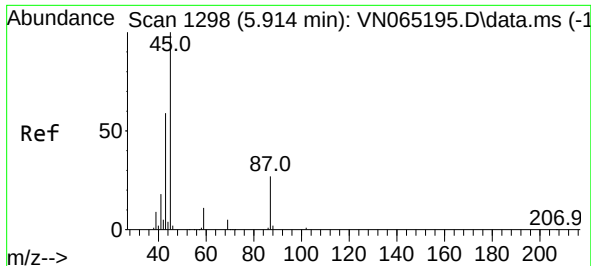


#22
Diisopropyl ether
Concen: 1.16 ug/l
RT: 5.897 min Scan# 1293
Delta R.T. -0.017 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Instrument :
MSVOA_N
ClientSampled :
CGP-11







Tgt Ion: 45 Resp: 8788
Ion Ratio Lower Upper
45 100
43 5.2 46.2 69.2#
87 0.0 24.1 36.1#
59 186.7 9.0 13.4#

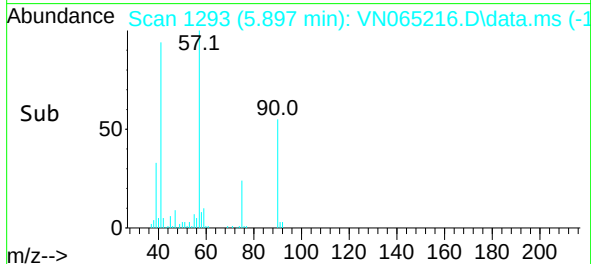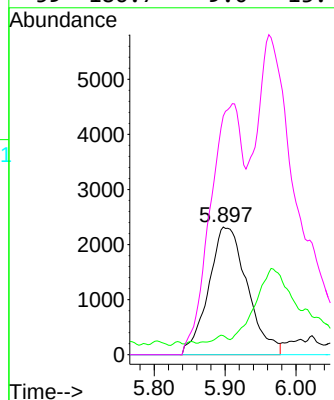

#25
2-Butanone
Concen: 12.42 ug/l
RT: 6.804 min Scan# 1575
Delta R.T. 0.006 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 43 Resp: 18557
Ion Ratio Lower Upper
43 100
72 26.2 21.0 31.6

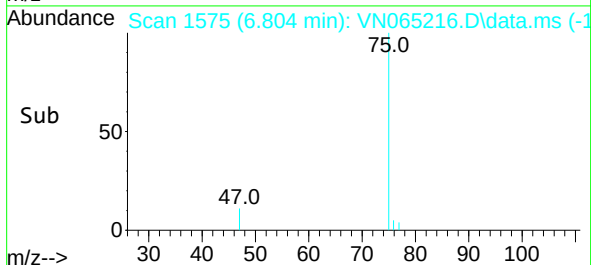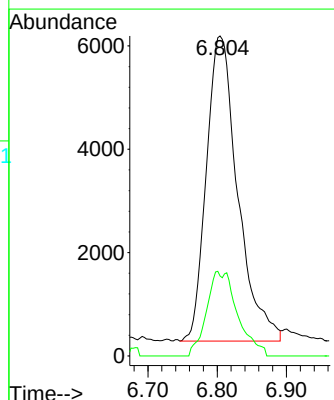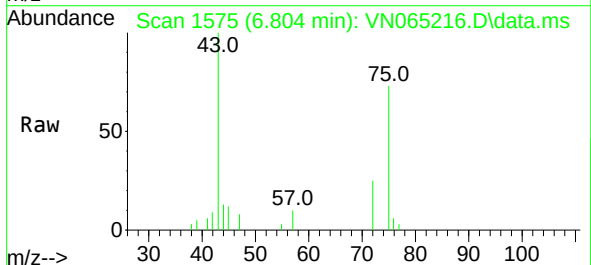

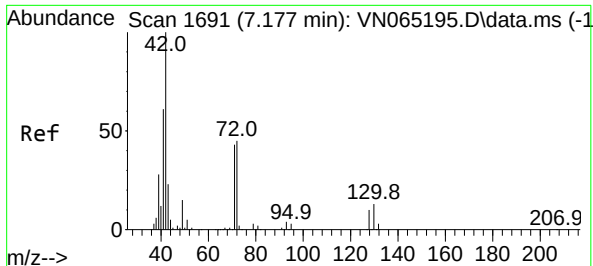

#29

Tetrahydrofuran

Concen: 0.58 ug/l

RT: 7.174 min Scan# 1690





Delta R.T. -0.003 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28

Instrument :
MSVOA_N
ClientSampled :
CGP-11

Tgt Ion: 42	Resp: 562
Ion Ratio	Lower Upper
42	100
72	0.0 36.6 54.8#
71	0.0 33.6 50.4#

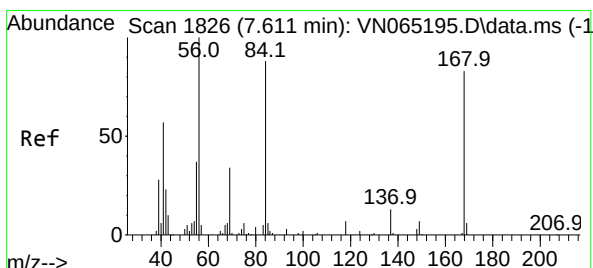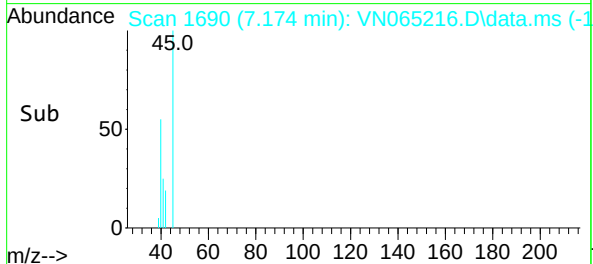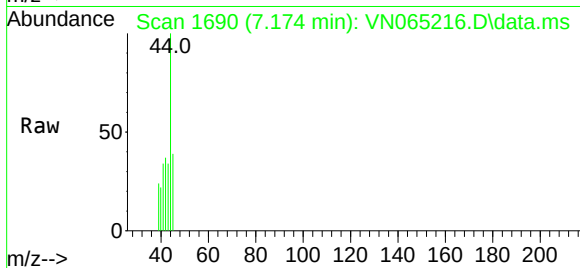

#31

Cyclohexane

Concen: 1.35 ug/l




RT: 7.624 min Scan# 1830


Delta R.T. 0.013 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28

Tgt Ion: 56	Resp: 5316
Ion Ratio	Lower Upper
56	100
69	151.4 27.5 41.3#
84	125.4 73.9 110.9#


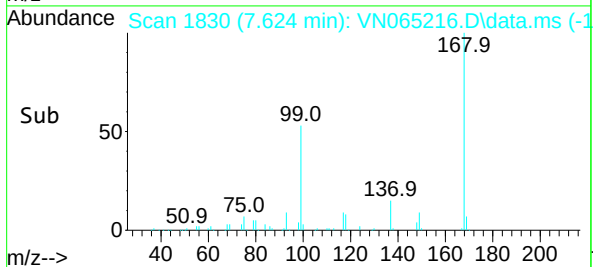

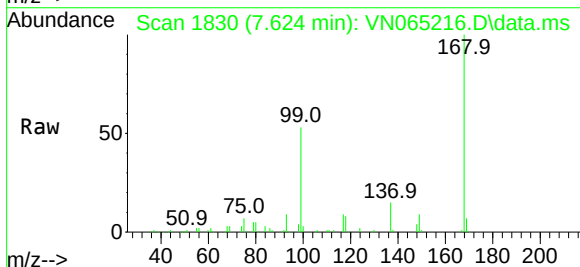


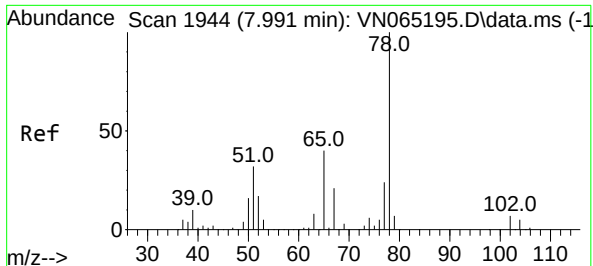

#33
1,2-Dichloroethane-d4
Concen: 52.63 ug/l
RT: 7.990 min Scan# 1944
Delta R.T. -0.001 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 65 Resp: 140015
Ion Ratio Lower Upper
65 100
67 51.8 0.0 108.2

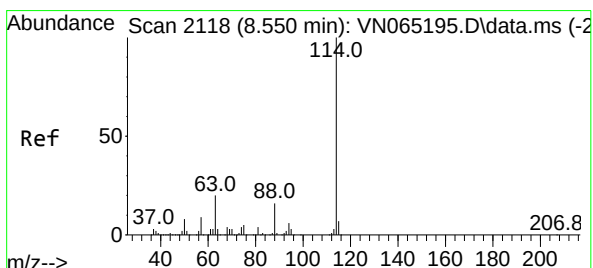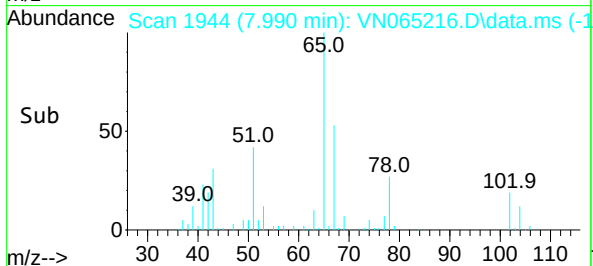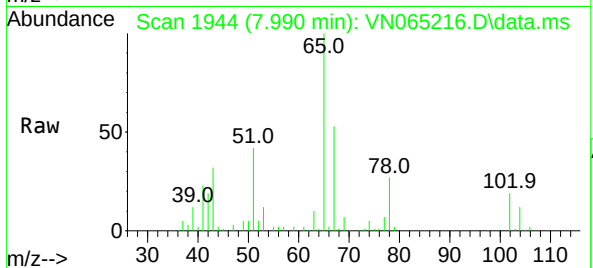

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 114 Resp: 390389
Ion Ratio Lower Upper
114 100
63 19.8 0.0 38.6
88 15.2 0.0 32.6

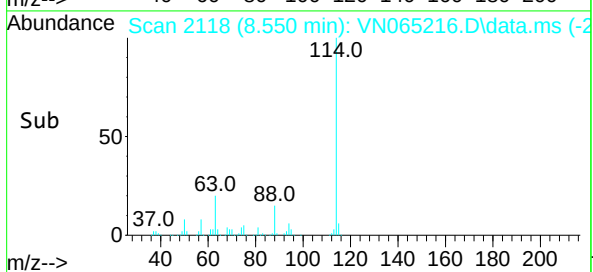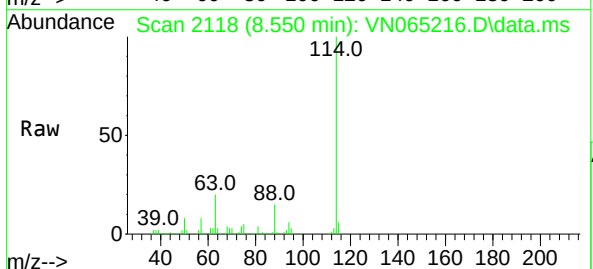

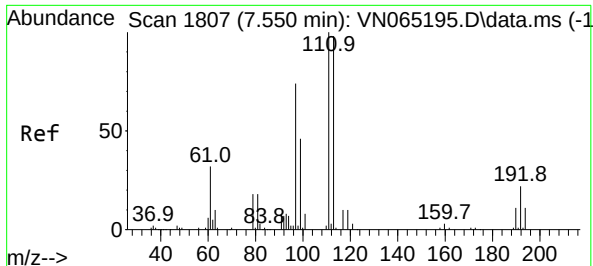

#35

Dibromofluoromethane

Concen: 51.63 ug/l

RT: 7.553 min Scan# 1808

Delta R.T. 0.003 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28





Tgt Ion:113 Resp: 121608

Ion Ratio Lower Upper

113 100

111 102.7 81.6 122.4

192 22.9 16.2 24.2

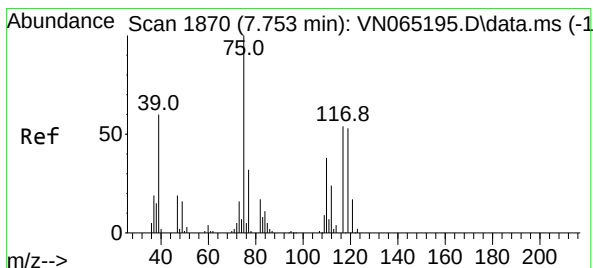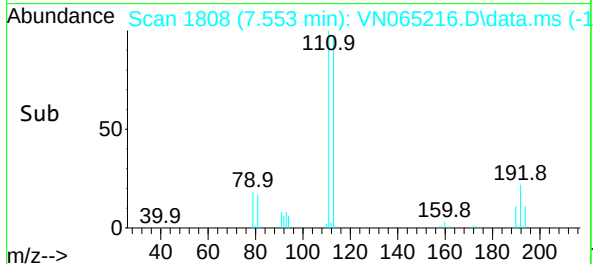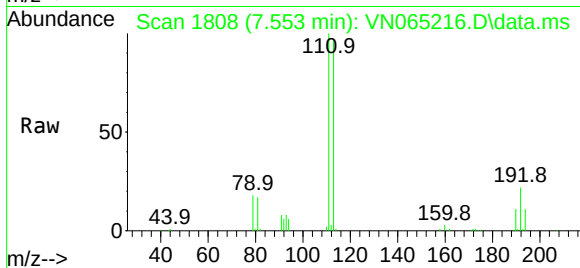

#36

1,1-Dichloropropene

Concen: 4.42 ug/l

RT: 7.627 min Scan# 1831

Delta R.T. -0.126 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28




Tgt Ion: 75 Resp: 15688


Ion Ratio Lower Upper

75 100

110 8.5 17.8 53.3#

77 0.0 25.0 37.4#

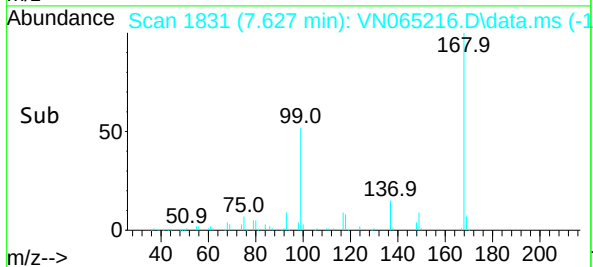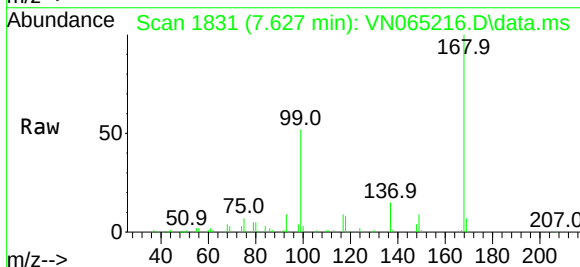

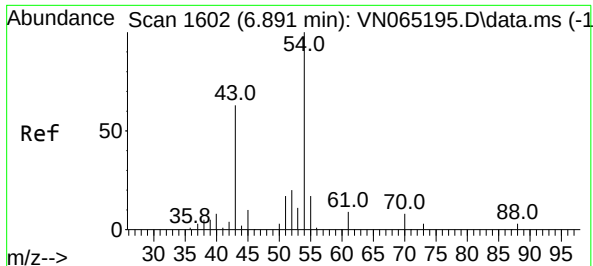

#37

Ethyl Acetate

Concen: 5.27 ug/l

RT: 6.804 min Scan# 1575

Delta R.T. -0.087 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28





Instrument :

MSVOA_N

ClientSampleId :

CGP-11

Tgt Ion: 43	Resp: 18557
Ion Ratio	Lower Upper
43 100	
61 0.4	12.8 19.2#
70 0.0	8.8 13.2#

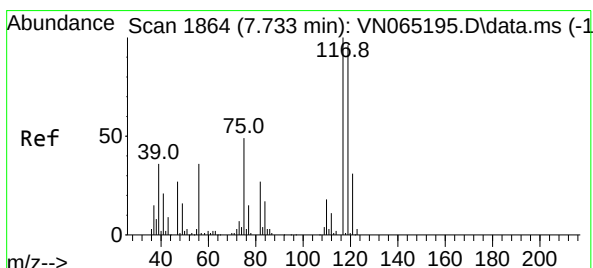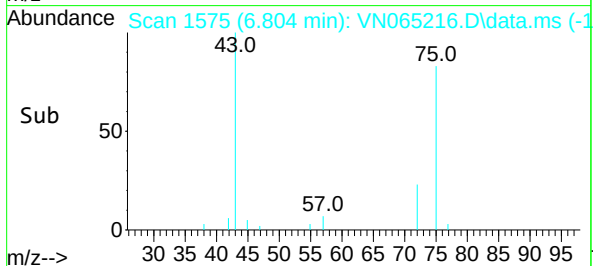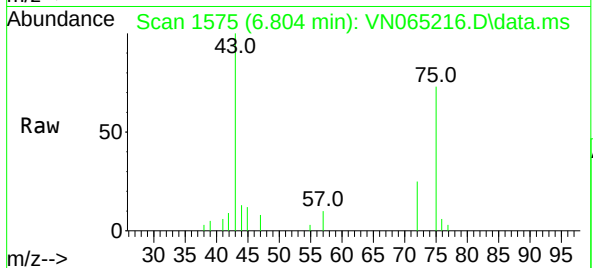

#38

Carbon Tetrachloride

Concen: 5.37 ug/l




RT: 7.627 min Scan# 1831


Delta R.T. -0.106 min

Lab File: VN065216.D

Acq: 22 Dec 2020 23:28

Tgt Ion: 117	Resp: 20020
Ion Ratio	Lower Upper
117 100	
119 5.3	76.7 115.1#
121 0.0	25.4 38.2#


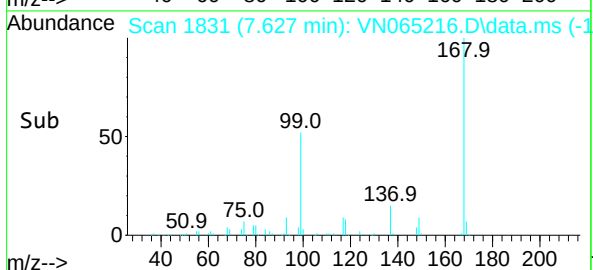

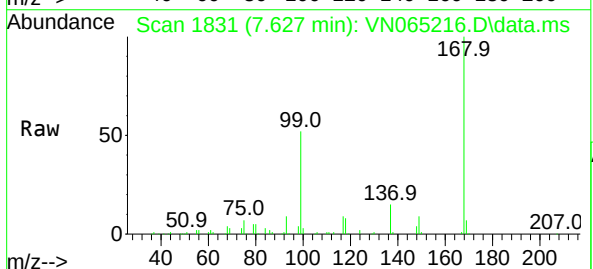


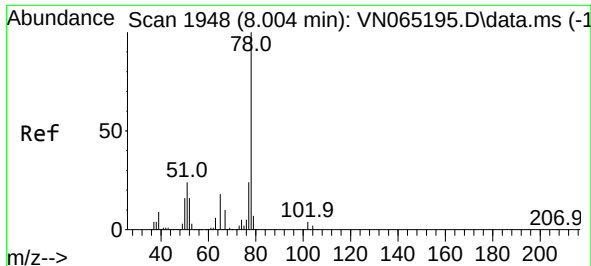

#40
Benzene
Concen: 5.14 ug/l
RT: 8.003 min Scan# 1948
Delta R.T. -0.001 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 78 Resp: 54325
Ion Ratio Lower Upper
78 100
77 24.2 17.9 26.9

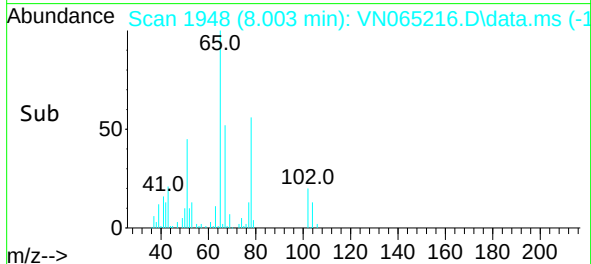

#43
Isopropyl Acetate
Concen: 8.02 ug/l
RT: 7.984 min Scan# 1942
Delta R.T. -0.148 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 43 Resp: 48652
Ion Ratio Lower Upper
43 100
61 6.7 17.2 25.8#
87 0.0 11.4 17.0#


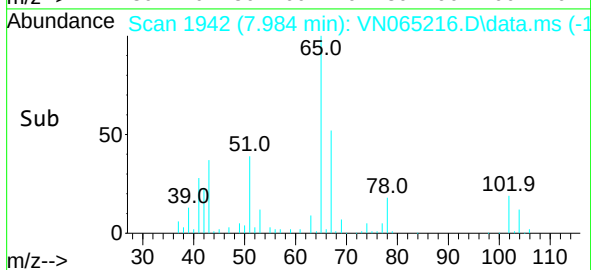

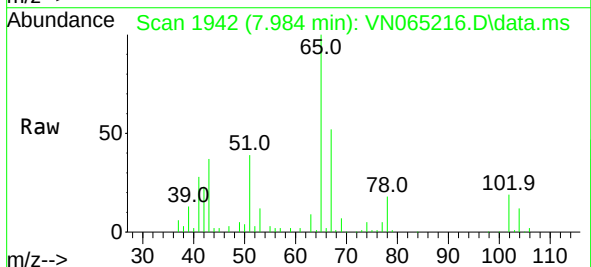




#48
Methyl methacrylate
Concen: 3.33 ug/l
RT: 9.135 min Scan# 2300
Delta R.T. -0.032 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 41 Resp: 9817
Ion Ratio Lower Upper
41 100
69 0.0 71.8 107.8#
39 53.3 44.1 66.1

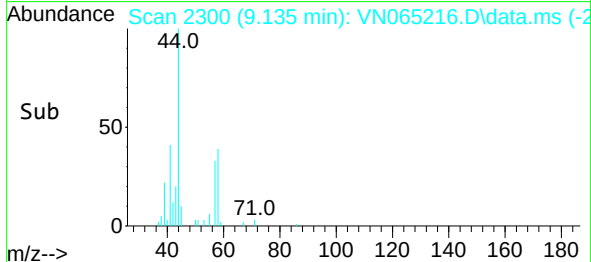

#49
1,4-Dioxane
Concen: 41.50 ug/l
RT: 9.170 min Scan# 2311
Delta R.T. -0.001 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 88 Resp: 1980
Ion Ratio Lower Upper
88 100
43 0.0 24.2 36.4#
58 0.0 52.5 78.7#


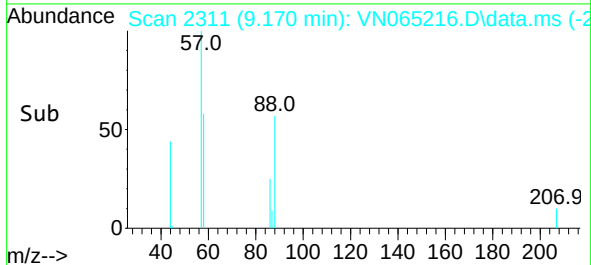

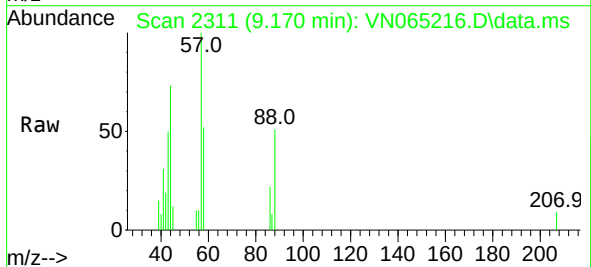


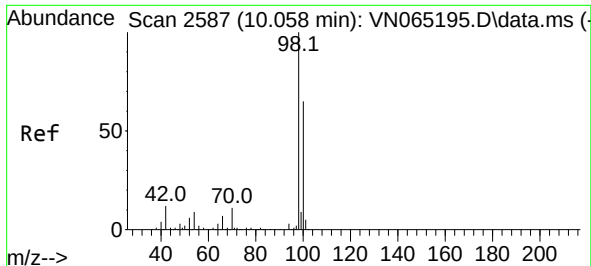

#50
Toluene-d8
Concen: 54.82 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 98 Resp: 483903
Ion Ratio Lower Upper
98 100
100 63.7 51.7 77.5

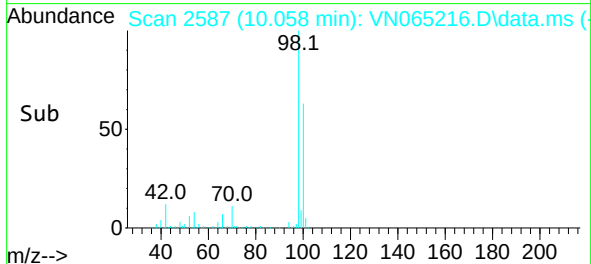

#51
4-Methyl-2-Pentanone
Concen: 2.43 ug/l
RT: 9.955 min Scan# 2555
Delta R.T. 0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 43 Resp: 8283
Ion Ratio Lower Upper
43 100
58 40.6 32.4 48.6

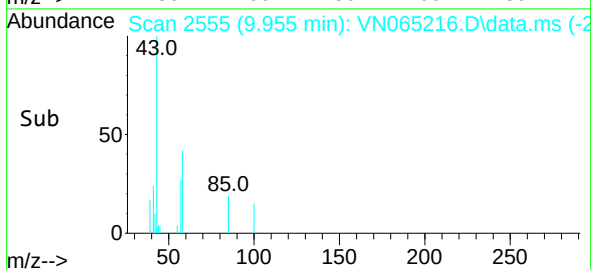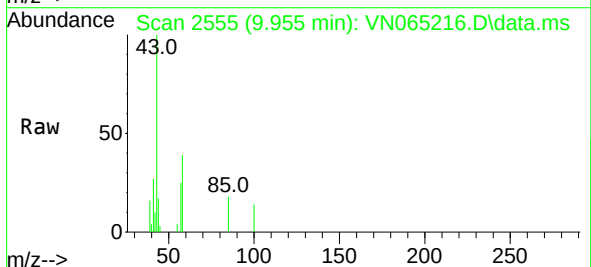

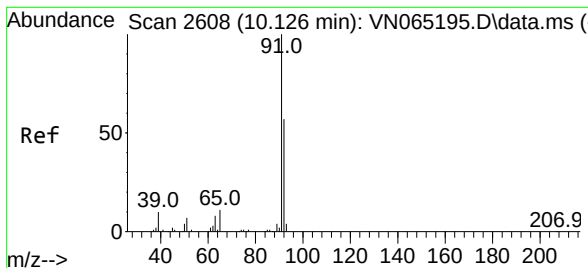

#52

Toluene

Concen: 9.93 ug/l

RT: 10.125 min Scan# 2608

Delta R.T. -0.001 min

Lab File: VN065216.D





Acq: 22 Dec 2020 23:28

Tgt Ion: 92 Resp: 66074

Ion Ratio Lower Upper

92 100

91 176.0 139.1 208.7

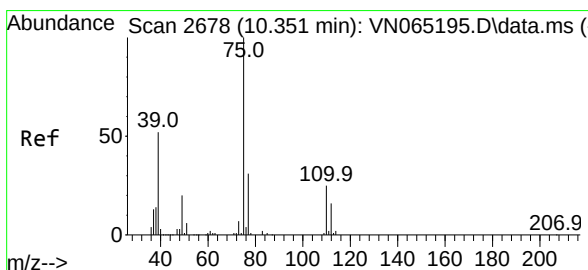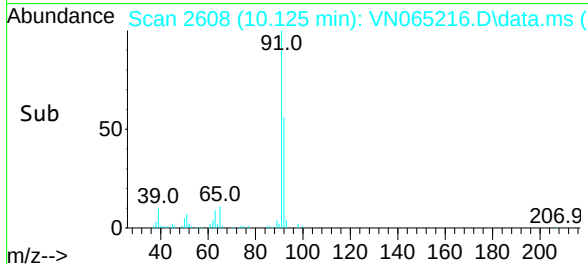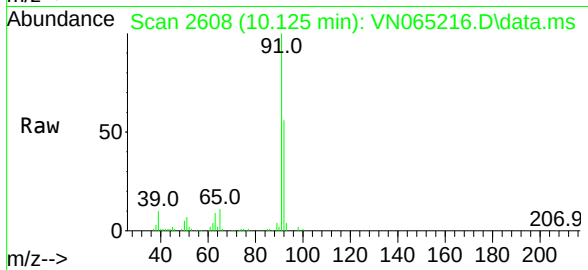

#53

t-1,3-Dichloropropene

Concen: 2.22 ug/l

RT: 10.212 min Scan# 2635

Delta R.T. -0.139 min

Lab File: VN065216.D




Acq: 22 Dec 2020 23:28


Tgt Ion: 75 Resp: 9854

Ion Ratio Lower Upper

75 100

77 0.0 25.8 38.6#


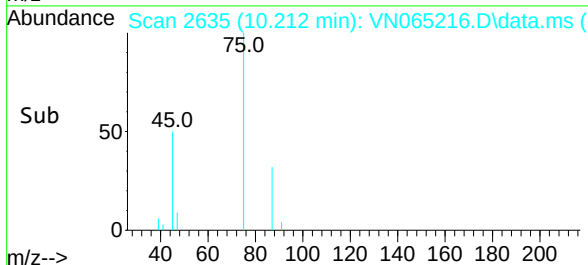

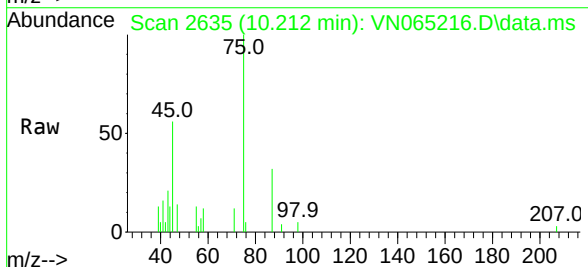


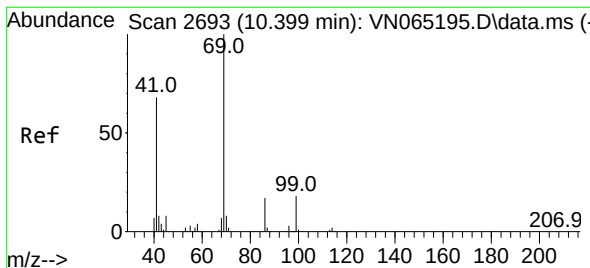

#56
Ethyl methacrylate
Concen: 0.34 ug/l
RT: 10.334 min Scan# 2673
Delta R.T. -0.065 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 69 Resp: 1394
Ion Ratio Lower Upper
69 100
41 86.8 49.4 74.0#
39 40.6 25.9 38.9#

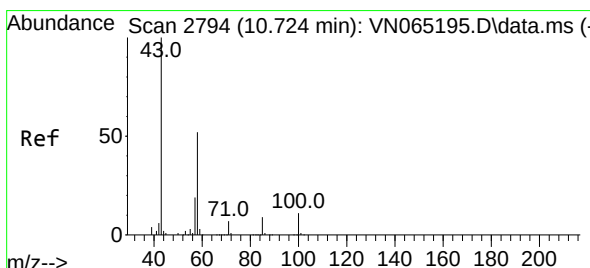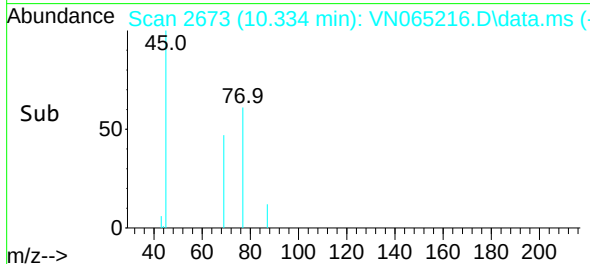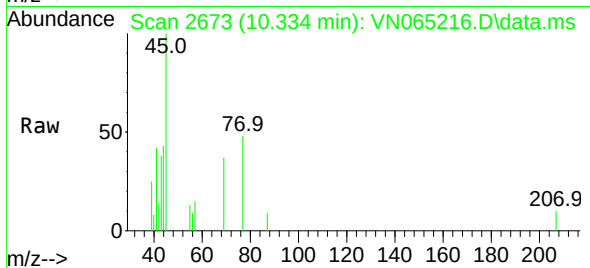

#59
2-Hexanone
Concen: 2.34 ug/l
RT: 10.736 min Scan# 2798
Delta R.T. 0.012 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 43 Resp: 5864
Ion Ratio Lower Upper
43 100
58 24.2 28.3 84.9#


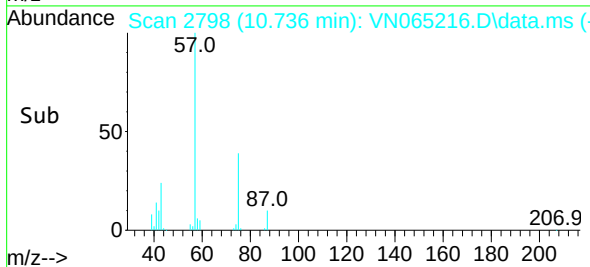

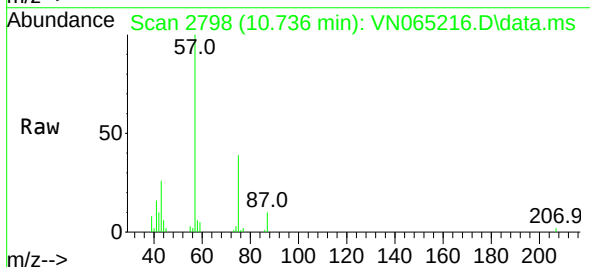


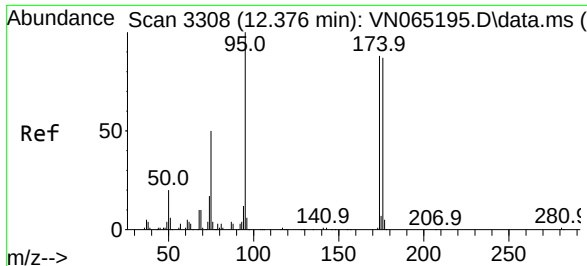

#62
4-Bromofluorobenzene
Concen: 56.66 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampleId :
CGP-11


Tgt Ion: 95 Resp: 200438
Ion Ratio Lower Upper
95 100
174 89.2 0.0 160.4
176 86.8 0.0 158.4

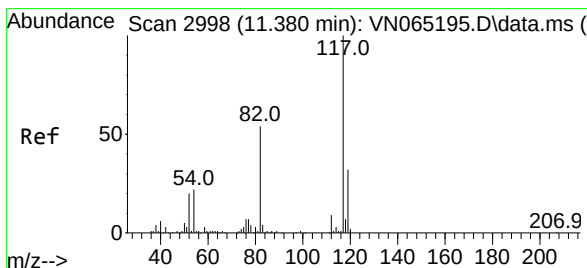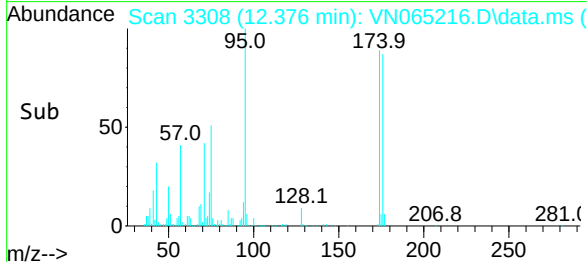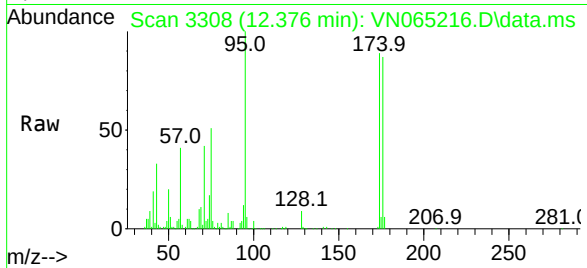

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.379 min Scan# 2998
Delta R.T. -0.001 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 117 Resp: 407155
Ion Ratio Lower Upper
117 100
82 53.5 44.2 66.2
119 31.8 25.8 38.6


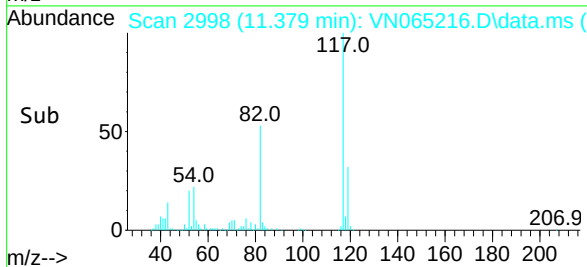

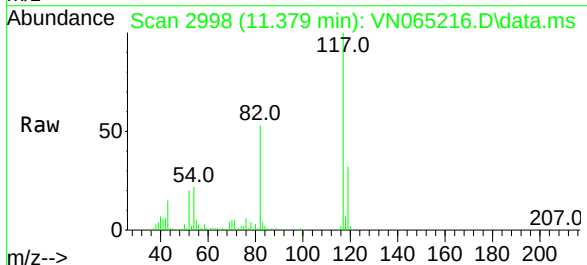




#67
Ethyl Benzene
Concen: 1.20 ug/l
RT: 11.486 min Scan# 3031
Delta R.T. 0.004 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion: 91 Resp: 17936
Ion Ratio Lower Upper
91 100
106 31.9 25.2 37.8

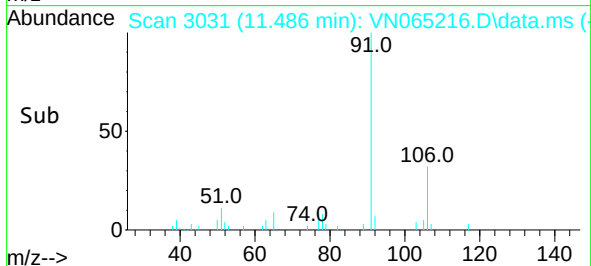

#68
m/p-Xylenes
Concen: 6.06 ug/l
RT: 11.588 min Scan# 3063
Delta R.T. -0.004 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion:106 Resp: 34118
Ion Ratio Lower Upper
106 100
91 205.5 161.0 241.4


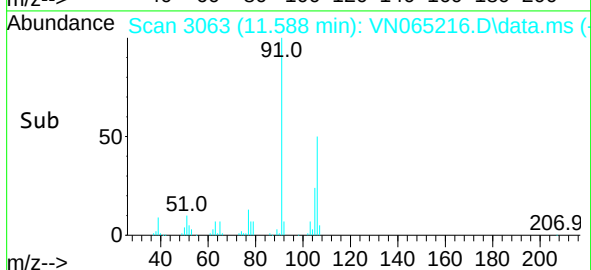

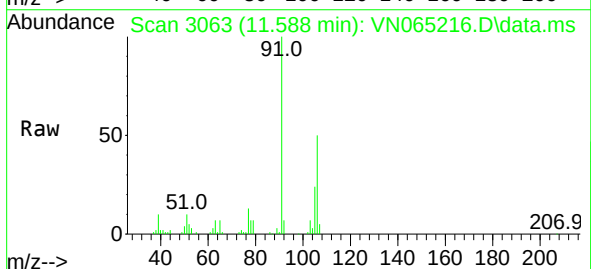


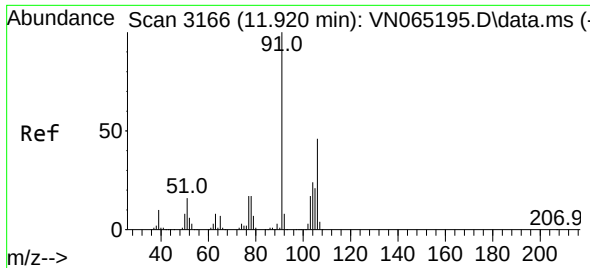

#69
o-Xylene
Concen: 3.18 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampled :
CGP-11


Tgt Ion:106 Resp: 17368
Ion Ratio Lower Upper
106 100
91 221.9 105.5 316.5

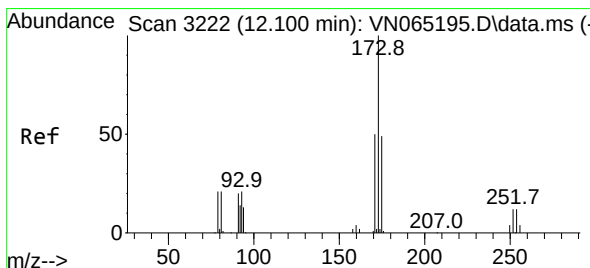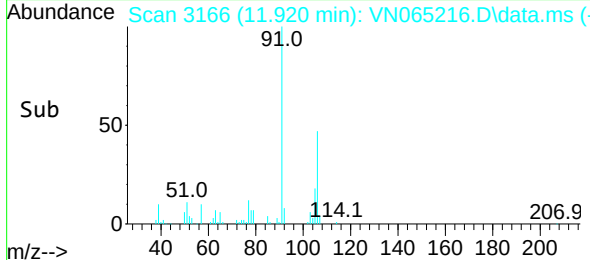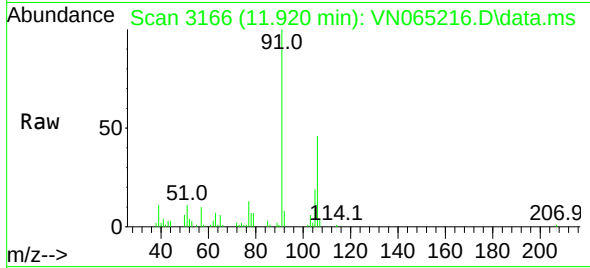

#71
Bromoform
Concen: 0.39 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.276 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion:173 Resp: 1084
Ion Ratio Lower Upper
173 100
175 999.8 24.3 72.8#
254 0.0 0.0 0.0


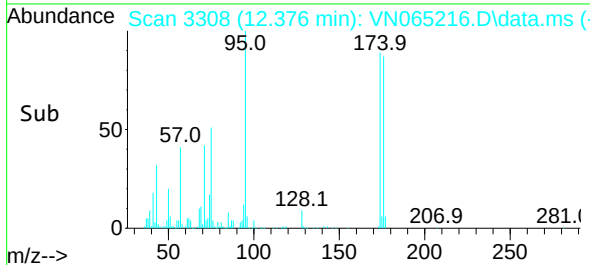

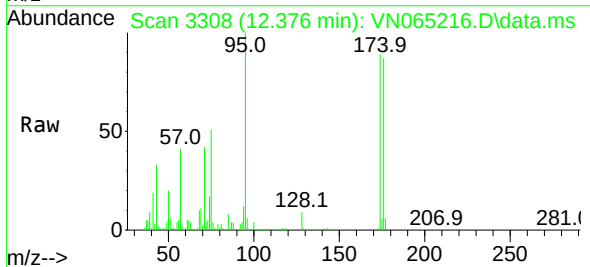




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.318 min Scan# 3601
 Delta R.T. 0.000 min
 Lab File: VN065216.D
 Acq: 22 Dec 2020 23:28




Instrument :
 MSVOA_N
 ClientSampled :
 CGP-11


Tgt Ion:152 Resp: 193619
 Ion Ratio Lower Upper
 152 100
 115 55.4 29.7 89.1
 150 156.6 0.0 350.6

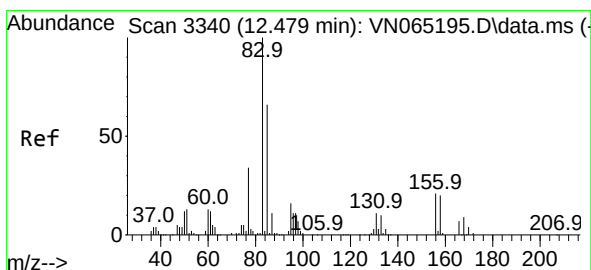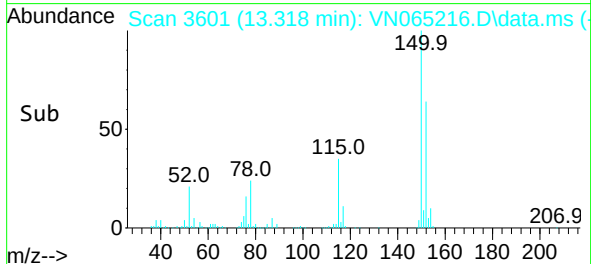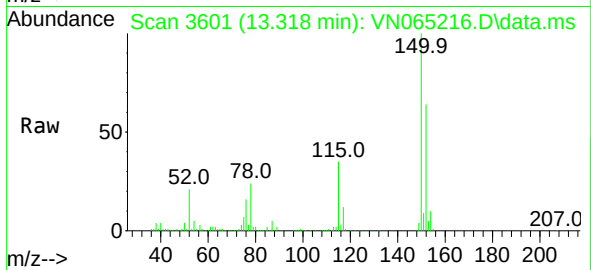

#75
 1,1,2,2-Tetrachloroethane
 Concen: 2.03 ug/l
 RT: 12.505 min Scan# 3348
 Delta R.T. 0.026 min
 Lab File: VN065216.D
 Acq: 22 Dec 2020 23:28

Tgt Ion: 83 Resp: 8072
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.1 15.3#
 85 0.0 33.0 99.0#




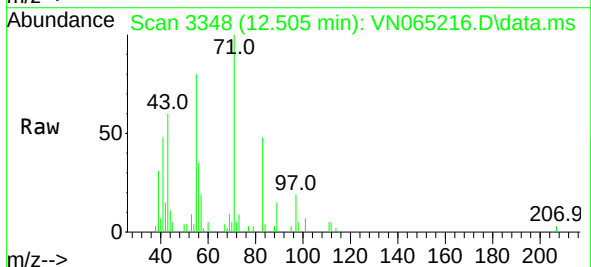


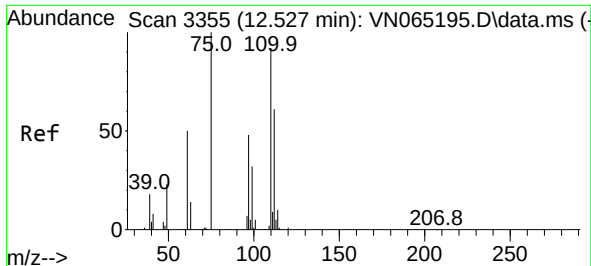

#76
1,2,3-Trichloropropane
Concen: 26.05 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. -0.151 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampleId :
CGP-11


Tgt Ion: 75 Resp: 102910
Ion Ratio Lower Upper
75 100
77 1.5 0.0 0.0#

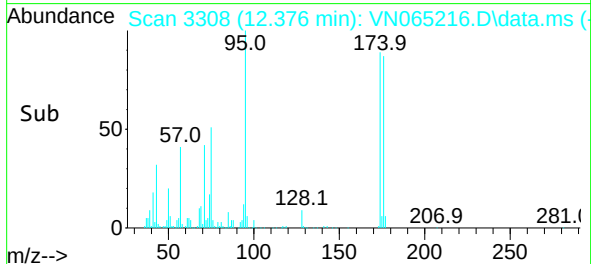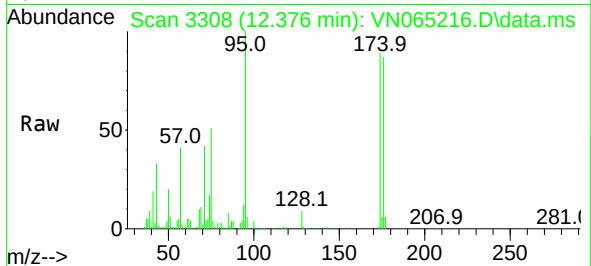

#80
1,3,5-Trimethylbenzene
Concen: 0.21 ug/l
RT: 12.707 min Scan# 3411
Delta R.T. -0.001 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion:105 Resp: 2620
Ion Ratio Lower Upper
105 100
120 49.2 24.6 73.6


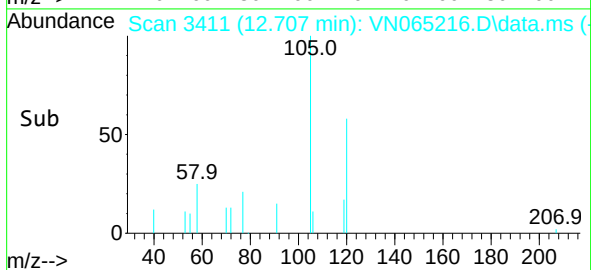

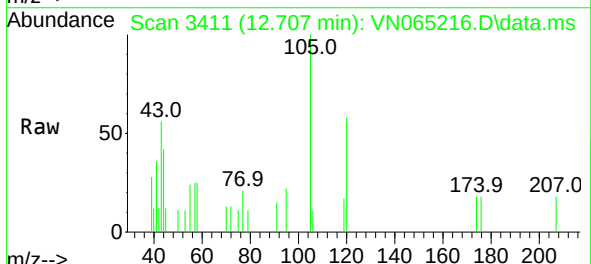




#81
trans-1,4-Dichloro-2-butene
Concen: 65.69 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.103 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28




Instrument :
MSVOA_N
ClientSampleId :
CGP-11


Tgt Ion: 75 Resp: 102910
Ion Ratio Lower Upper
75 100
53 3.0 67.0 100.4#
89 0.0 39.6 59.4#

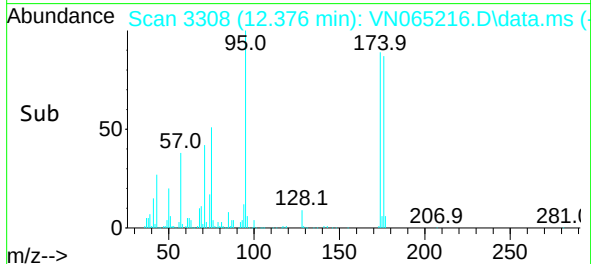

#84
1,2,4-Trimethylbenzene
Concen: 0.77 ug/l
RT: 13.013 min Scan# 3506
Delta R.T. -0.000 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Tgt Ion: 105 Resp: 9485
Ion Ratio Lower Upper
105 100
120 41.6 23.1 69.2

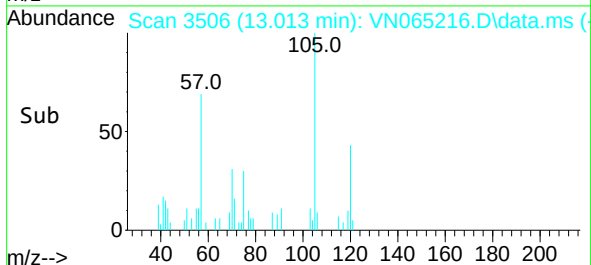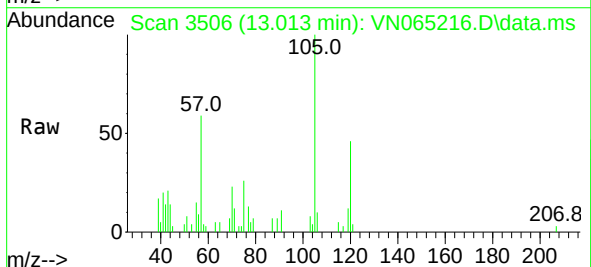

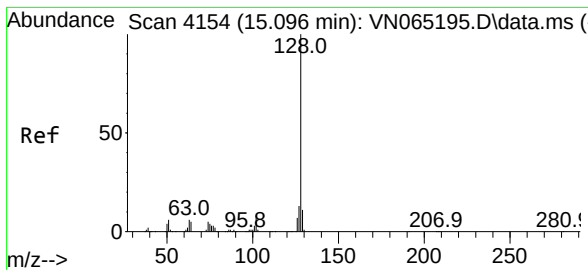

#95
Naphthalene
Concen: 4.02 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. 0.004 min
Lab File: VN065216.D
Acq: 22 Dec 2020 23:28

Instrument :
MSVOA_N
ClientSampleId :
CGP-11

Tgt Ion:128 Resp: 6997
Ion Ratio Lower Upper
128 100
127 10.1 10.3 15.5#
129 9.3 8.7 13.1

