


Acrolein


Response Ratio

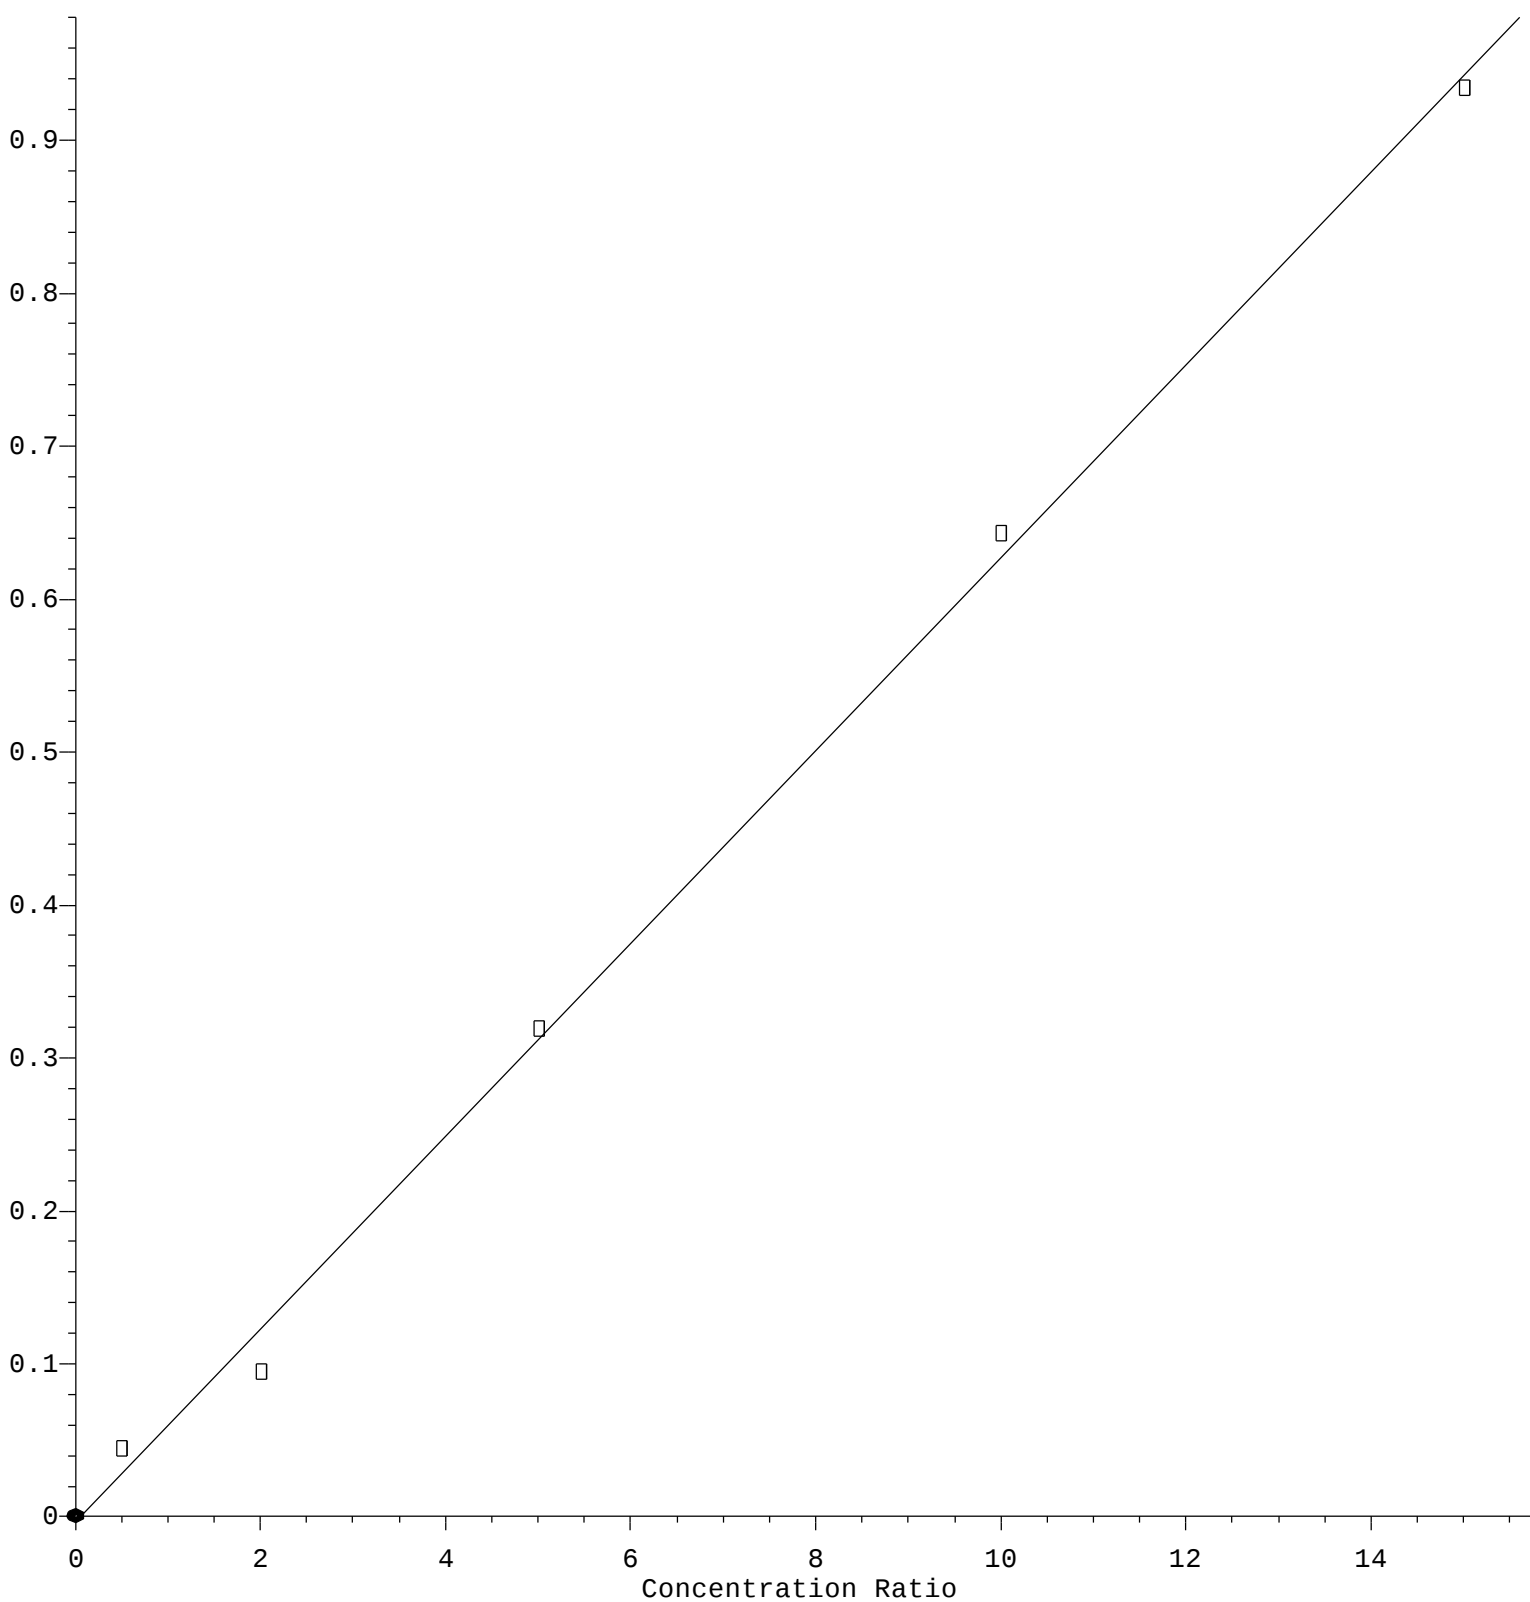

Response = 6.307e-002 * Amt - 3.041e-003
Coef of Det (r^2) = 0.997547 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

Acetone


Response Ratio

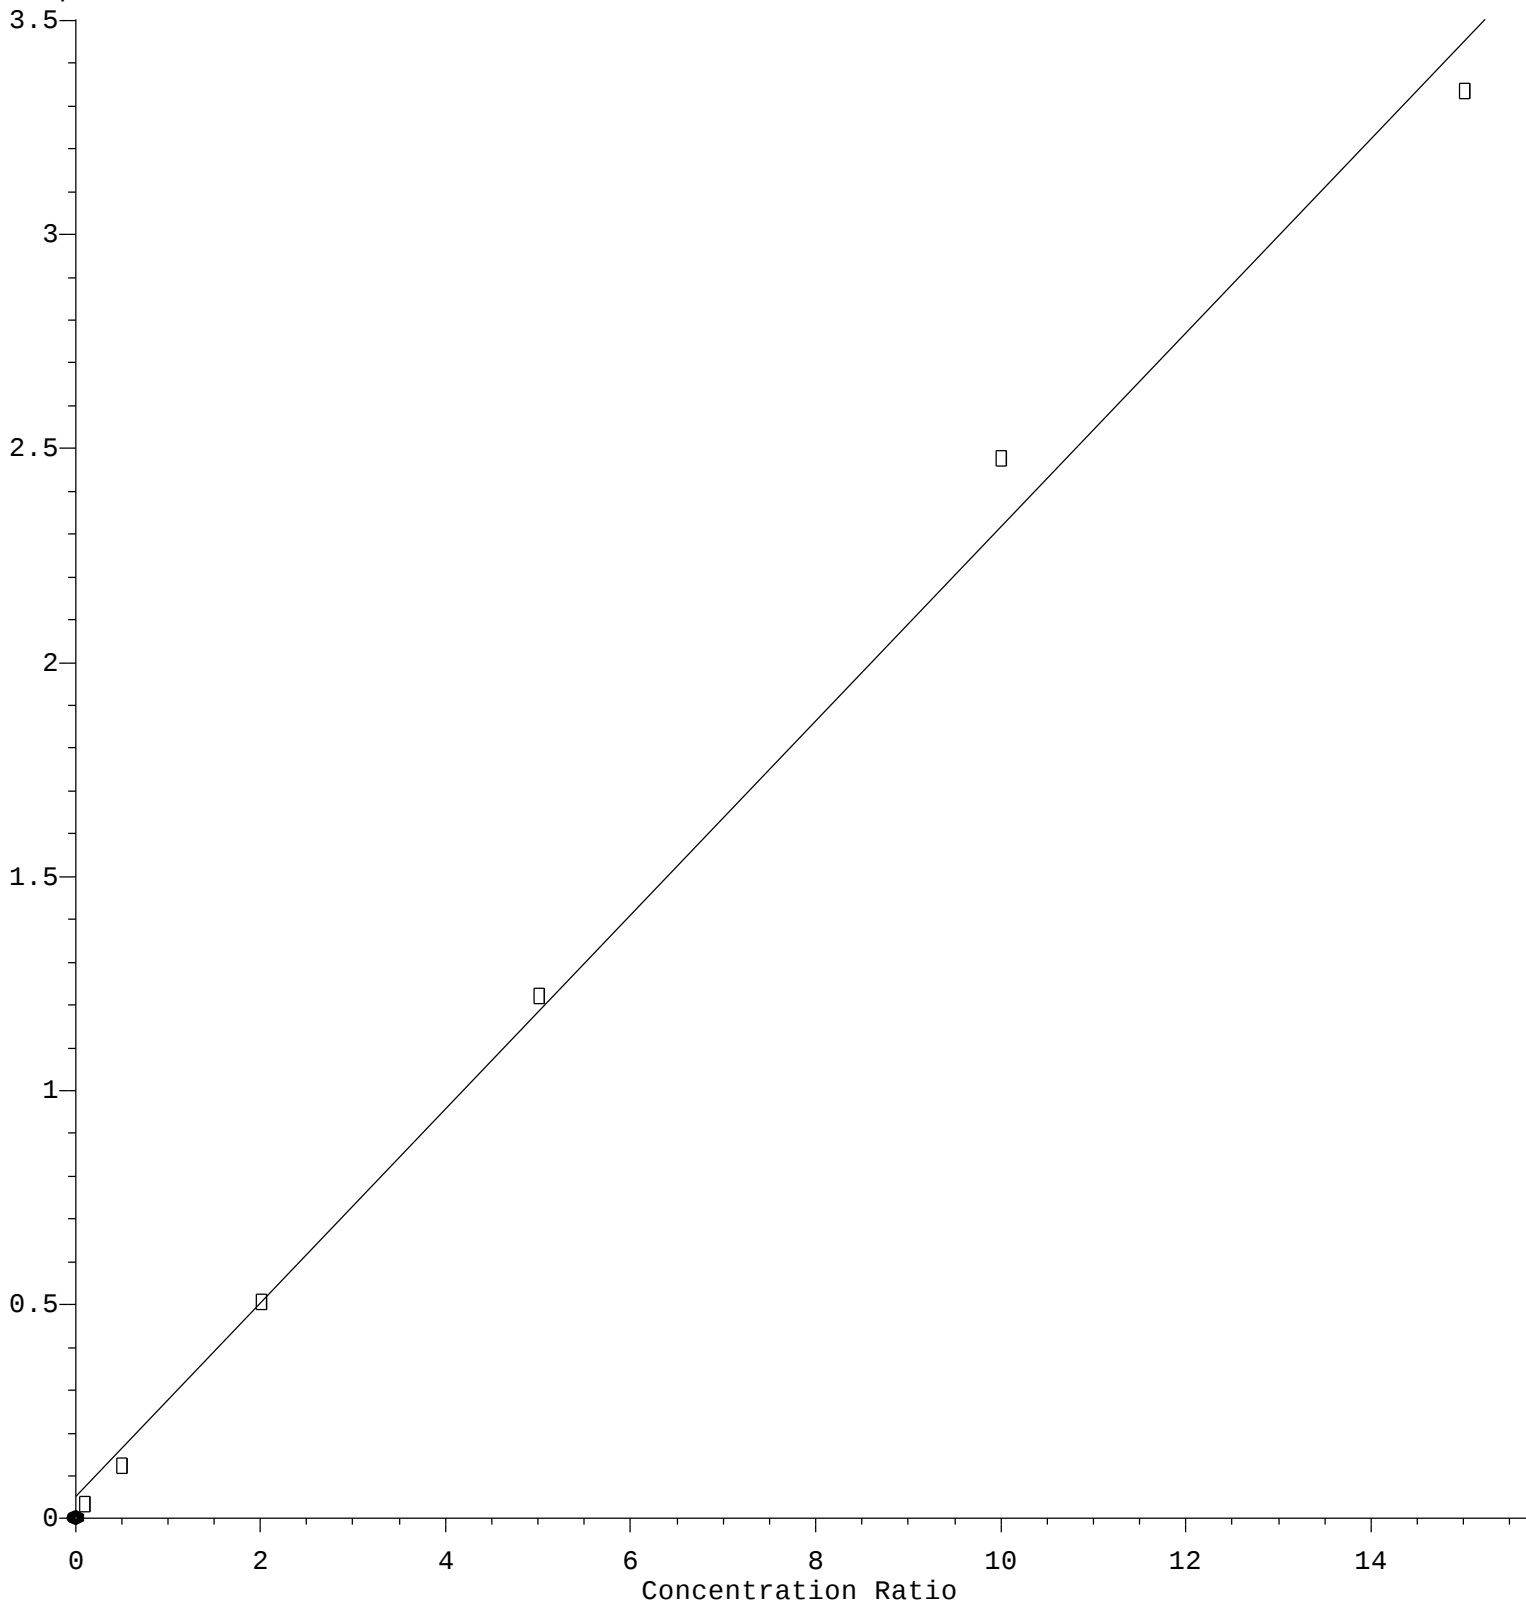

Response = 2.267e-001 * Amt + 5.097e-002
Coef of Det (r^2) = 0.995274 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

Bromochloromethane

Response Ratio

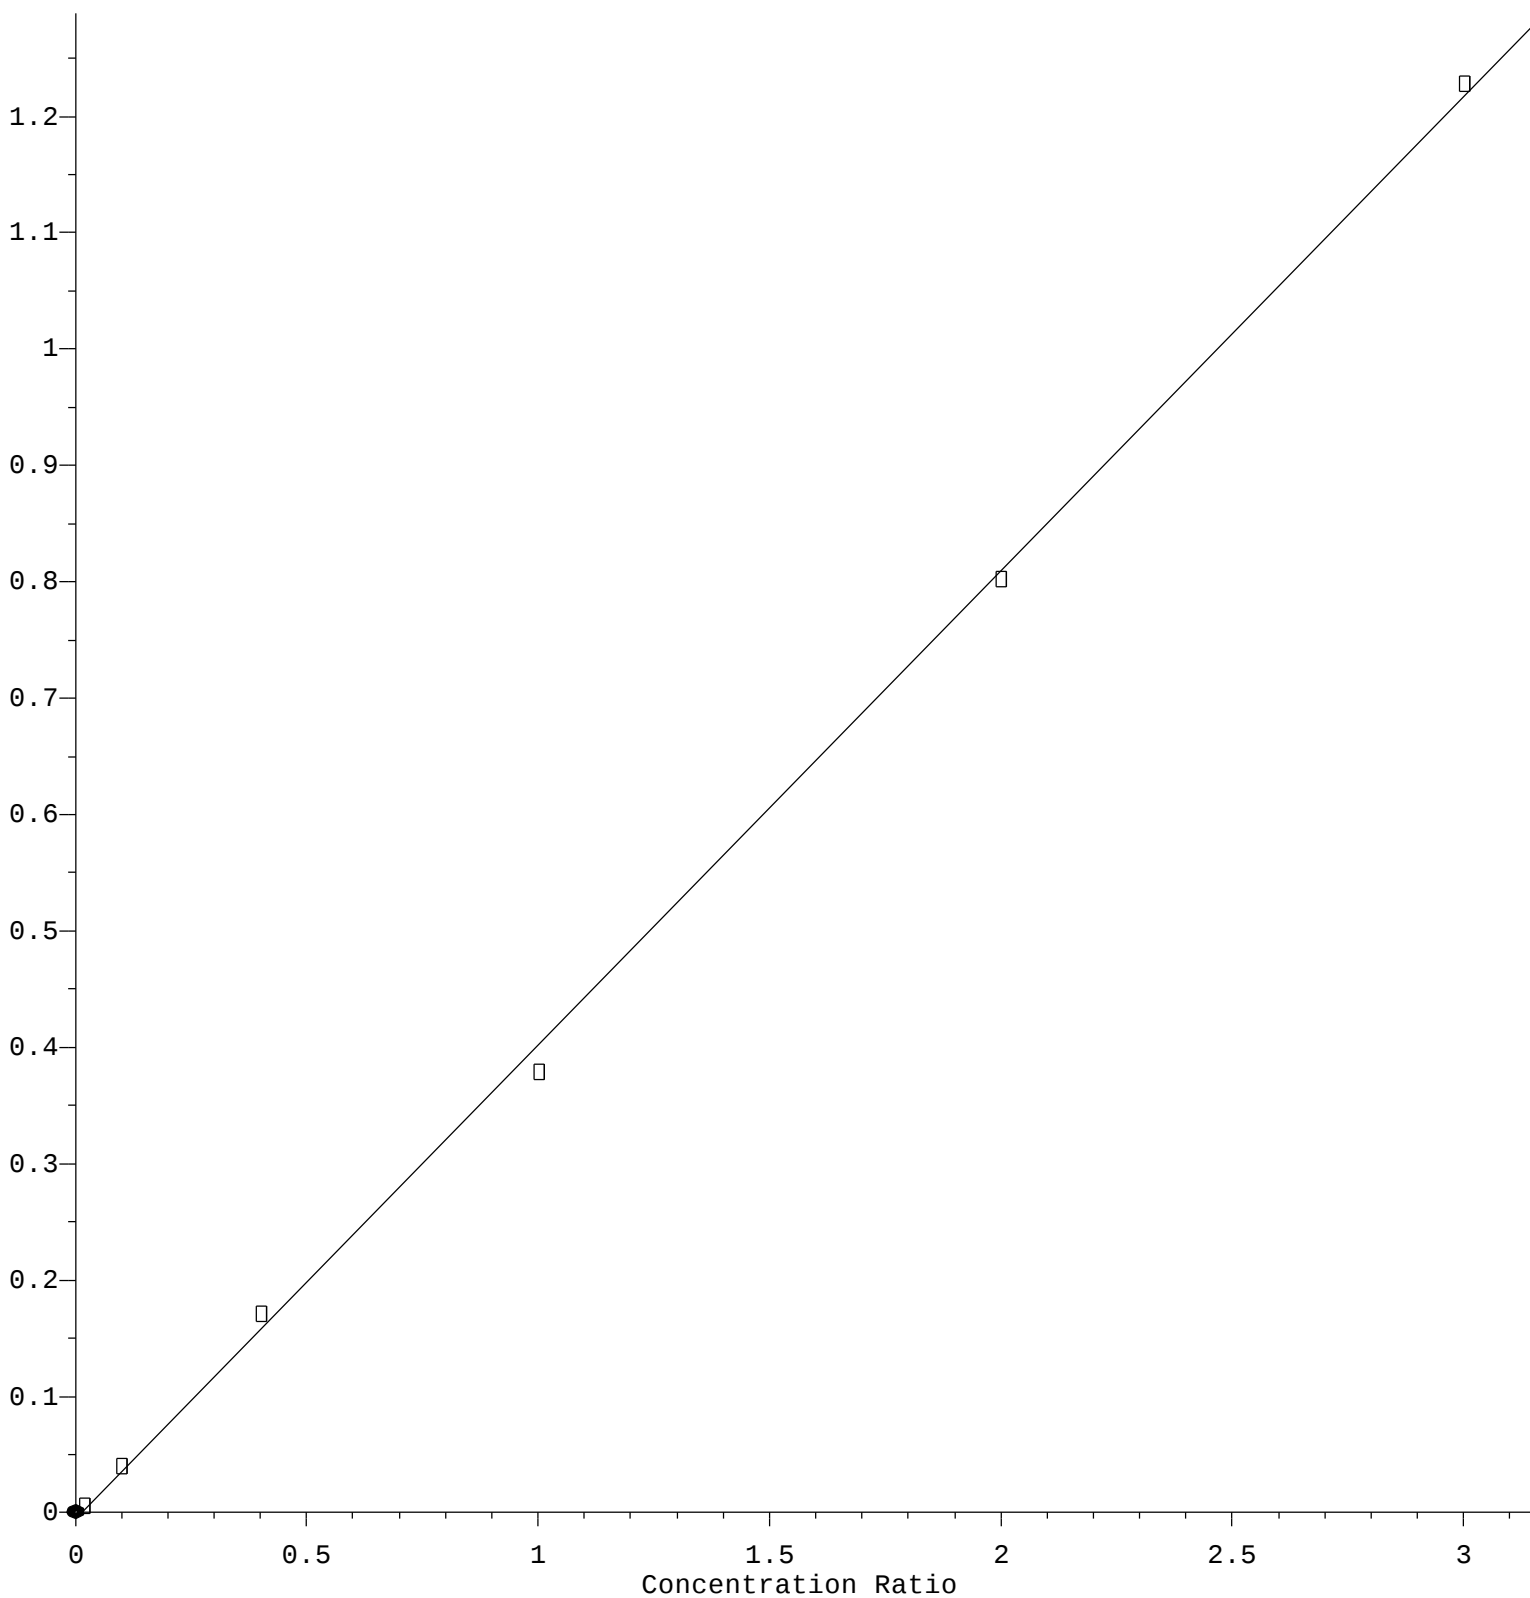

$$\text{Response} = 4.074\text{e-}001 * \text{Amt} - 5.267\text{e-}003$$


Coef of Det (r^2) = 0.999231 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M

Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

Naphthalene


Response Ratio

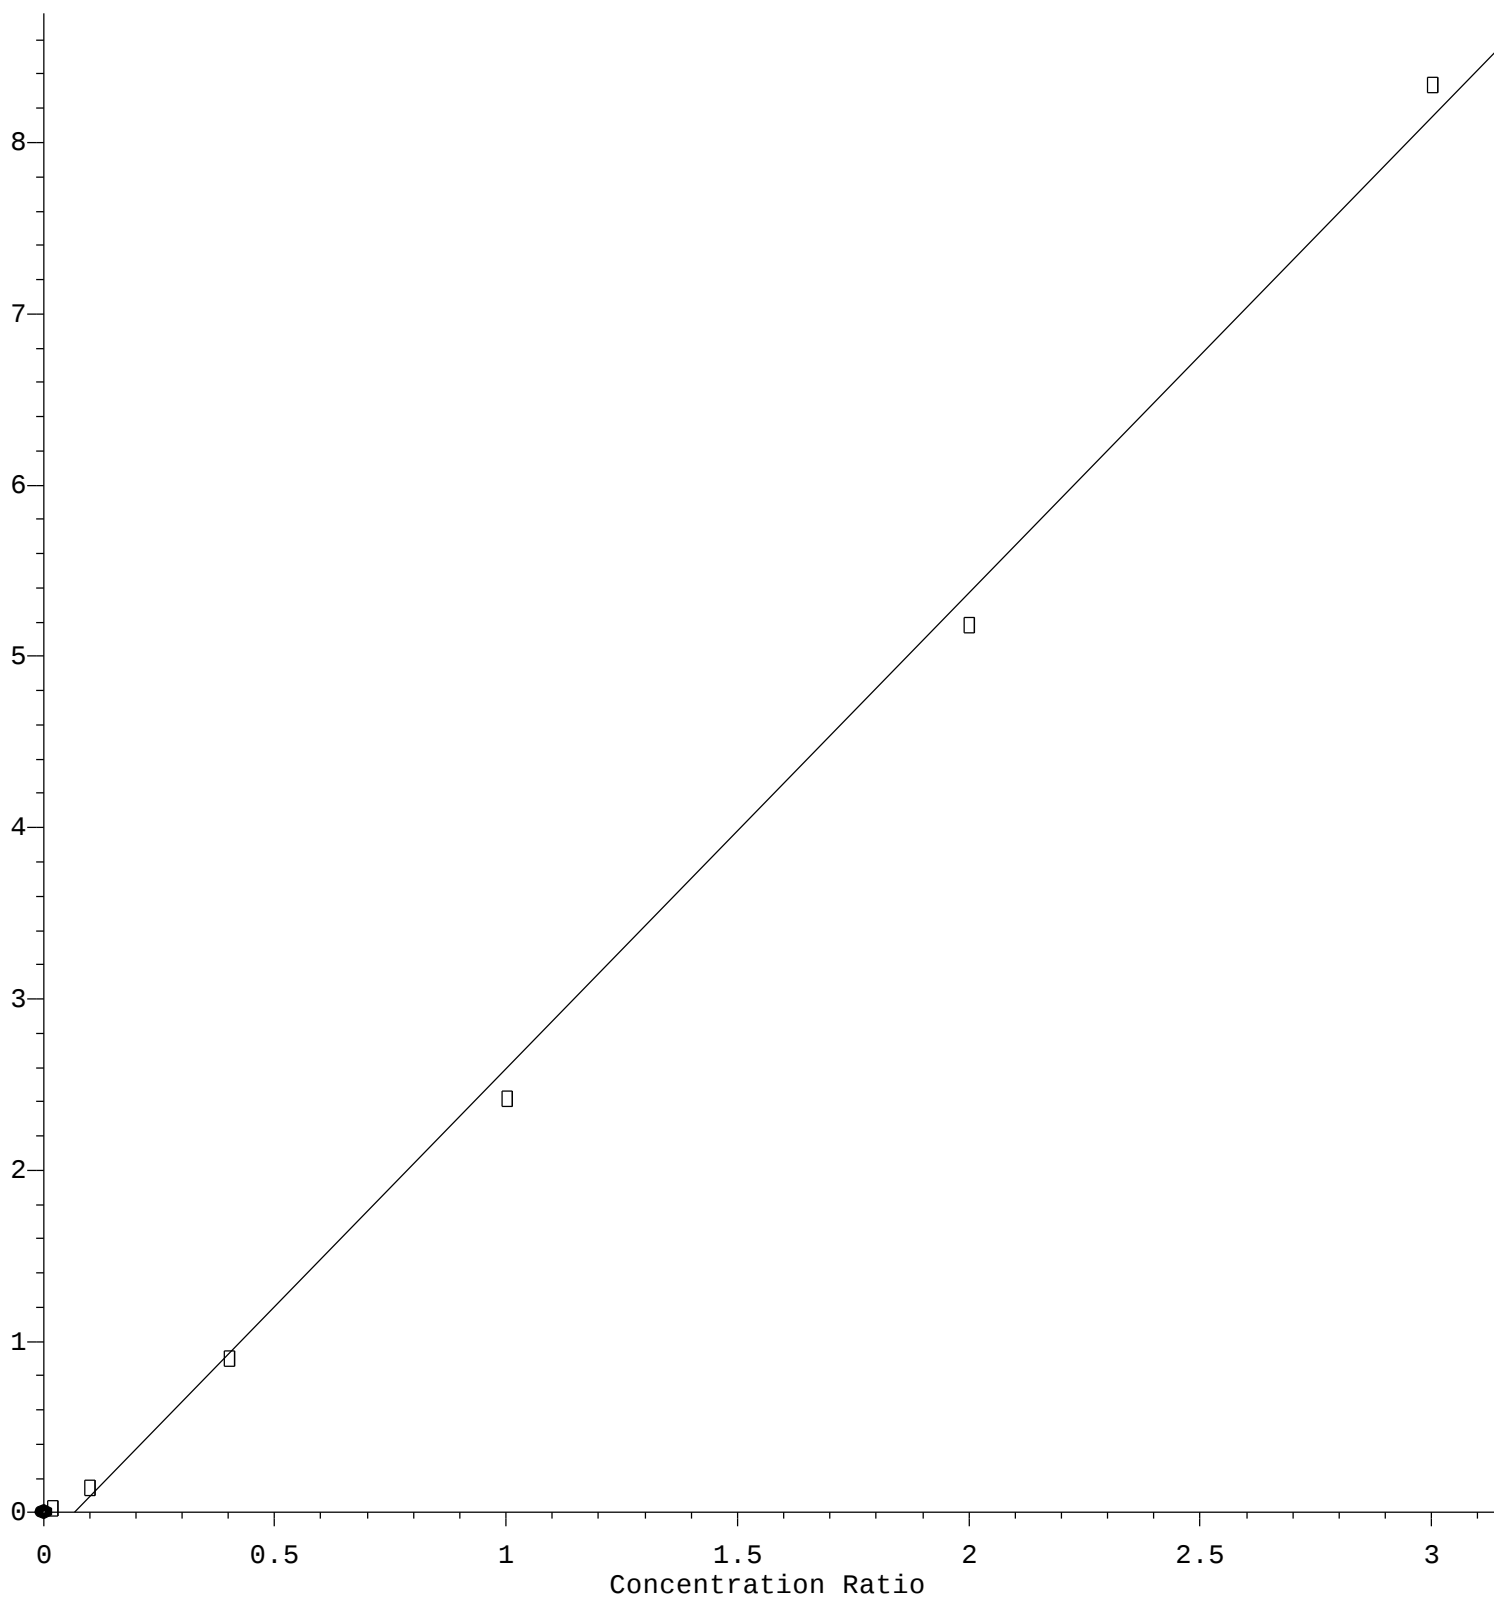

Response = 2.778e+000 * Amt - 1.874e-001
 Coef of Det (r^2) = 0.997608 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

1,2,3-Trichloropropane

Response Ratio

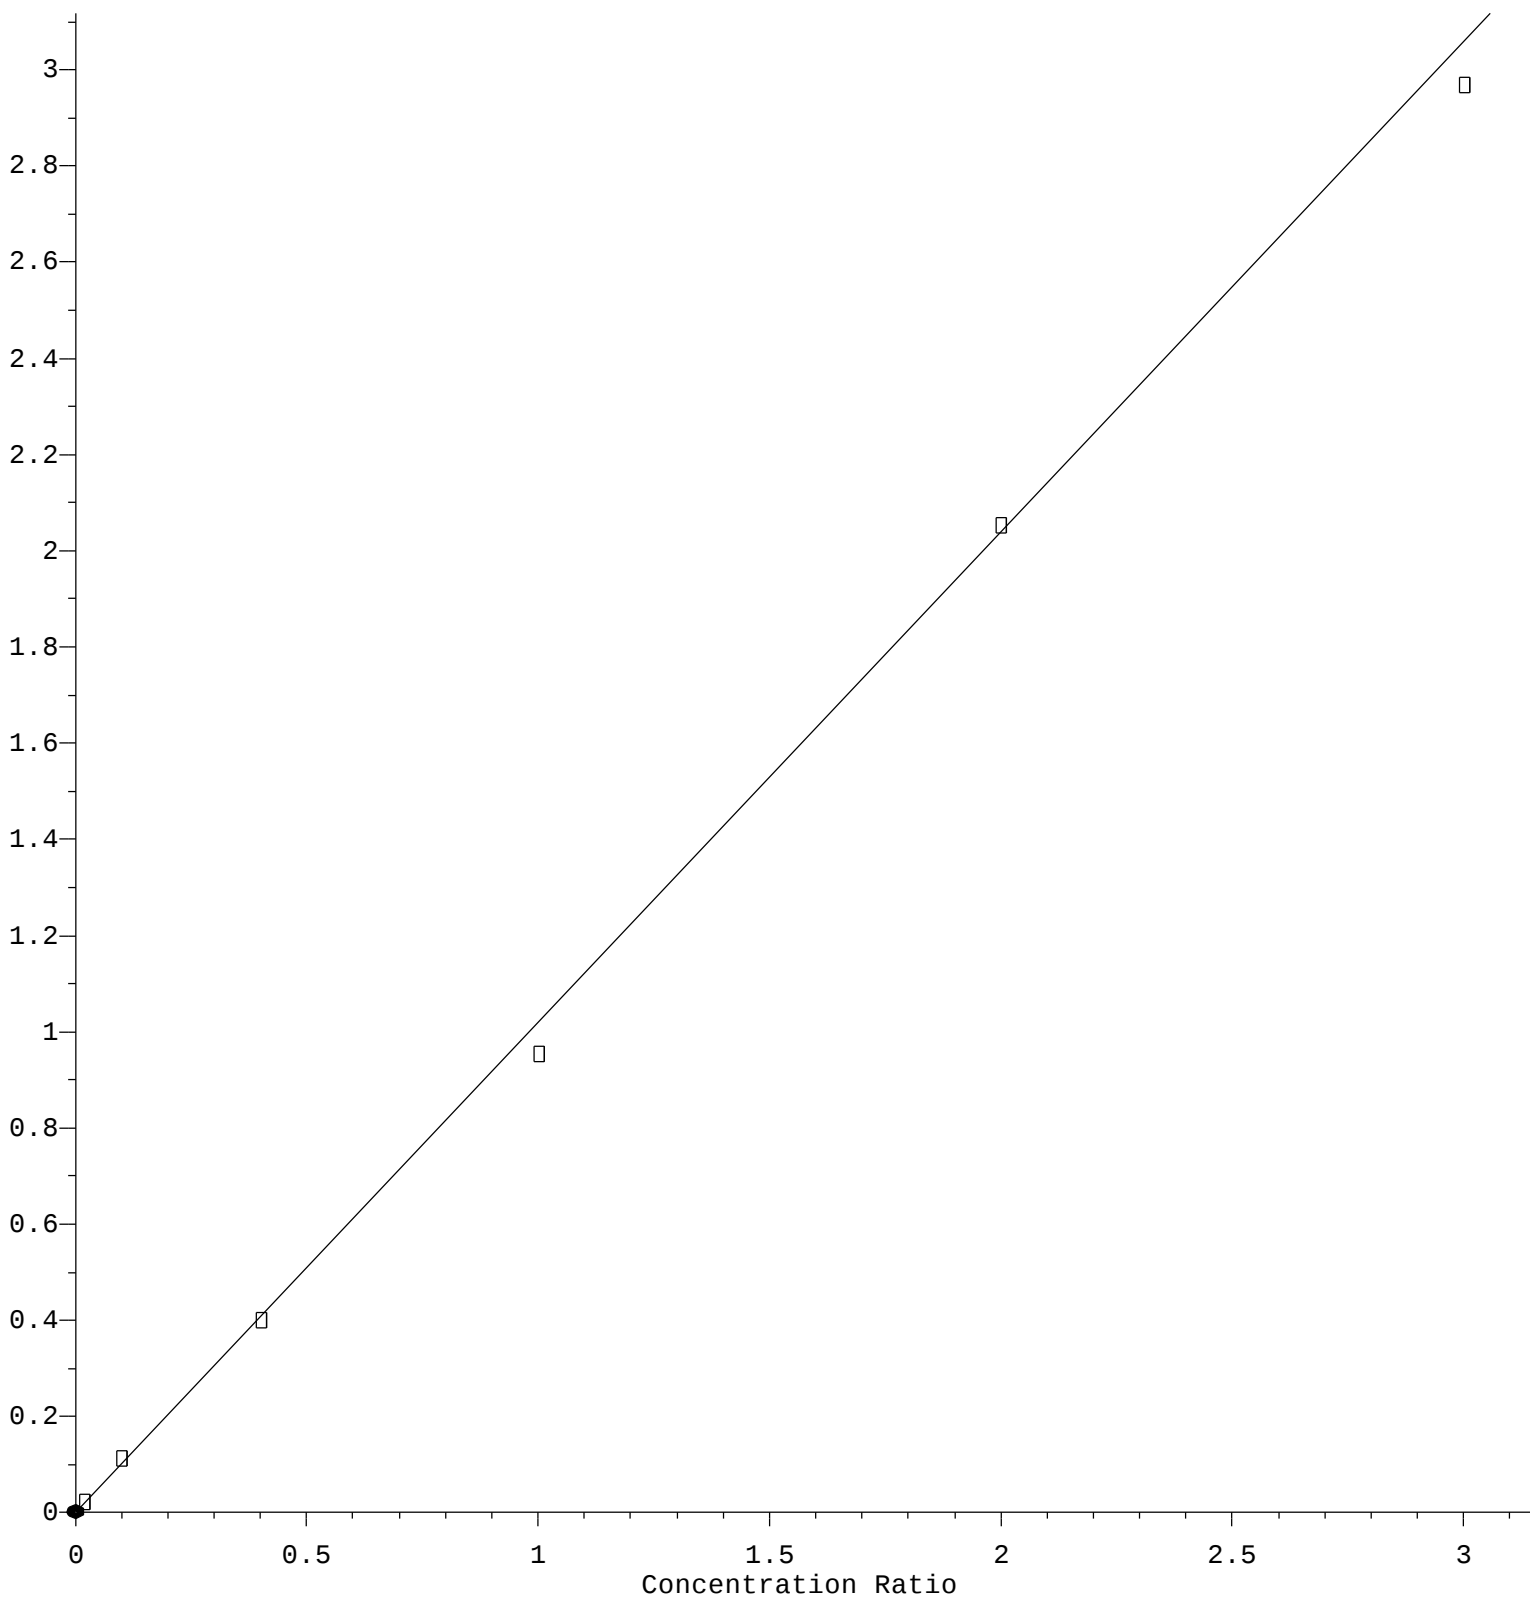

$$\text{Response} = 1.020\text{e}+000 * \text{Amt}$$


RF Rel Std Dev = 5.235% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M

Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

4-Bromofluorobenzene


Response Ratio

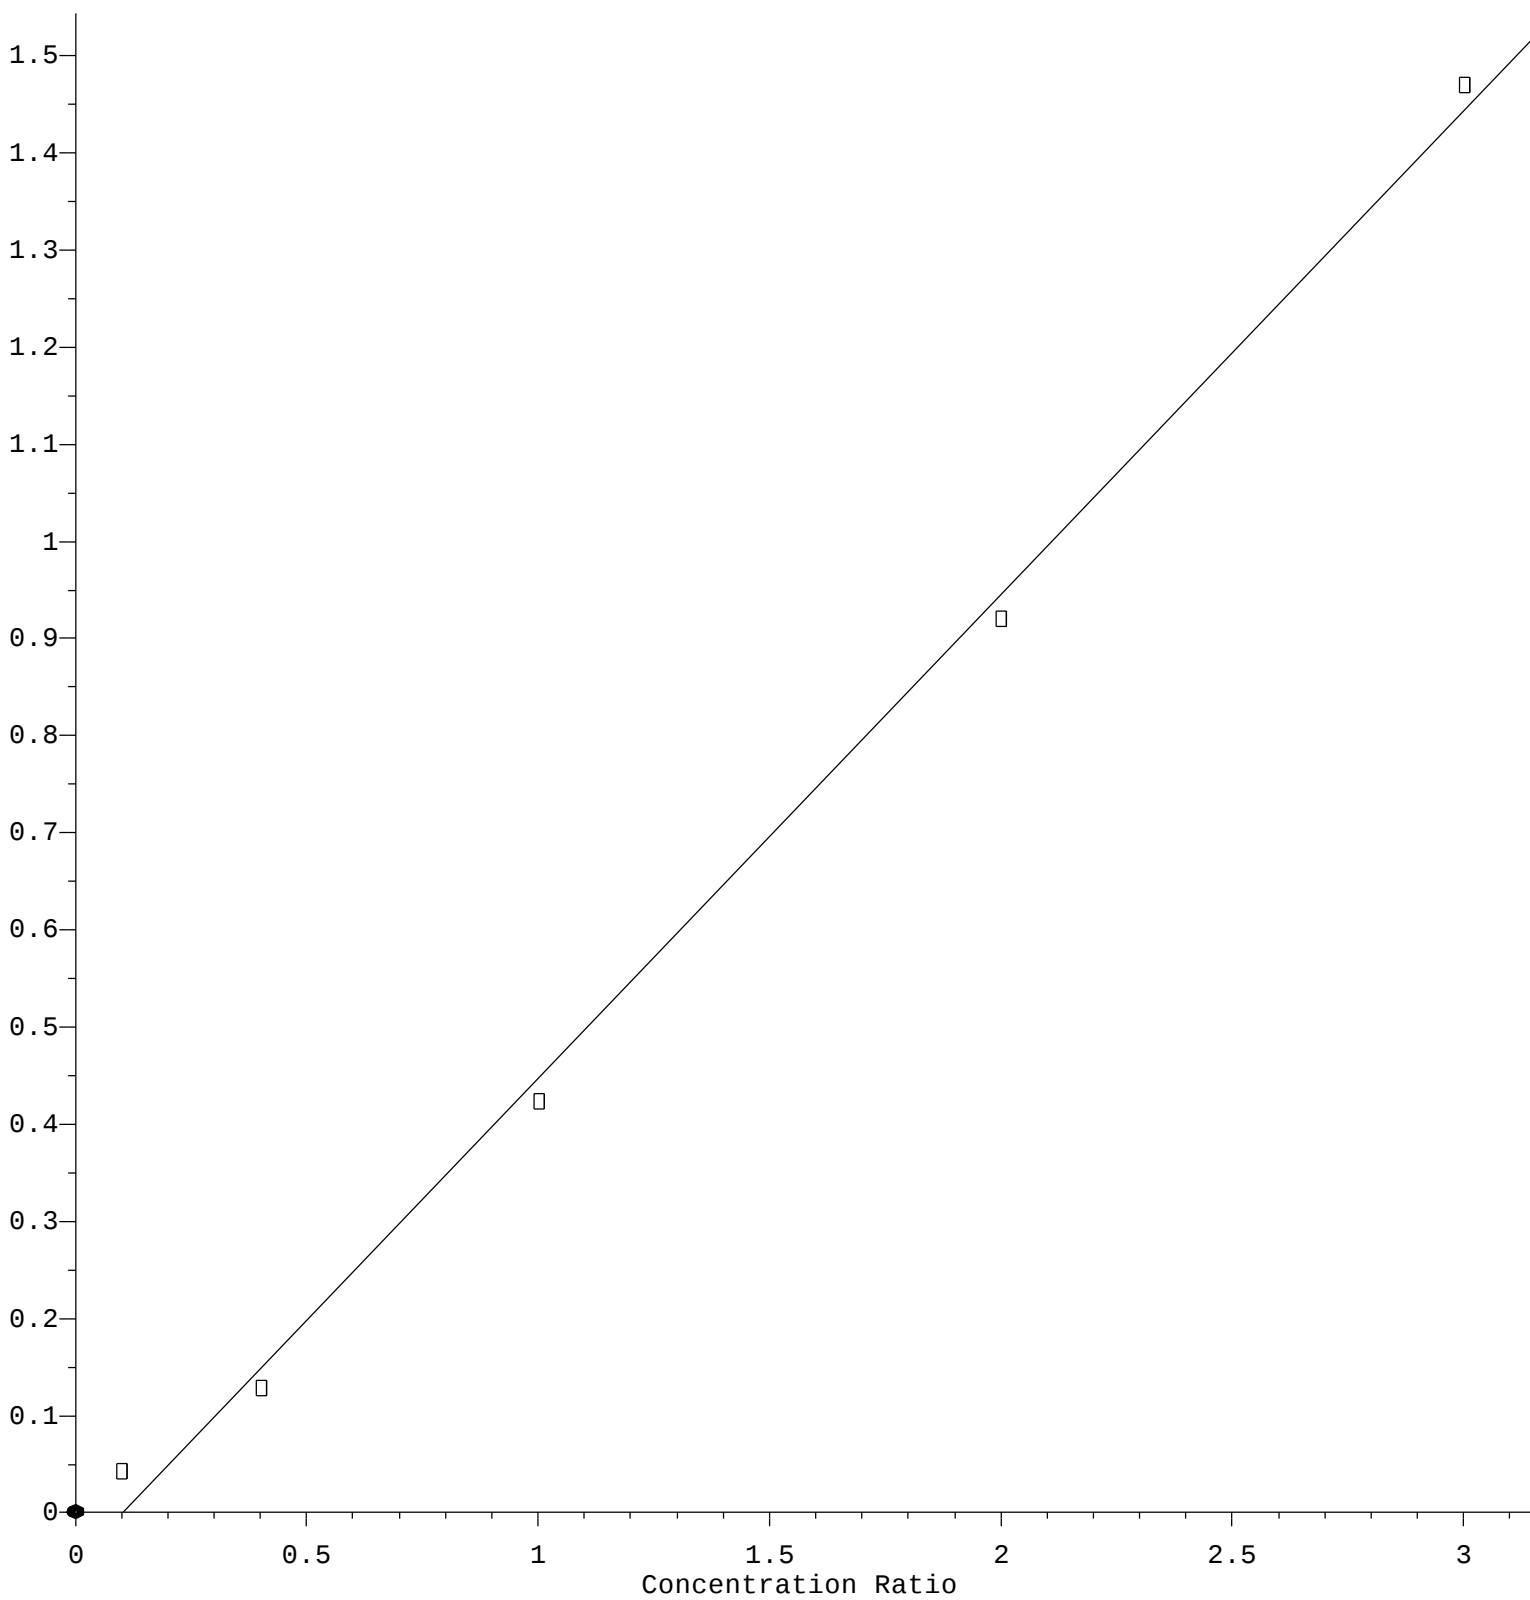

Response = 4.980e-001 * Amt - 5.090e-002
Coef of Det (r^2) = 0.996986 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

1,2,3-Trichlorobenzene

Response Ratio

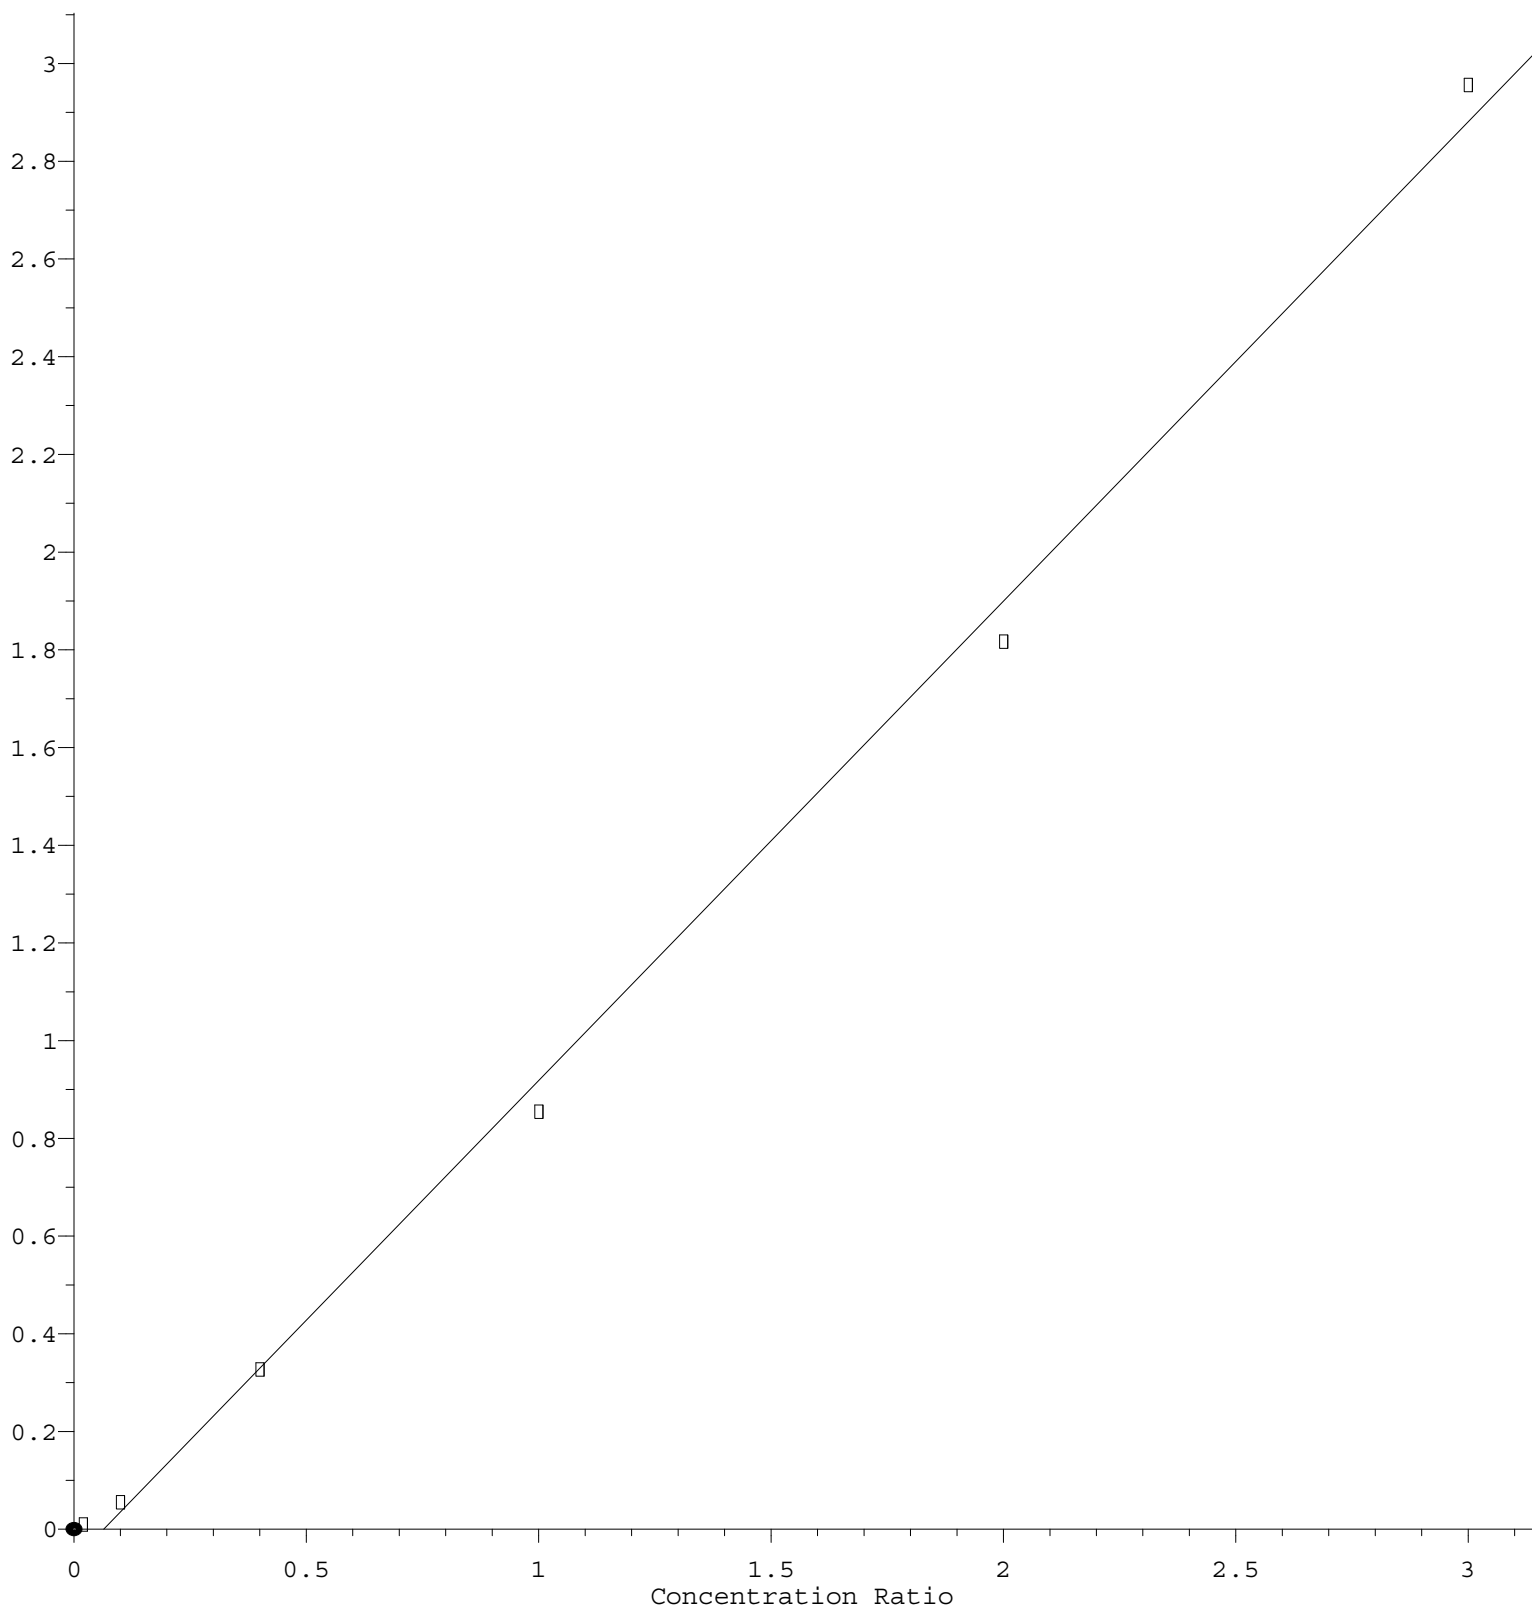

$$\text{Response} = 9.812\text{e-}001 * \text{Amt} - 6.321\text{e-}002$$


Coef of Det (r^2) = 0.997110 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122220W.M

Calibration Table Last Updated: Tue Dec 22 15:42:18 2020

1,2,4-Trichlorobenzene

Response Ratio

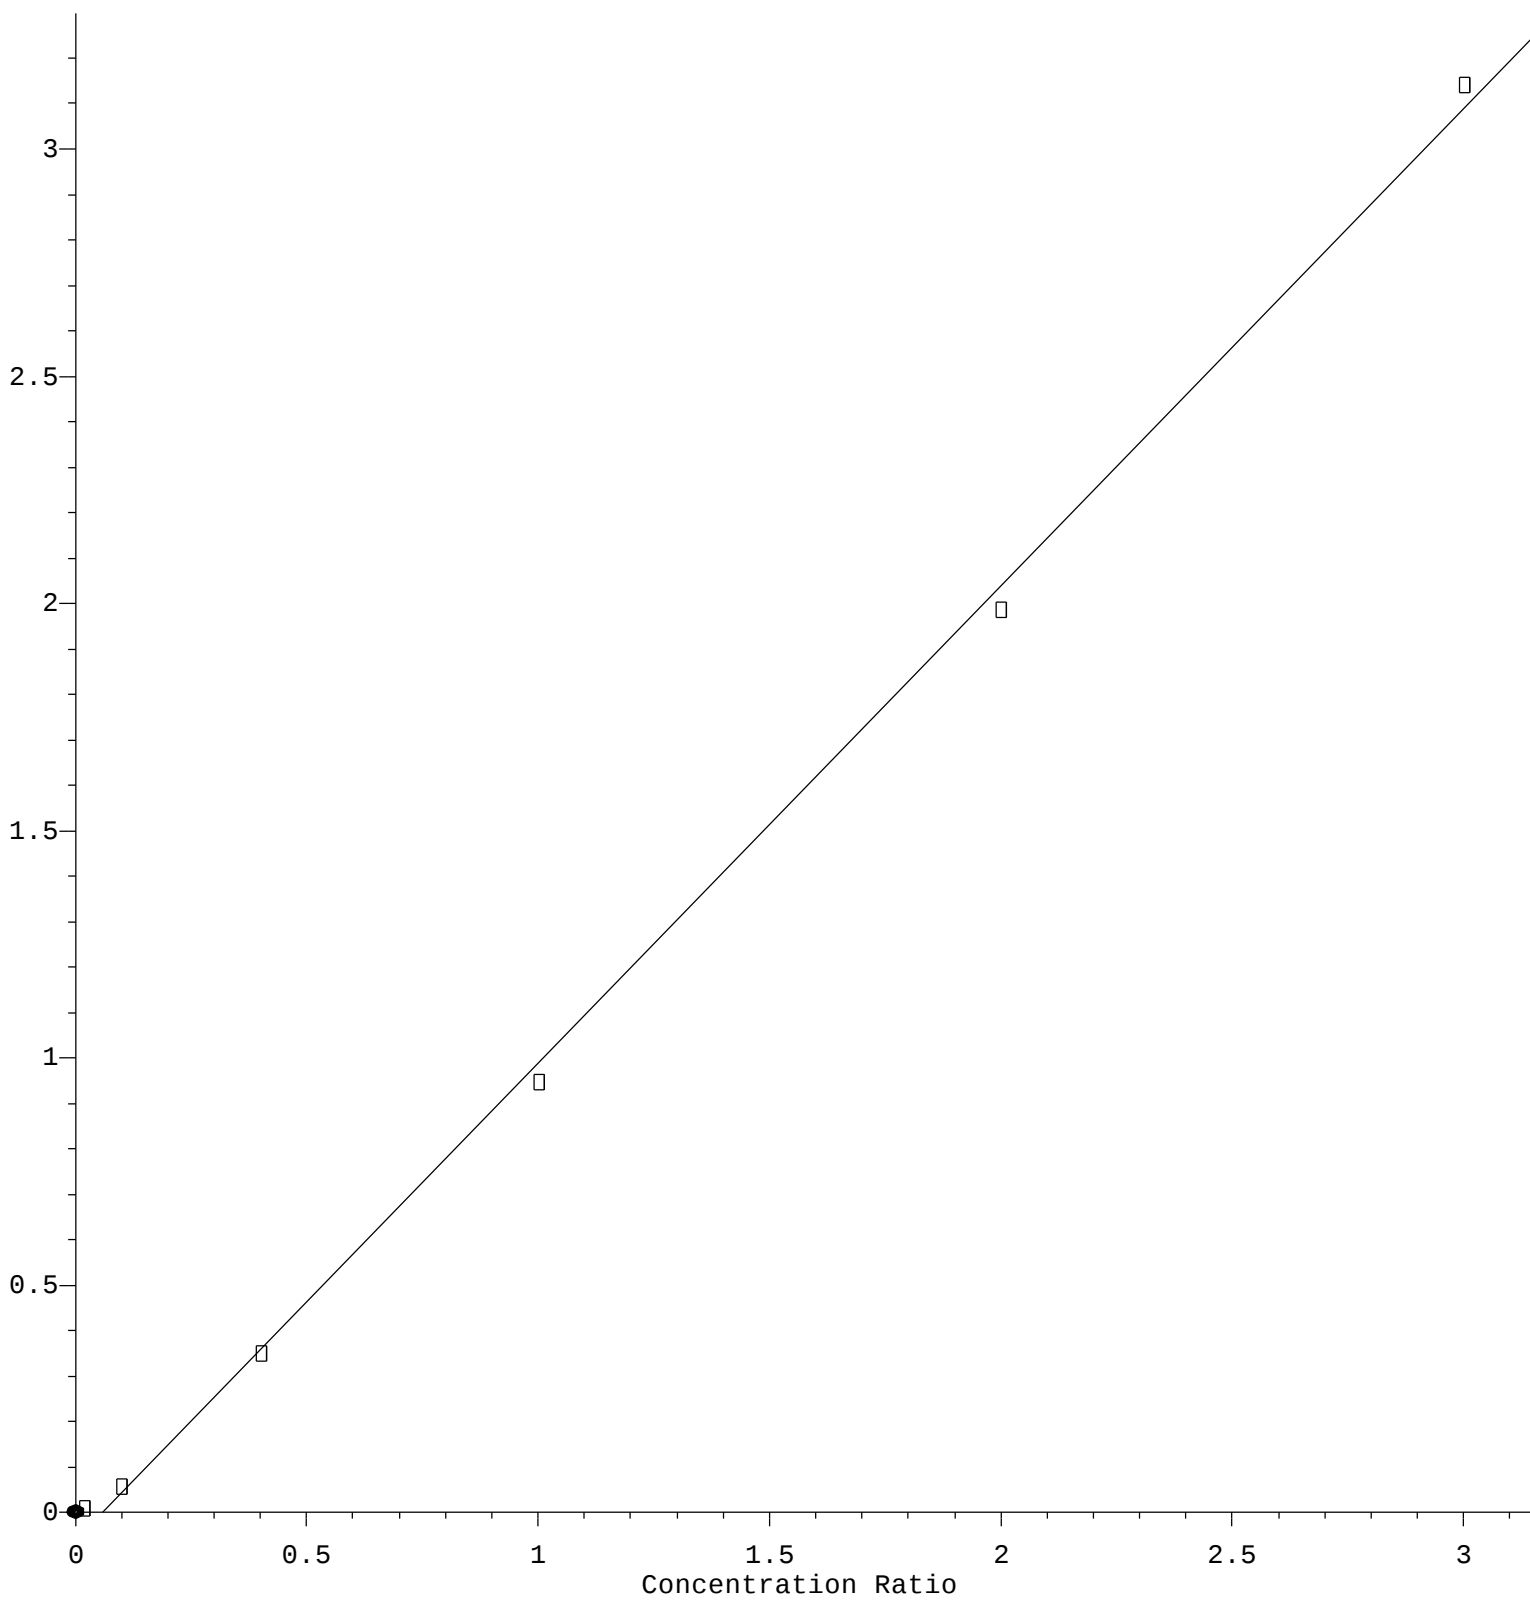

Response = 1.049e+000 * Amt - 5.944e-002
Coef of Det (r^2) = 0.998703 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Calibration Table Last Updated: Tue Dec 22 15:42:18 2020