


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122220\
Data File : VN065191.D
Acq On : 22 Dec 2020 10:58
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Title : Sw846 8260
Last Update : Tue Dec 22 15:42:18 2020

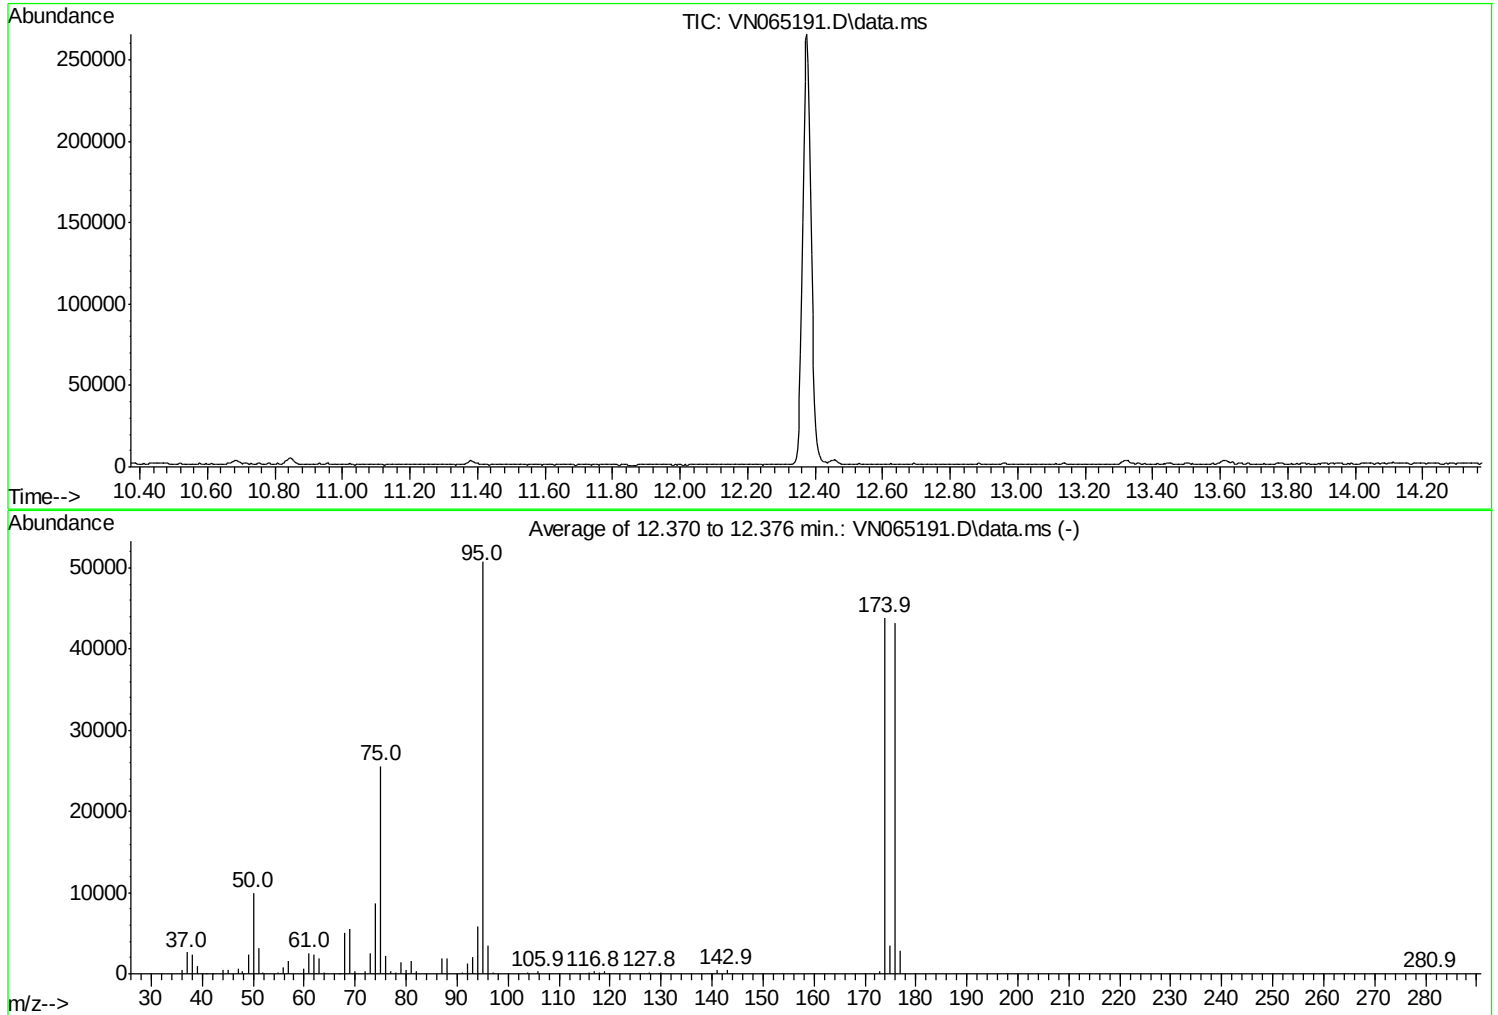

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	9962	PASS
75	95	30	60	50.4	25592	PASS
95	95	100	100	100.0	50776	PASS
96	95	5	9	6.9	3509	PASS
173	174	0.00	2	0.7	323	PASS
174	95	50	100	86.4	43877	PASS
175	174	5	9	7.9	3448	PASS
176	174	95	101	98.7	43296	PASS
177	176	5	9	6.7	2886	PASS