
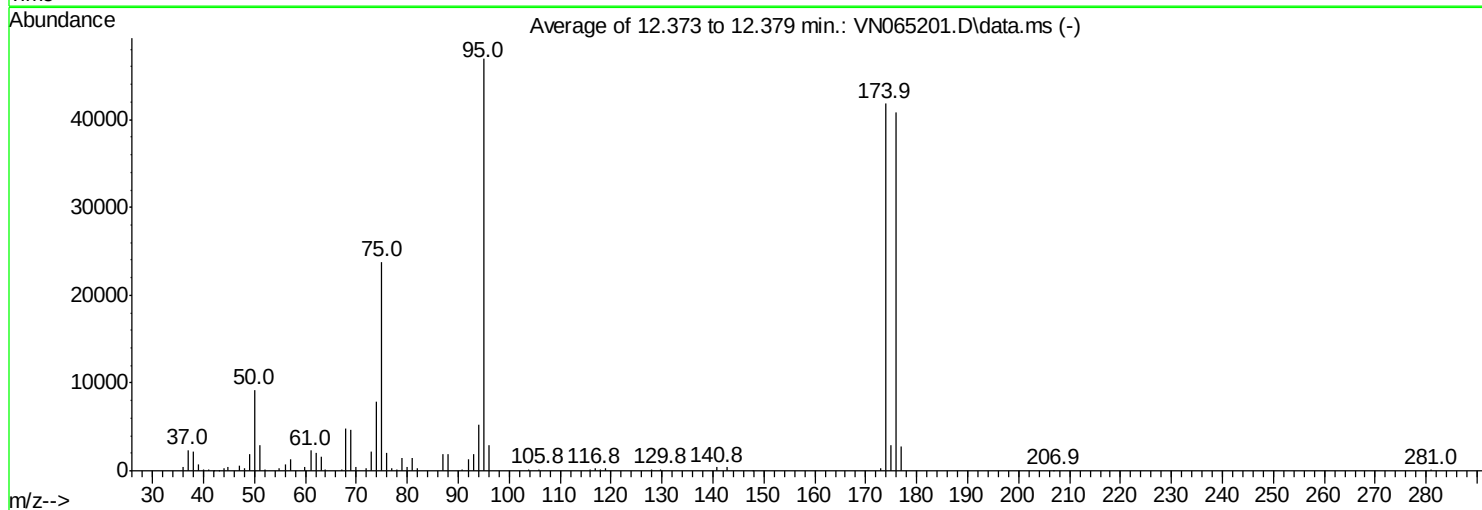


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122220\
 Data File : VN065201.D
 Acq On : 22 Dec 2020 16:37
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Title : SW846 8260
 Last Update : Tue Dec 22 15:42:18 2020

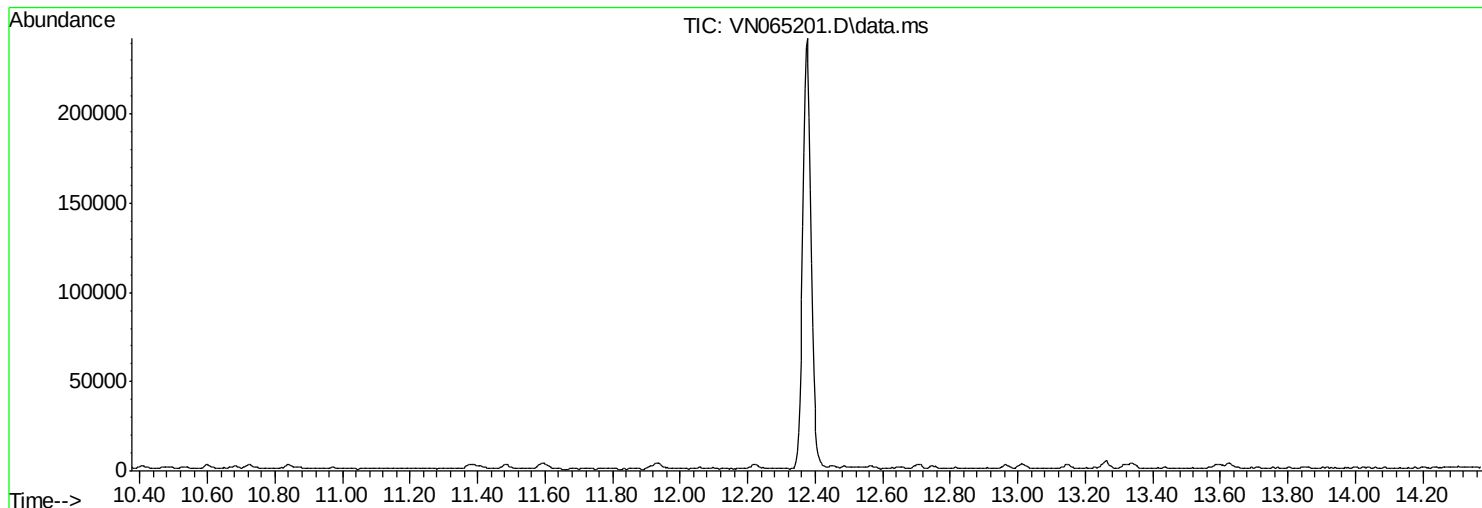

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	9260	PASS
75	95	30	60	50.7	23771	PASS
95	95	100	100	100.0	46925	PASS
96	95	5	9	6.4	2986	PASS
173	174	0.00	2	0.8	337	PASS
174	95	50	100	89.0	41776	PASS
175	174	5	9	7.1	2955	PASS
176	174	95	101	97.7	40803	PASS
177	176	5	9	6.7	2734	PASS